




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027139.D
 Acq On : 01 Aug 2022 20:54
 Operator : SY/MD
 Sample : N3955-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Aug 02 00:37:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 02 00:27:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/02/2022
 Supervised By :Mahesh Dadoda 08/03/2022

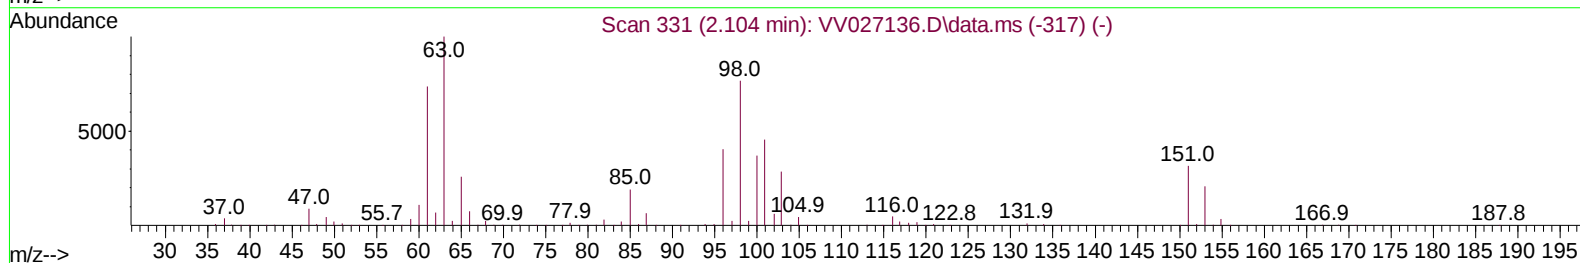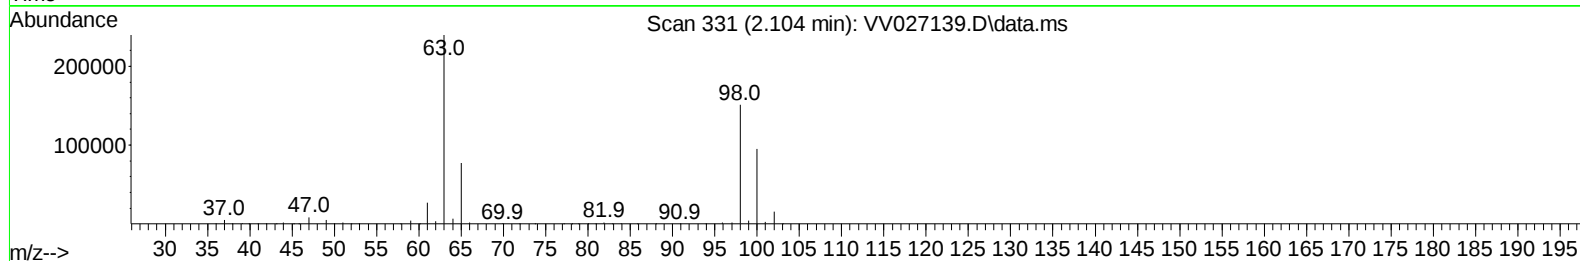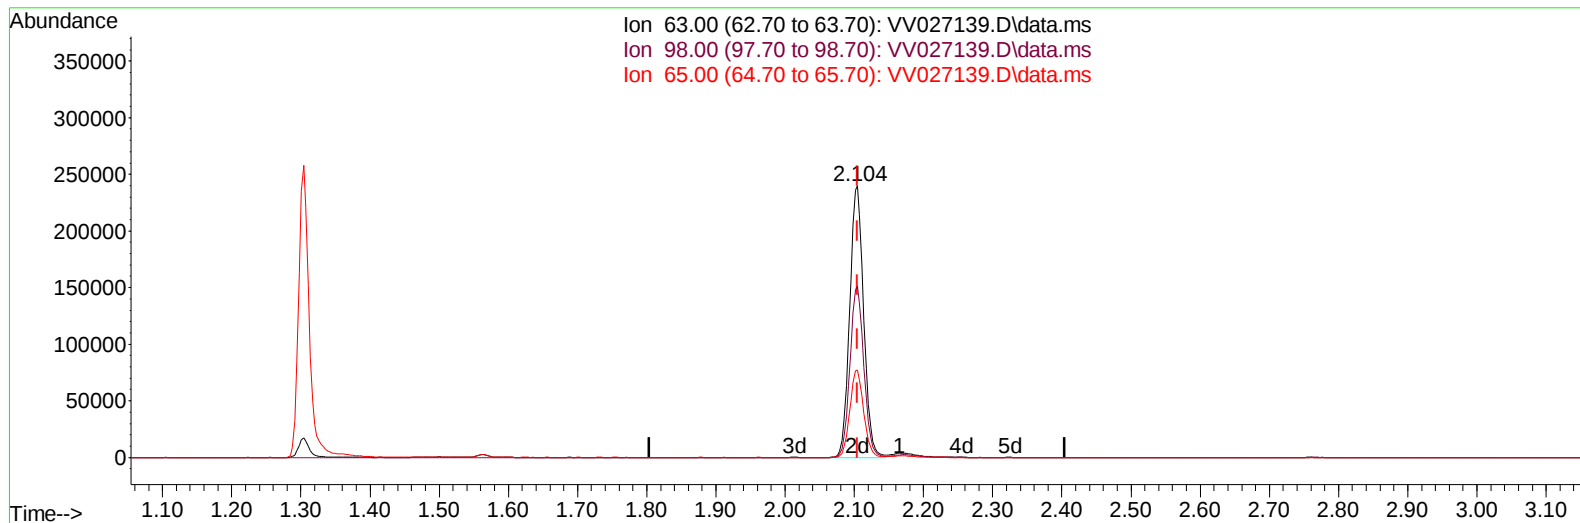

TIC: VV027139.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.104min (+ 0.000) 44.32 ug/L m

response 339147

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	79.90	1.79#
65.00	23.50	0.86#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027139.D
 Acq On : 01 Aug 2022 20:54
 Operator : SY/MD
 Sample : N3955-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Aug 02 00:37:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 02 00:27:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/02/2022
 Supervised By :Mahesh Dadoda 08/03/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	619997	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	595231	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	246855	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	277389	69.035	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	138.060%#	
7) Chloroethane-d5	1.561	69	211106	70.209	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	140.420%#	
11) 1,1-Dichloroethene-d2	2.104	63	339147m	44.325	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	88.640%	
21) 2-Butanone-d5	3.873	46	299455	113.197	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	113.200%	
24) Chloroform-d	4.342	84	438620	54.004	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	108.000%	
26) 1,2-Dichloroethane-d4	5.027	65	267167	57.977	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	115.960%	
32) Benzene-d6	5.047	84	918731	58.330	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	116.660%	
36) 1,2-Dichloropropane-d6	6.066	67	288689	59.250	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	118.500%	
41) Toluene-d8	7.313	98	775919	54.644	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	109.280%	
43) trans-1,3-Dichloroprop...	7.619	79	117802	55.088	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	110.180%	
47) 2-Hexanone-d5	8.088	63	227264	120.817	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	120.820%	
56) 1,1,2,2-Tetrachloroeth...	10.213	84	393531	54.032	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	108.060%	
66) 1,2-Dichlorobenzene-d4	11.622	152	272326	62.772	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	125.540%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027139.D
Acq On : 01 Aug 2022 20:54
Operator : SY/MD
Sample : N3955-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Aug 02 00:37:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122\WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 02 00:27:15 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/02/2022
Supervised By :Mahesh Dadoda 08/03/2022

