




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027166.D
 Acq On : 02 Aug 2022 12:36
 Operator : SY/MD
 Sample : N4008-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ZE7

Manual IntegrationsAPPROVED

Quant Time: Aug 03 01:16:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 02 04:33:39 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/03/2022
 Supervised By :Mahesh Dadoda 08/03/2022

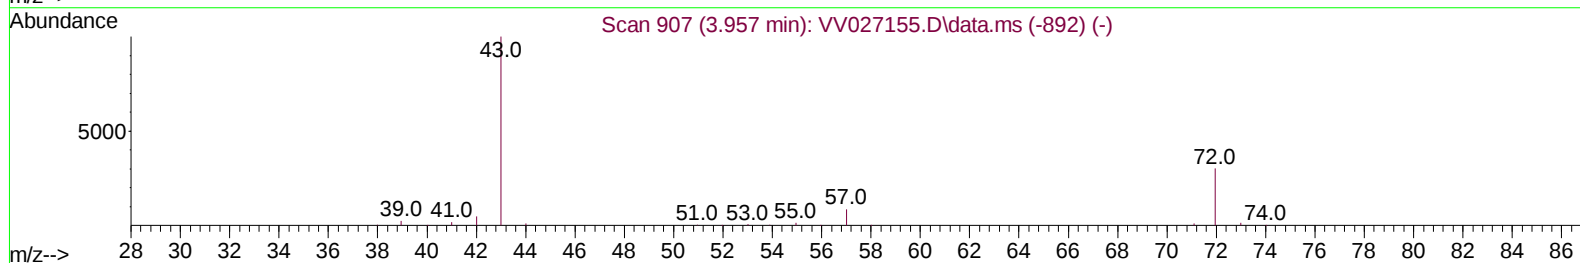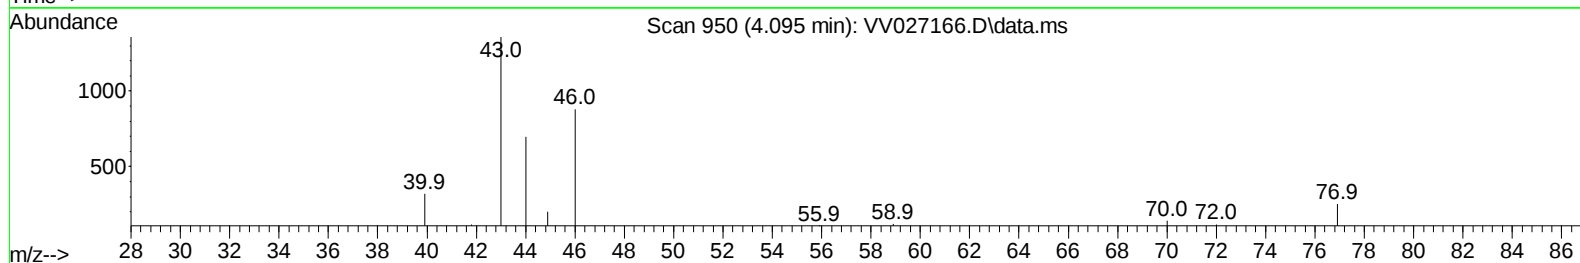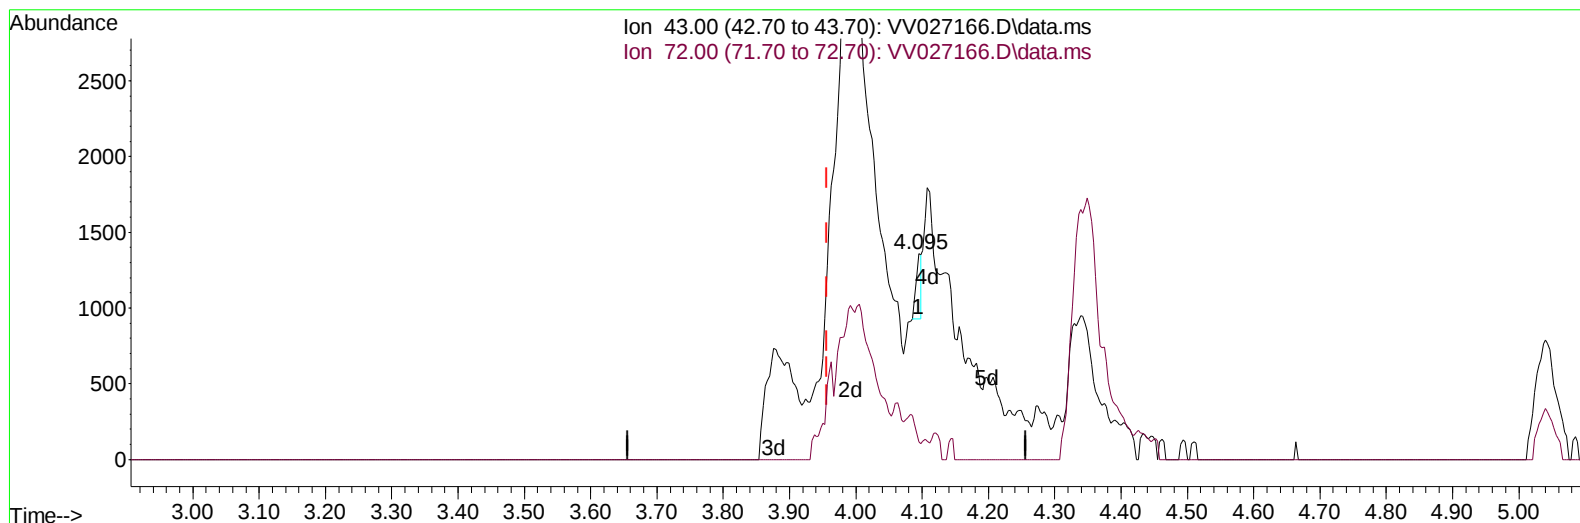

TIC: VV027166.D\data.ms

(22) 2-Butanone (T)

4.095min (+ 0.138) 0.08 ug/L

response 246

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	31.40	31.71
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027166.D
 Acq On : 02 Aug 2022 12:36
 Operator : SY/MD
 Sample : N4008-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ZE7

Manual IntegrationsAPPROVED

Quant Time: Aug 03 01:16:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 02 04:33:39 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/03/2022
 Supervised By :Mahesh Dadoda 08/03/2022

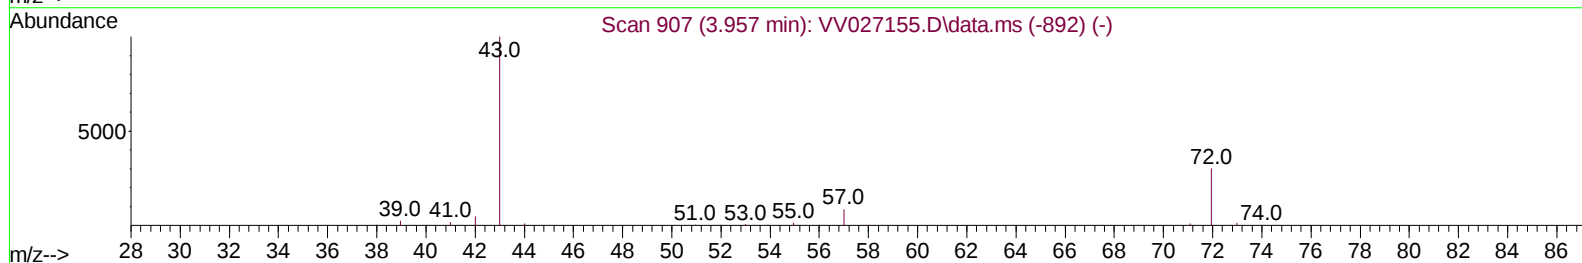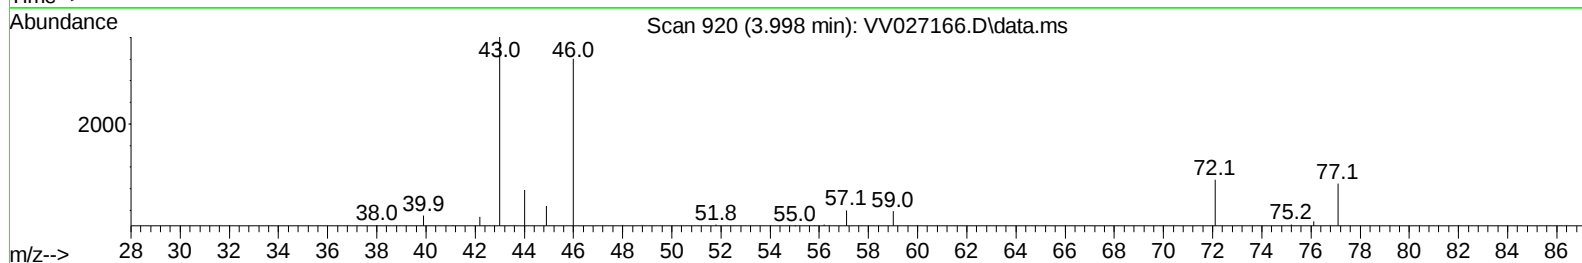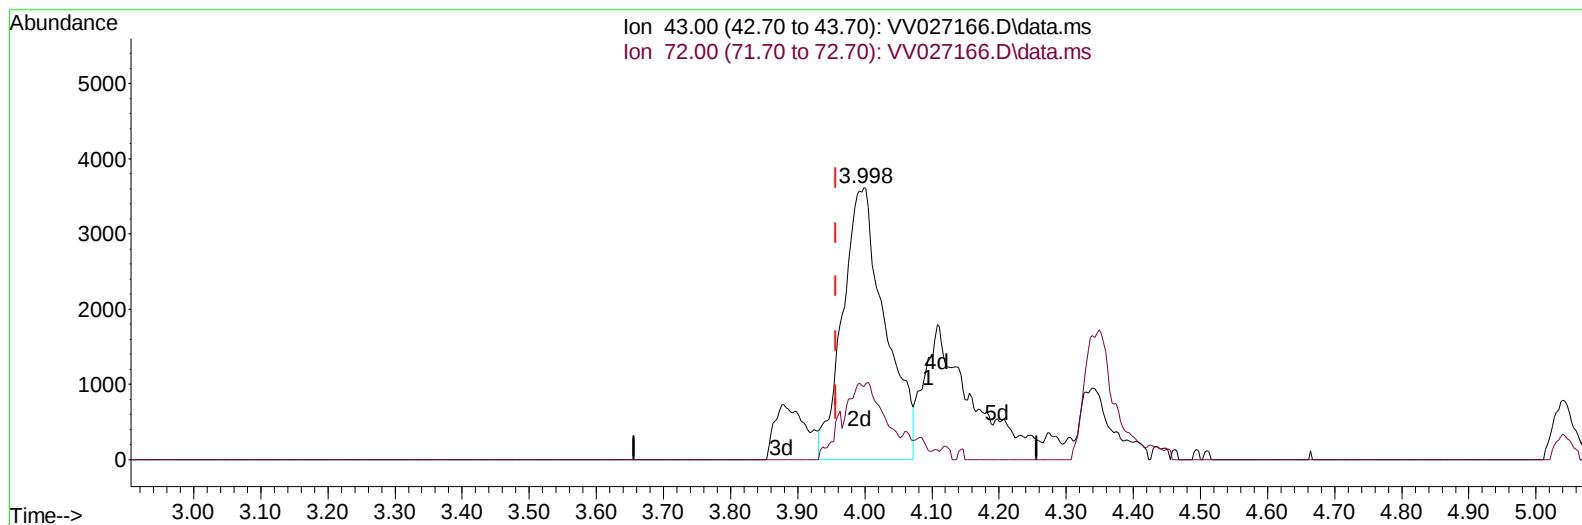

TIC: VV027166.D\data.ms

(22) 2-Butanone (T)

3.998min (+ 0.042) 5.04 ug/L m

response 15702

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	31.40	0.50#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027166.D
 Acq On : 02 Aug 2022 12:36
 Operator : SY/MD
 Sample : N4008-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ZE7

Manual IntegrationsAPPROVED

Quant Time: Aug 03 01:16:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 02 04:33:39 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/03/2022
 Supervised By :Mahesh Dadoda 08/03/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	627558	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	616182	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	265420	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	224966	55.313	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	110.620%	
7) Chloroethane-d5	1.561	69	172622	56.719	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	113.440%	
11) 1,1-Dichloroethene-d2	2.101	63	290176	37.468	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	74.940%	
21) 2-Butanone-d5	3.876	46	282834	105.626	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	105.630%	
24) Chloroform-d	4.339	84	403531	49.085	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	98.180%	
26) 1,2-Dichloroethane-d4	5.024	65	240023	51.459	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	102.920%	
32) Benzene-d6	5.043	84	803962	49.308	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	98.620%	
36) 1,2-Dichloropropane-d6	6.066	67	256758	50.905	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	101.800%	
41) Toluene-d8	7.313	98	666497	45.342	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	90.680%	
43) trans-1,3-Dichloroprop...	7.619	79	107264	48.455	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	96.900%	
47) 2-Hexanone-d5	8.088	63	208819	107.237	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	107.240%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	369758	49.042	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	98.080%	
66) 1,2-Dichlorobenzene-d4	11.622	152	265517	56.921	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	113.840%	
Target Compounds						Qvalue
22) 2-Butanone	3.998	43	15702m	5.039	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027166.D
Acq On : 02 Aug 2022 12:36
Operator : SY/MD
Sample : N4008-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ZE7

Manual IntegrationsAPPROVED

Quant Time: Aug 03 01:16:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 02 04:33:39 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/03/2022
Supervised By :Mahesh Dadoda 08/03/2022

