

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027173.D
 Acq On : 02 Aug 2022 16:08
 Operator : SY/MD
 Sample : N4003-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E50

Quant Time: Aug 03 02:01:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 03 02:00:39 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	565742	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	554165	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	243989	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	205266	55.984	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 111.960%		
7) Chloroethane-d5	1.561	69	153493	55.944	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 111.880%		
11) 1,1-Dichloroethene-d2	2.102	63	262728	37.630	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 75.260%		
21) 2-Butanone-d5	3.876	46	257494	106.670	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 106.670%		
24) Chloroform-d	4.343	84	365032	49.254	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 98.500%		
26) 1,2-Dichloroethane-d4	5.027	65	228189	54.267	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 108.540%		
32) Benzene-d6	5.047	84	743084	50.674	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 101.340%		
36) 1,2-Dichloropropane-d6	6.066	67	240130	52.936	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 105.880%		
41) Toluene-d8	7.314	98	605256	45.784	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 91.560%		
43) trans-1,3-Dichloroprop...	7.619	79	98004	49.226	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 98.460%		
47) 2-Hexanone-d5	8.088	63	208514	119.064	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 119.060%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	356663	52.599	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 105.200%		
66) 1,2-Dichlorobenzene-d4	11.622	152	250667	58.458	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 116.920%		
Target Compounds						
13) Acetone	2.169	43	4971	2.439	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027173.D
Acq On : 02 Aug 2022 16:08
Operator : SY/MD
Sample : N4003-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E50

Quant Time: Aug 03 02:01:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 03 02:00:39 2022
Response via : Initial Calibration

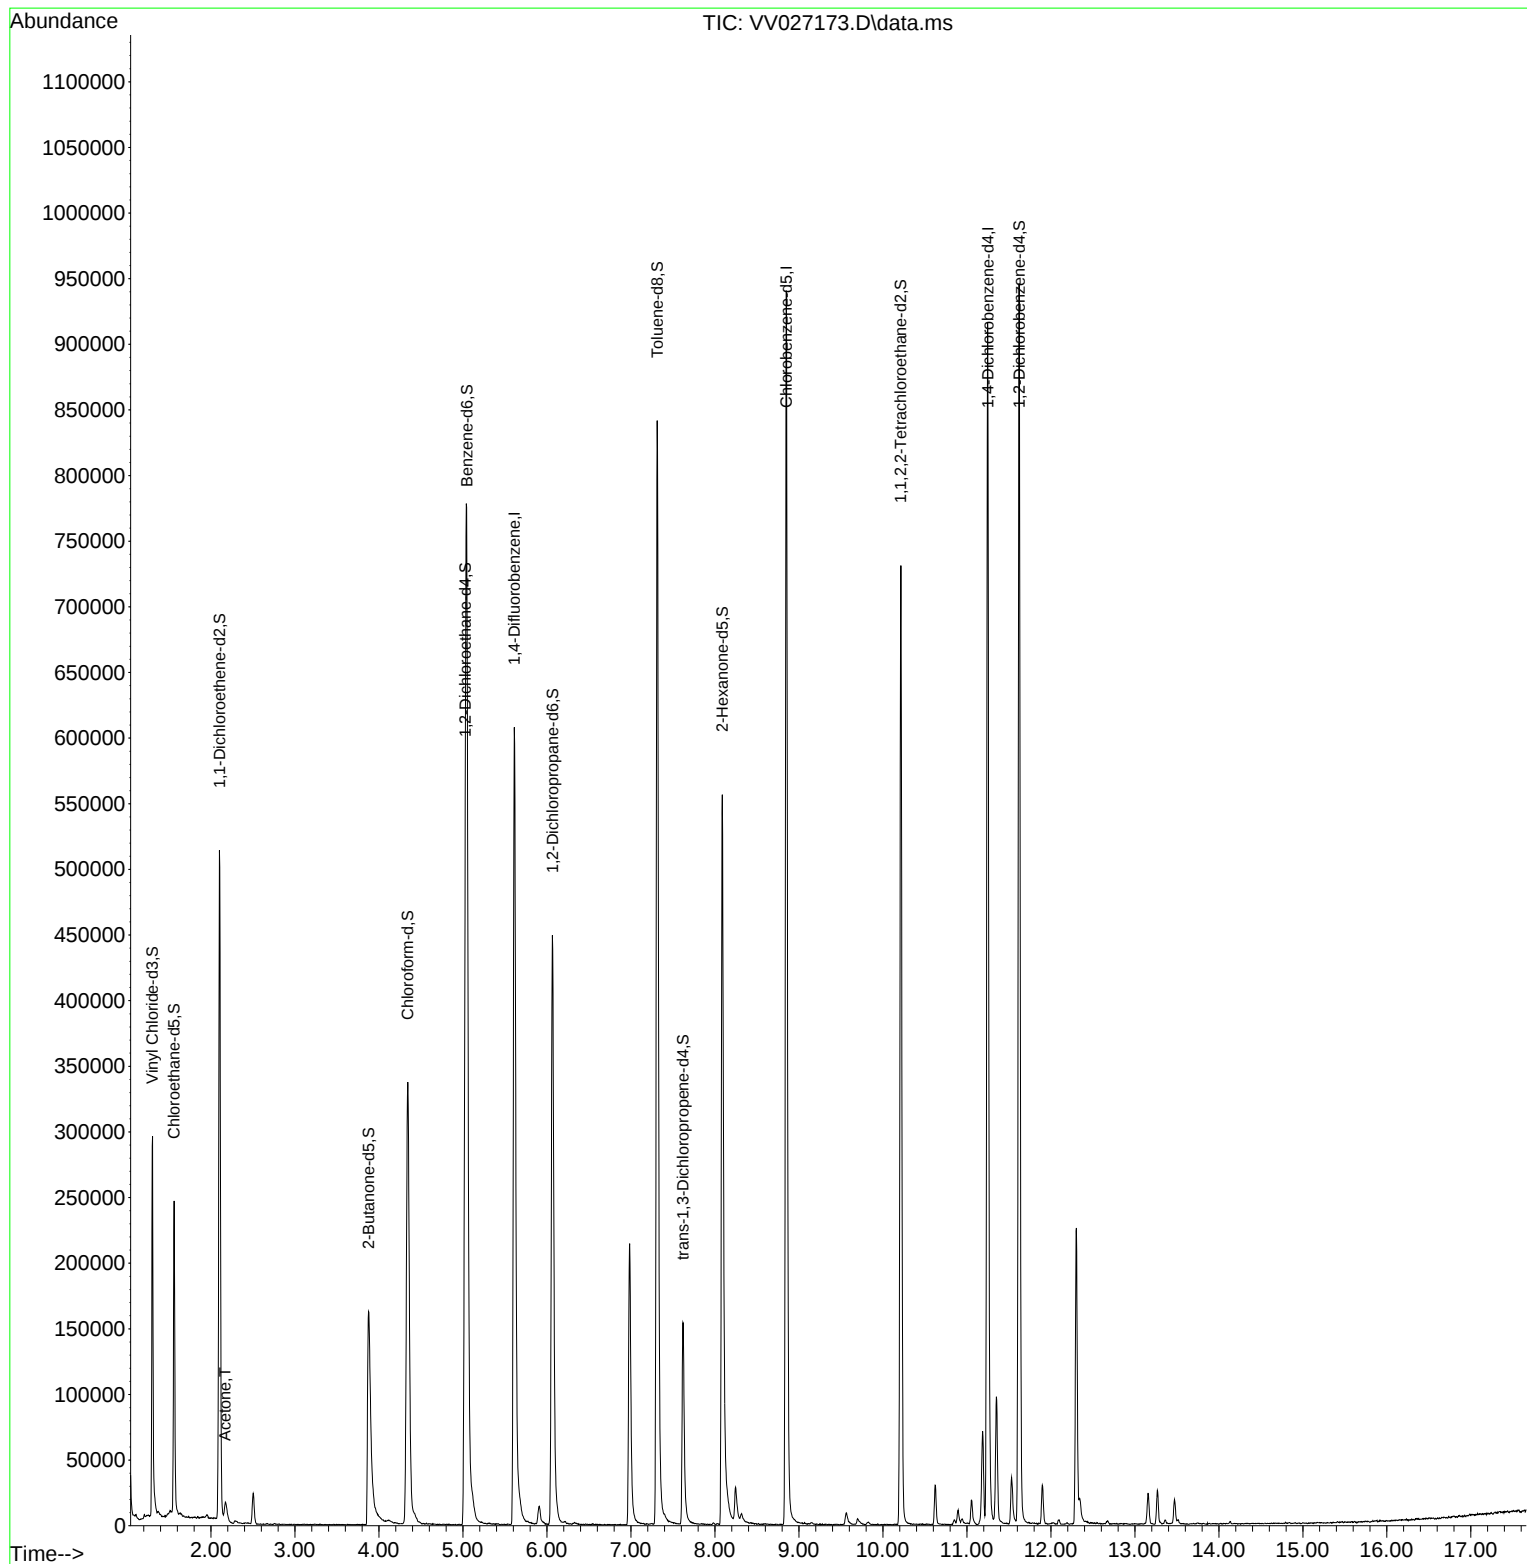

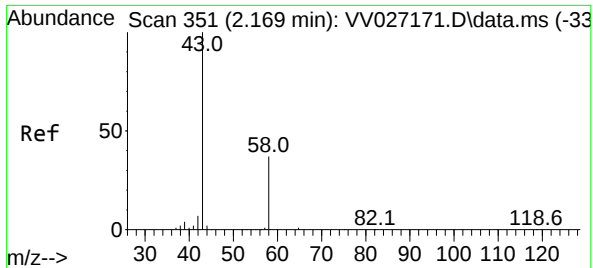

#13
 Acetone
 Concen: 2.439 ug/L
 RT: 2.169 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: VV027173.D
 Acq: 02 Aug 2022 16:08

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E50

Tgt Ion: 43 Resp: 4971
 Ion Ratio Lower Upper
 43 100
 58 34.3 0.0 73.6

