

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027184.D
 Acq On : 02 Aug 2022 20:38
 Operator : SY/MD
 Sample : VIBLK269
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK269

Quant Time: Aug 03 02:04:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 03 02:00:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	619463	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	593956	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	249273	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	196113	48.849	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	97.700%
7) Chloroethane-d5	1.561	69	161828	53.867	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	107.740%
11) 1,1-Dichloroethene-d2	2.101	63	251574	32.908	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.820%
21) 2-Butanone-d5	3.873	46	266745	100.919	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.920%
24) Chloroform-d	4.342	84	373768	46.059	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.120%
26) 1,2-Dichloroethane-d4	5.027	65	226859	49.272	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.540%
32) Benzene-d6	5.047	84	754483	48.005	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.000%
36) 1,2-Dichloropropane-d6	6.066	67	239710	49.303	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.600%
41) Toluene-d8	7.313	98	614832	43.392	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.780%
43) trans-1,3-Dichloroprop...	7.619	79	95343	44.682	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.360%
47) 2-Hexanone-d5	8.088	63	210374	112.078	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	112.080%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	355940	48.975	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.960%
66) 1,2-Dichlorobenzene-d4	11.622	152	239086	54.575	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.160%
Target Compounds						
17) trans-1,2-Dichloroethene	2.757	96	8646	1.891	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027184.D
Acq On : 02 Aug 2022 20:38
Operator : SY/MD
Sample : VIBLK269
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK269

Quant Time: Aug 03 02:04:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 03 02:00:39 2022
Response via : Initial Calibration

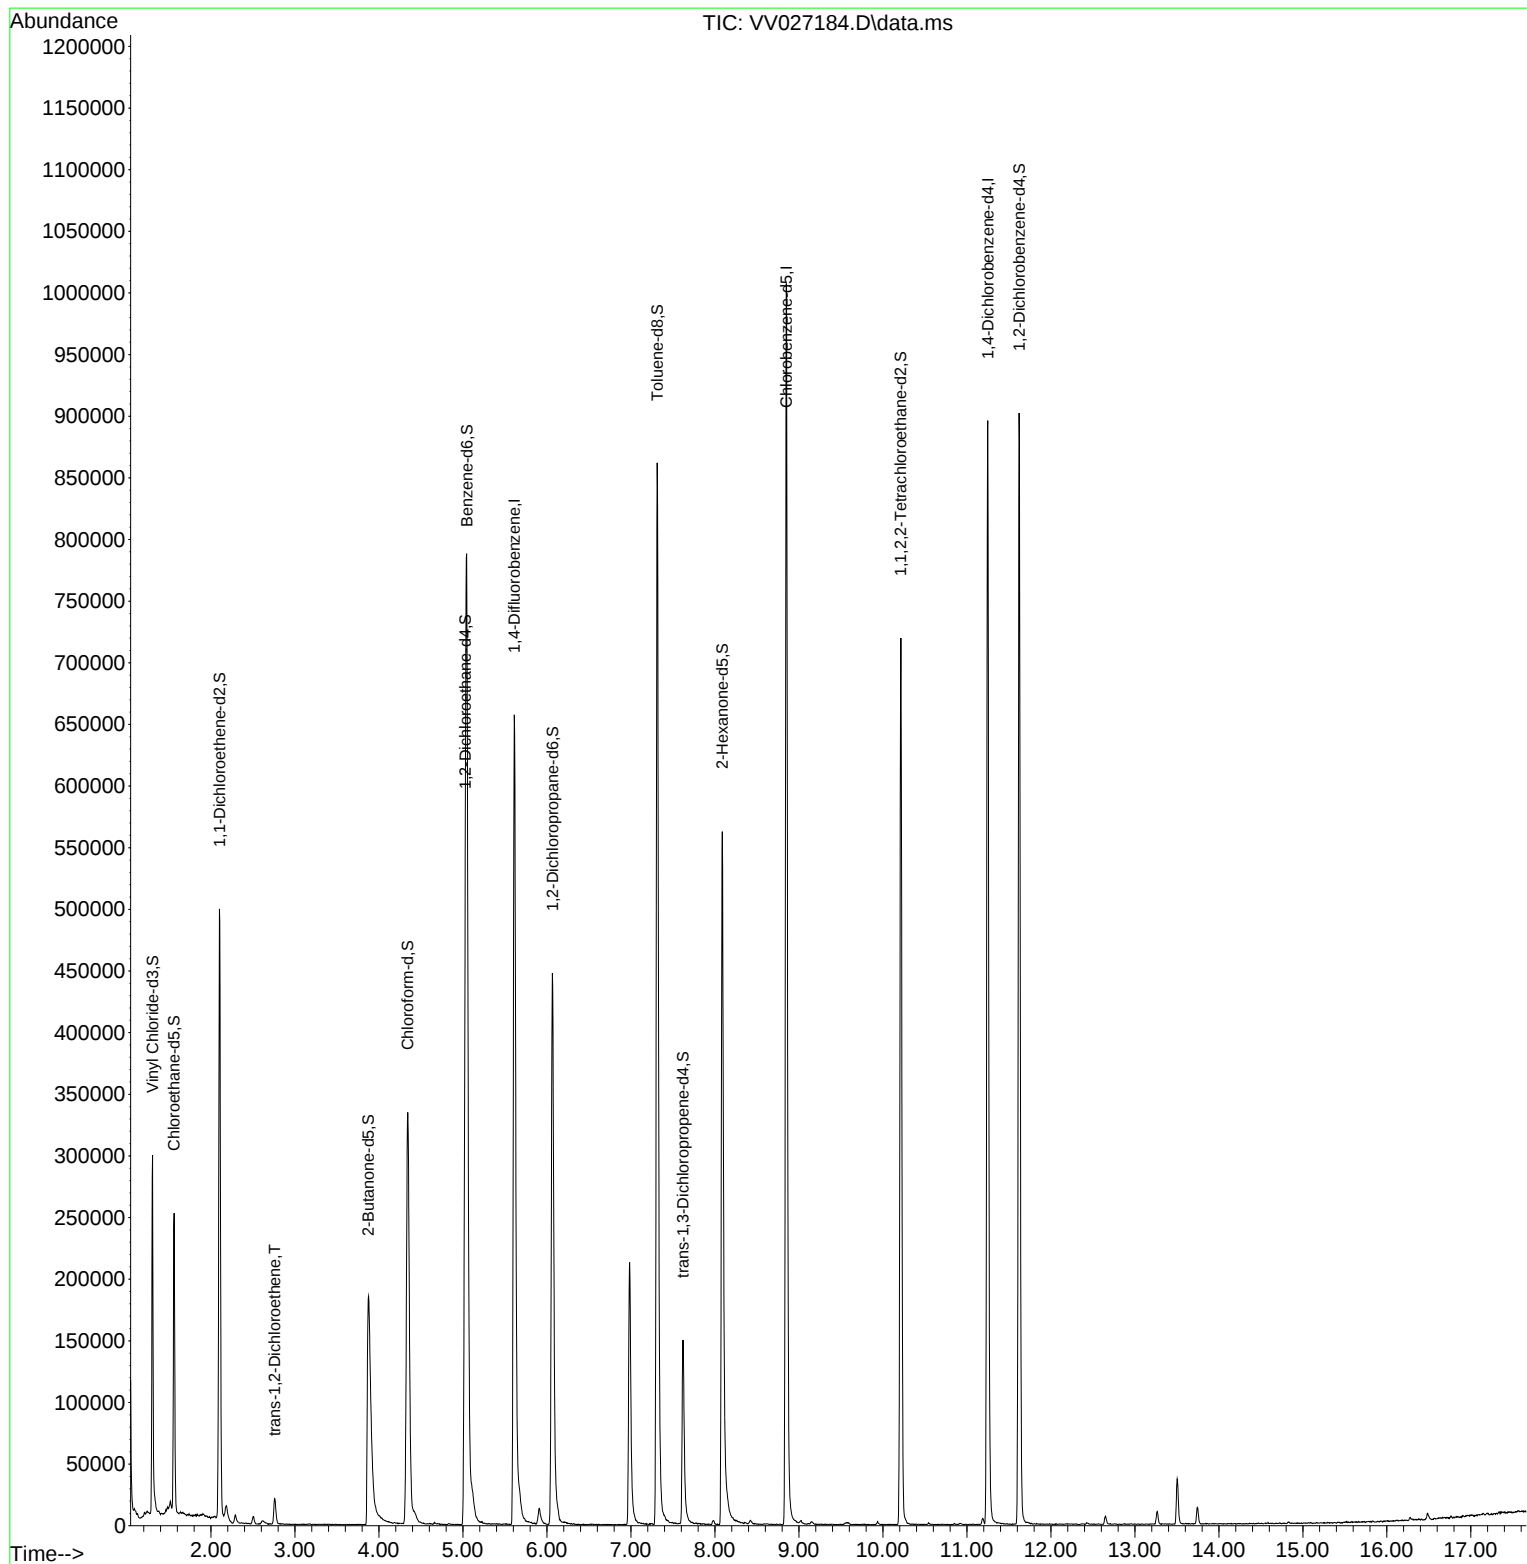

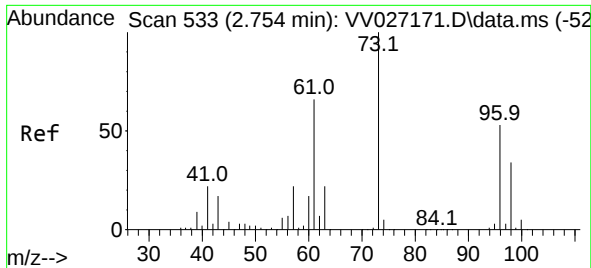

#17
 trans-1,2-Dichloroethene
 Concen: 1.891 ug/L
 RT: 2.757 min Scan# 51
 Delta R.T. 0.003 min
 Lab File: VV027184.D
 Acq: 02 Aug 2022 20:38

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK269

Tgt Ion:	96	Resp:	8646
Ion	Ratio	Lower	Upper
96	100		
61	126.9	89.2	165.6
98	63.1	43.3	80.3

