

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027137.D
 Acq On : 01 Aug 2022 20:05
 Operator : SY/MD
 Sample : VV0801WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK245

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027137.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rBV	276785	289678	13.48%	1.798%
2	1.561	155	162	176	rVB	246174	281994	13.12%	1.750%
3	2.105	321	331	344	rBV	508327	724095	33.69%	4.495%
4	2.503	446	455	465	rBV2	9062	14590	0.68%	0.091%
5	2.754	529	533	534	rBV2	1235	743	0.03%	0.005%
6	2.966	596	599	602	rBV	236	165	0.01%	0.001%
7	3.040	620	622	623	rBV	291	80	0.00%	0.000%
8	3.182	665	666	668	rBV	225	104	0.00%	0.001%
9	3.387	728	730	733	rVB3	297	122	0.01%	0.001%
10	3.455	749	751	754	rBV	304	141	0.01%	0.001%
11	3.513	765	769	772	rBV2	511	469	0.02%	0.003%
12	3.574	783	788	791	rBV3	288	214	0.01%	0.001%
13	3.699	824	827	830	rBV2	308	214	0.01%	0.001%
14	3.809	859	861	866	rBV3	238	212	0.01%	0.001%
15	3.841	866	871	872	rBV2	150	124	0.01%	0.001%
16	3.873	872	881	918	rBV	160318	463717	21.57%	2.878%
17	4.342	1011	1027	1067	rBV	345004	868115	40.39%	5.389%
18	4.812	1171	1173	1174	rBV2	260	93	0.00%	0.001%
19	4.854	1185	1186	1188	rBV	168	72	0.00%	0.000%
20	4.889	1192	1197	1198	rBV3	247	178	0.01%	0.001%
21	4.957	1215	1218	1222	rVB2	497	333	0.02%	0.002%
22	4.979	1222	1225	1227	rBV2	352	229	0.01%	0.001%
23	5.043	1227	1245	1284	rBV2	815736	2149434	100.00%	13.342%
24	5.426	1362	1364	1365	rBV	408	180	0.01%	0.001%
25	5.612	1410	1422	1458	rBV	657592	1370659	63.77%	8.508%
26	5.905	1504	1513	1530	rBV5	12470	27394	1.27%	0.170%
27	5.989	1537	1539	1540	rBV2	328	136	0.01%	0.001%
28	6.066	1549	1563	1600	rBV	467715	984399	45.80%	6.110%
29	6.317	1638	1641	1643	rBV2	487	408	0.02%	0.003%
30	6.349	1649	1651	1654	rBV2	250	141	0.01%	0.001%
31	6.378	1658	1660	1661	rVB2	377	79	0.00%	0.000%
32	6.400	1665	1667	1672	rBV2	376	295	0.01%	0.002%
33	6.439	1675	1679	1680	rBV	374	271	0.01%	0.002%
34	6.506	1698	1700	1701	rBV	560	169	0.01%	0.001%
35	6.558	1713	1716	1719	rBV3	419	395	0.02%	0.002%
36	6.629	1735	1738	1739	rBV2	210	134	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027137.D
 Acq On : 01 Aug 2022 20:05
 Operator : SY/MD
 Sample : VV0801WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK245

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.648	1742	1744	1745	rBV	261	125	0.01%	0.001%
38	6.731	1769	1770	1774	rBV	353	150	0.01%	0.001%
39	6.793	1783	1789	1792	rBV3	388	517	0.02%	0.003%
40	6.828	1797	1800	1801	rBV	144	72	0.00%	0.000%
41	6.866	1809	1812	1819	rBV3	256	264	0.01%	0.002%
42	6.982	1833	1848	1885	rBV	226293	430206	20.01%	2.670%
43	7.239	1926	1928	1935	rVB4	678	454	0.02%	0.003%
44	7.313	1939	1951	1981	rBV	942602	1664107	77.42%	10.329%
45	7.619	2036	2046	2076	rBV	158527	288027	13.40%	1.788%
46	7.944	2143	2147	2148	rBV2	477	196	0.01%	0.001%
47	7.976	2152	2157	2159	rBV3	2038	2074	0.10%	0.013%
48	8.037	2173	2176	2181	rBV3	496	381	0.02%	0.002%
49	8.088	2181	2192	2230	rBV	487023	932018	43.36%	5.785%
50	8.542	2331	2333	2337	rBV	573	343	0.02%	0.002%
51	8.770	2400	2404	2409	rBV2	276	255	0.01%	0.002%
52	8.850	2417	2429	2456	rBV	1013375	1661350	77.29%	10.312%
53	9.220	2542	2544	2549	rVB3	561	445	0.02%	0.003%
54	9.275	2558	2561	2565	rBV2	281	224	0.01%	0.001%
55	9.310	2569	2572	2575	rBV2	243	207	0.01%	0.001%
56	9.355	2584	2586	2587	rBV	132	36	0.00%	0.000%
57	9.484	2624	2626	2628	rBV	218	96	0.00%	0.001%
58	9.493	2628	2629	2631	rBV2	141	52	0.00%	0.000%
59	9.522	2631	2638	2644	rBV2	416	585	0.03%	0.004%
60	9.551	2644	2647	2648	rBV2	1048	615	0.03%	0.004%
61	9.651	2671	2678	2682	rBV2	360	494	0.02%	0.003%
62	9.722	2697	2700	2701	rBV	177	102	0.00%	0.001%
63	9.747	2706	2708	2711	rVB2	236	128	0.01%	0.001%
64	9.905	2755	2757	2761	rVB3	541	390	0.02%	0.002%
65	9.921	2761	2762	2763	rBV	591	210	0.01%	0.001%
66	10.001	2784	2787	2788	rBV	102	52	0.00%	0.000%
67	10.014	2788	2791	2796	rVB3	257	272	0.01%	0.002%
68	10.124	2823	2825	2827	rBV2	208	105	0.00%	0.001%
69	10.214	2840	2853	2881	rBV	696694	1089276	50.68%	6.761%
70	10.445	2922	2925	2933	rVB3	593	807	0.04%	0.005%
71	10.487	2935	2938	2941	rVB	291	130	0.01%	0.001%
72	10.509	2941	2945	2947	rBV	364	231	0.01%	0.001%
73	10.661	2989	2992	2994	rBV2	290	204	0.01%	0.001%
74	10.783	3027	3030	3032	rBV	308	164	0.01%	0.001%
75	10.808	3032	3038	3039	rBV2	456	459	0.02%	0.003%
76	10.853	3049	3052	3059	rBV6	534	656	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027137.D
 Acq On : 01 Aug 2022 20:05
 Operator : SY/MD
 Sample : VV0801WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK245

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	10.915	3067	3071	3073	rBV2	615	508	0.02%	0.003%
78	10.953	3081	3083	3085	rBV	250	137	0.01%	0.001%
79	11.091	3122	3126	3128	rBV2	362	272	0.01%	0.002%
80	11.104	3128	3130	3134	rVB	495	201	0.01%	0.001%
81	11.246	3163	3174	3201	rBV	898241	1401968	65.22%	8.702%
82	11.622	3279	3291	3315	rBV	905417	1413368	65.76%	8.773%
83	12.654	3605	3612	3623	rVB7	3760	6128	0.29%	0.038%
84	13.265	3795	3802	3812	rBV4	4392	7341	0.34%	0.046%
85	13.509	3871	3878	3896	rVB	10434	17291	0.80%	0.107%
86	13.747	3946	3952	3964	rVB7	4544	6963	0.32%	0.043%




Sum of corrected areas: 16110432

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027137.D
Acq On : 01 Aug 2022 20:05
Operator : SY/MD
Sample : VV0801WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK245

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

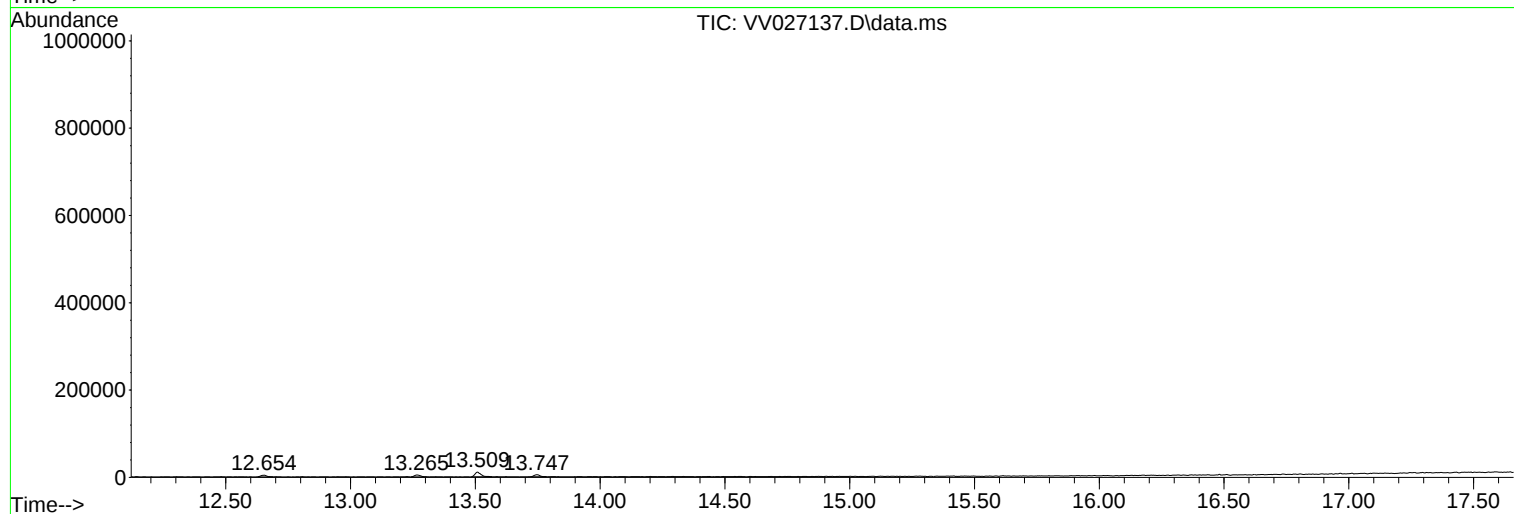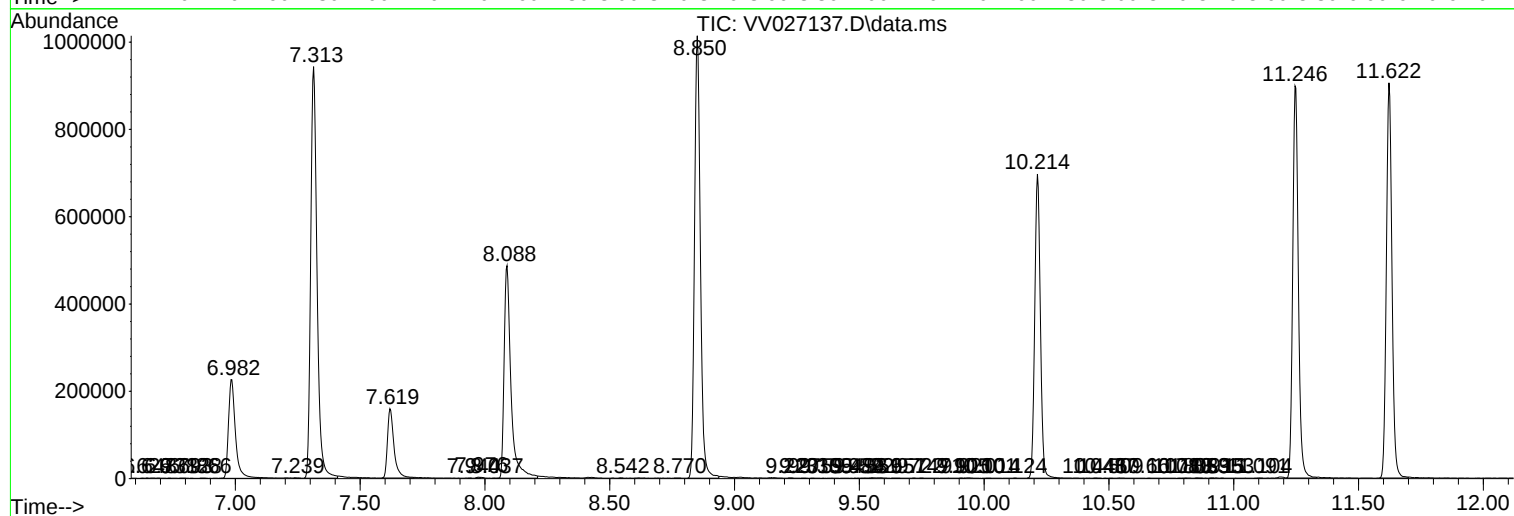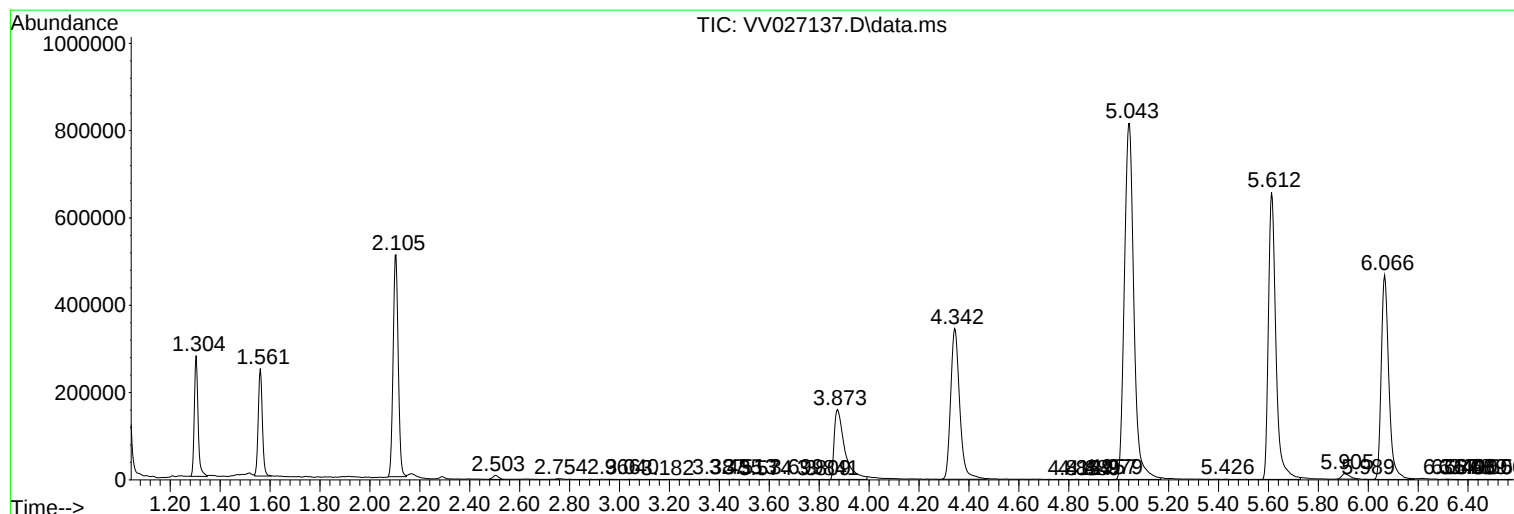

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027137.D
Acq On : 01 Aug 2022 20:05
Operator : SY/MD
Sample : VV0801WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK245

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027137.D
Acq On : 01 Aug 2022 20:05
Operator : SY/MD
Sample : VV0801WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK245

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc