

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027144.D
 Acq On : 01 Aug 2022 22:56
 Operator : SY/MD
 Sample : VIBLK264
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027144.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	93	rBV	399156	414076	16.32%	2.264%
2	1.561	155	162	176	rVB	320290	365017	14.39%	1.996%
3	2.105	321	331	345	rBV	646132	911617	35.93%	4.985%
4	2.285	384	387	388	rBV2	1326	778	0.03%	0.004%
5	2.503	445	455	469	rVB2	9064	15034	0.59%	0.082%
6	2.908	578	581	588	rVB4	291	349	0.01%	0.002%
7	2.947	588	593	595	rBV2	360	359	0.01%	0.002%
8	3.047	622	624	628	rBV2	487	345	0.01%	0.002%
9	3.134	647	651	654	rBV	323	272	0.01%	0.001%
10	3.375	724	726	731	rVB2	351	323	0.01%	0.002%
11	3.394	731	732	736	rBV	392	280	0.01%	0.002%
12	3.642	805	809	812	rBV	323	276	0.01%	0.002%
13	3.873	871	881	923	rBV	181639	528176	20.82%	2.888%
14	4.262	999	1002	1005	rBV2	444	345	0.01%	0.002%
15	4.343	1009	1027	1068	rVV	404423	1011241	39.86%	5.529%
16	4.757	1151	1156	1158	rBV2	542	445	0.02%	0.002%
17	4.796	1161	1168	1169	rBV3	561	594	0.02%	0.003%
18	4.905	1198	1202	1207	rBV3	423	410	0.02%	0.002%
19	4.976	1218	1224	1225	rBV3	332	278	0.01%	0.002%
20	5.043	1227	1245	1284	rBV2	970401	2537277	100.00%	13.873%
21	5.551	1399	1403	1405	rVB3	503	266	0.01%	0.001%
22	5.613	1410	1422	1458	rBV	661321	1382570	54.49%	7.560%
23	5.908	1504	1514	1534	rVB3	11184	24573	0.97%	0.134%
24	6.066	1548	1563	1599	rBV	544964	1145926	45.16%	6.266%
25	6.355	1648	1653	1654	rBV3	500	435	0.02%	0.002%
26	6.413	1667	1671	1673	rBV2	500	331	0.01%	0.002%
27	6.465	1683	1687	1690	rVB2	405	318	0.01%	0.002%
28	6.510	1695	1701	1706	rBV4	319	419	0.02%	0.002%
29	6.654	1740	1746	1747	rBV	480	431	0.02%	0.002%
30	6.674	1750	1752	1756	rVB2	390	283	0.01%	0.002%
31	6.892	1814	1820	1822	rBV2	370	297	0.01%	0.002%
32	6.982	1835	1848	1871	rBV	263502	496898	19.58%	2.717%
33	7.313	1938	1951	1986	rBV	1079188	1939784	76.45%	10.606%
34	7.619	2036	2046	2075	rBV	188550	338853	13.35%	1.853%
35	7.809	2100	2105	2108	rVB4	632	637	0.03%	0.003%
36	7.828	2108	2111	2116	rBV3	332	264	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027144.D
 Acq On : 01 Aug 2022 22:56
 Operator : SY/MD
 Sample : VIBLK264
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	7.857	2117	2120	2123	rVB2	616	295	0.01%	0.002%
38	7.899	2130	2133	2137	rBV3	640	587	0.02%	0.003%
39	7.928	2140	2142	2145	rVB	485	247	0.01%	0.001%
40	7.979	2146	2158	2169	rBV6	7644	14392	0.57%	0.079%
41	8.088	2181	2192	2234	rBV	621271	1176550	46.37%	6.433%
42	8.423	2289	2296	2298	rBV5	1767	1911	0.08%	0.010%
43	8.487	2314	2316	2320	rVV3	338	241	0.01%	0.001%
44	8.522	2325	2327	2328	rVB2	798	242	0.01%	0.001%
45	8.603	2349	2352	2354	rBV2	414	263	0.01%	0.001%
46	8.690	2376	2379	2383	rBV2	416	319	0.01%	0.002%
47	8.747	2393	2397	2401	rBV4	537	389	0.02%	0.002%
48	8.792	2409	2411	2416	rBV3	386	370	0.01%	0.002%
49	8.850	2416	2429	2456	rBV	1004366	1651516	65.09%	9.030%
50	9.024	2481	2483	2487	rVB2	547	353	0.01%	0.002%
51	9.137	2514	2518	2520	rBV3	535	390	0.02%	0.002%
52	9.227	2543	2546	2549	rBV3	318	241	0.01%	0.001%
53	9.281	2559	2563	2568	rVV2	246	258	0.01%	0.001%
54	9.548	2636	2646	2647	rBV2	495	503	0.02%	0.003%
55	9.680	2683	2687	2690	rBV	449	386	0.02%	0.002%
56	9.722	2695	2700	2706	rVV4	516	564	0.02%	0.003%
57	9.786	2717	2720	2726	rVB2	281	263	0.01%	0.001%
58	9.989	2778	2783	2786	rBV3	401	472	0.02%	0.003%
59	10.005	2786	2788	2794	rVB3	547	455	0.02%	0.002%
60	10.043	2794	2800	2802	rBV	270	269	0.01%	0.001%
61	10.133	2825	2828	2831	rVB2	402	243	0.01%	0.001%
62	10.169	2834	2839	2841	rBV2	345	309	0.01%	0.002%
63	10.214	2841	2853	2877	rBV	812022	1272869	50.17%	6.960%
64	10.455	2922	2928	2930	rBV2	352	330	0.01%	0.002%
65	10.468	2930	2932	2934	rVV2	444	272	0.01%	0.001%
66	10.490	2937	2939	2943	rVV2	451	358	0.01%	0.002%
67	10.577	2962	2966	2970	rBV2	298	306	0.01%	0.002%
68	10.603	2970	2974	2978	rVB2	395	290	0.01%	0.002%
69	10.641	2979	2986	2990	rBV2	389	471	0.02%	0.003%
70	10.693	2998	3002	3005	rBV2	478	482	0.02%	0.003%
71	10.850	3049	3051	3056	rVB2	966	760	0.03%	0.004%
72	11.017	3099	3103	3104	rBV2	545	318	0.01%	0.002%
73	11.079	3118	3122	3124	rBV2	429	268	0.01%	0.001%
74	11.181	3151	3154	3158	rBV3	588	513	0.02%	0.003%
75	11.246	3162	3174	3201	rBV	893225	1388045	54.71%	7.590%
76	11.622	3278	3291	3314	rBV	1035297	1619674	63.84%	8.856%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027144.D
 Acq On : 01 Aug 2022 22:56
 Operator : SY/MD
 Sample : VIBLK264
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	12.548	3576	3579	3583	rBV2	346	254	0.01%	0.001%
78	12.606	3595	3597	3602	rVB	476	312	0.01%	0.002%
79	12.654	3606	3612	3616	rVV	697	664	0.03%	0.004%
80	12.754	3640	3643	3647	rVB2	617	423	0.02%	0.002%
81	12.808	3657	3660	3665	rBV	458	341	0.01%	0.002%
82	12.940	3698	3701	3708	rBV2	384	481	0.02%	0.003%
83	13.072	3735	3742	3746	rBV2	408	500	0.02%	0.003%
84	13.262	3798	3801	3803	rBV2	530	364	0.01%	0.002%
85	13.329	3819	3822	3825	rBV	371	243	0.01%	0.001%
86	13.406	3842	3846	3849	rVB2	404	302	0.01%	0.002%
87	13.445	3849	3858	3859	rBV2	706	746	0.03%	0.004%
88	13.513	3872	3879	3886	rBV3	2423	3661	0.14%	0.020%
89	13.583	3898	3901	3903	rBV2	620	371	0.01%	0.002%
90	13.699	3935	3937	3942	rBV2	371	282	0.01%	0.002%
91	13.750	3949	3953	3959	rBV4	553	522	0.02%	0.003%
92	13.805	3967	3970	3973	rVB	493	344	0.01%	0.002%
93	14.416	4156	4160	4164	rBV2	461	489	0.02%	0.003%
94	14.638	4223	4229	4237	rBV4	2770	4444	0.18%	0.024%
95	14.821	4279	4286	4297	rBV8	2163	3868	0.15%	0.021%
96	15.130	4380	4382	4385	rBV2	702	316	0.01%	0.002%
97	15.191	4396	4401	4403	rBV6	785	810	0.03%	0.004%
98	15.371	4452	4457	4462	rVB5	1690	1903	0.08%	0.010%
99	15.455	4480	4483	4485	rBV2	788	575	0.02%	0.003%
100	16.483	4799	4803	4812	rVB4	7596	9778	0.39%	0.053%




Sum of corrected areas: 18288754

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027144.D
Acq On : 01 Aug 2022 22:56
Operator : SY/MD
Sample : VIBLK264
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

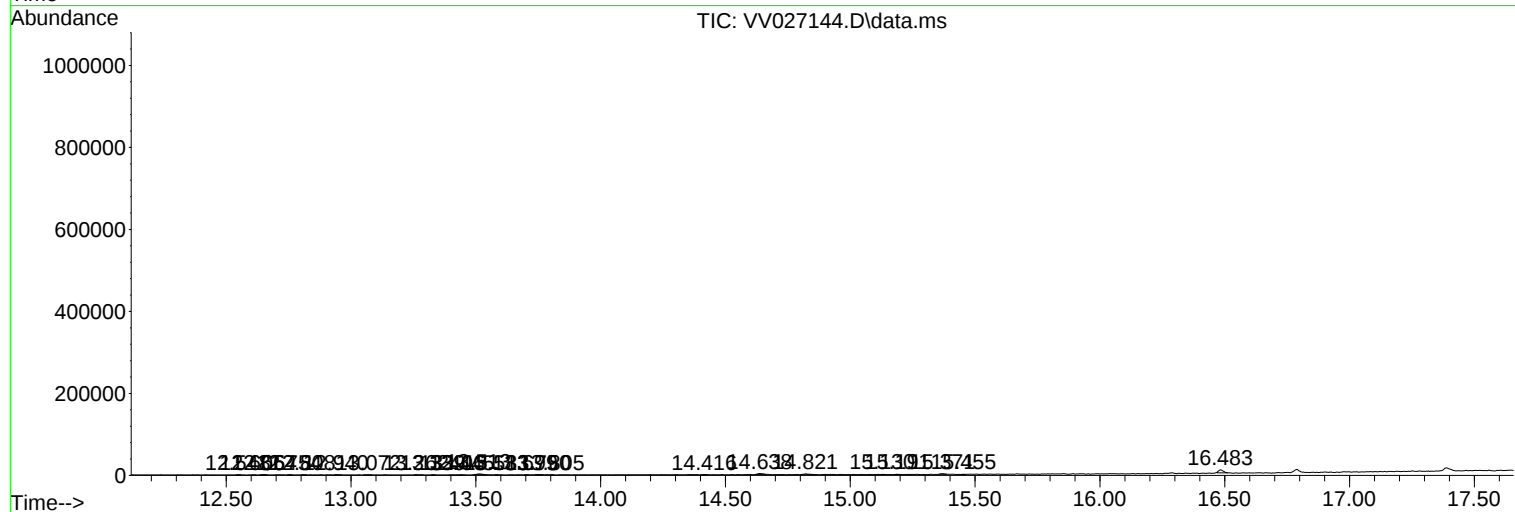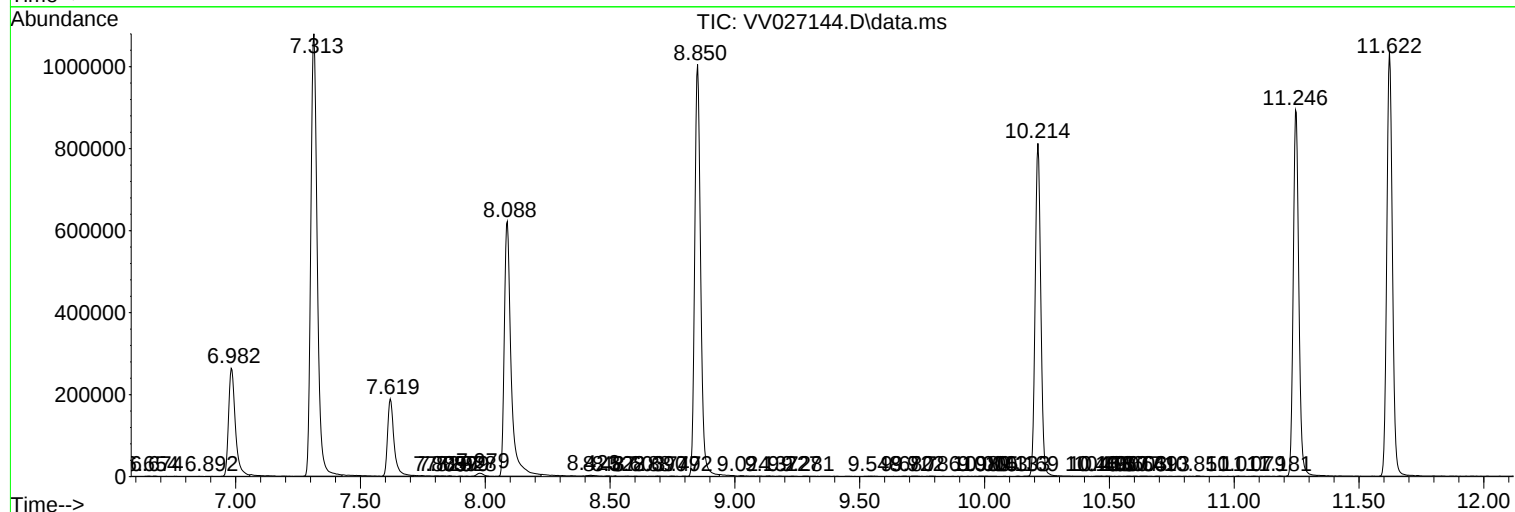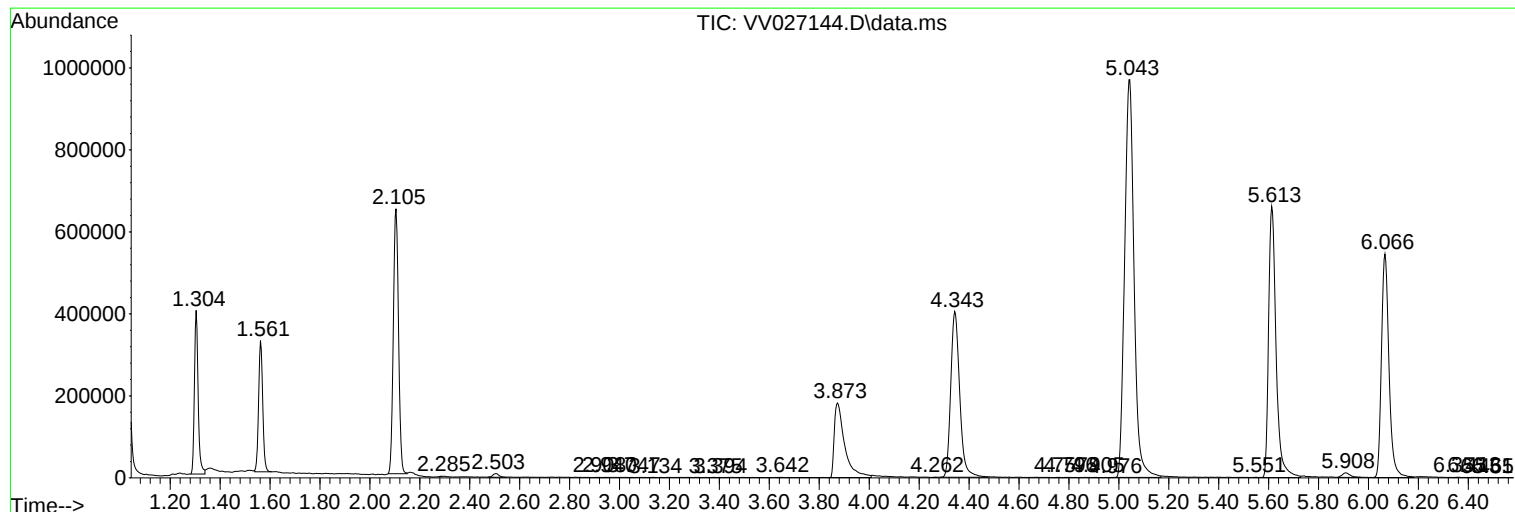

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027144.D
Acq On : 01 Aug 2022 22:56
Operator : SY/MD
Sample : VIBLK264
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027144.D
Acq On : 01 Aug 2022 22:56
Operator : SY/MD
Sample : VIBLK264
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------