

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027153.D
 Acq On : 02 Aug 2022 02:35
 Operator : SY/MD
 Sample : N3880-16 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027153.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	15	20	33	rVB	29478	30986	1.05%	0.144%
2	1.207	49	52	57	rBV	5022	4273	0.14%	0.020%
3	1.304	75	82	111	rVB	356016	422148	14.27%	1.966%
4	1.555	154	160	172	rBV	182176	198494	6.71%	0.924%
5	2.095	318	328	358	rVB	650374	946806	32.00%	4.409%
6	2.285	382	387	392	rBV5	1701	2277	0.08%	0.011%
7	2.500	445	454	470	rVB	15599	25452	0.86%	0.119%
8	2.613	476	489	502	rBV	19527	41930	1.42%	0.195%
9	2.767	535	537	542	rVB3	1037	743	0.03%	0.003%
10	2.857	560	565	567	rVV2	445	405	0.01%	0.002%
11	2.989	602	606	612	rBV3	281	352	0.01%	0.002%
12	3.040	617	622	629	rVB4	541	710	0.02%	0.003%
13	3.166	656	661	665	rBV5	633	639	0.02%	0.003%
14	3.355	716	720	725	rBV	333	362	0.01%	0.002%
15	3.391	729	731	735	rVB2	459	321	0.01%	0.001%
16	3.439	735	746	750	rBV3	436	830	0.03%	0.004%
17	3.670	816	818	824	rVB3	432	371	0.01%	0.002%
18	3.703	824	828	832	rBV3	488	413	0.01%	0.002%
19	3.876	872	882	931	rBV	174205	557084	18.83%	2.594%
20	4.272	1003	1005	1009	rVB3	609	296	0.01%	0.001%
21	4.339	1009	1026	1065	rBV	405708	1018811	34.44%	4.744%
22	4.667	1126	1128	1132	rVB2	476	304	0.01%	0.001%
23	4.719	1140	1144	1147	rBV	412	304	0.01%	0.001%
24	4.818	1173	1175	1179	rVB3	405	256	0.01%	0.001%
25	4.844	1179	1183	1186	rBV2	516	307	0.01%	0.001%
26	4.886	1193	1196	1199	rVB2	466	329	0.01%	0.002%
27	4.905	1199	1202	1204	rBV2	536	395	0.01%	0.002%
28	5.040	1226	1244	1289	rBV2	995593	2578806	87.17%	12.008%
29	5.333	1324	1335	1337	rBV7	2691	4056	0.14%	0.019%
30	5.455	1369	1373	1377	rVB3	481	338	0.01%	0.002%
31	5.477	1377	1380	1385	rBV3	367	362	0.01%	0.002%
32	5.503	1385	1388	1395	rVB3	560	550	0.02%	0.003%
33	5.545	1395	1401	1404	rBV3	360	349	0.01%	0.002%
34	5.612	1409	1422	1457	rBV	674104	1383782	46.77%	6.444%
35	5.915	1502	1516	1534	rBV6	48038	108942	3.68%	0.507%
36	6.063	1549	1562	1596	rBV	550309	1138579	38.49%	5.302%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027153.D
 Acq On : 02 Aug 2022 02:35
 Operator : SY/MD
 Sample : N3880-16 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.320	1640	1642	1647	rVB4	725	475	0.02%	0.002%
38	6.352	1647	1652	1659	rBV5	590	682	0.02%	0.003%
39	6.381	1659	1661	1664	rBV2	419	286	0.01%	0.001%
40	6.583	1721	1724	1731	rVB	403	285	0.01%	0.001%
41	6.770	1779	1782	1785	rVB3	575	357	0.01%	0.002%
42	6.799	1789	1791	1795	rBV2	630	319	0.01%	0.001%
43	6.828	1795	1800	1803	rBV	304	279	0.01%	0.001%
44	6.918	1822	1828	1833	rBV4	619	652	0.02%	0.003%
45	6.982	1836	1848	1882	rBV	267516	500786	16.93%	2.332%
46	7.204	1913	1917	1920	rBV3	630	515	0.02%	0.002%
47	7.313	1938	1951	1979	rBV	1082329	1908762	64.52%	8.888%
48	7.619	2036	2046	2081	rBV	189426	338875	11.45%	1.578%
49	7.902	2132	2134	2137	rVB2	637	298	0.01%	0.001%
50	7.972	2142	2156	2182	rBV	1776976	2958453	100.00%	13.776%
51	8.088	2182	2192	2238	rVB	601056	1214775	41.06%	5.657%
52	8.413	2289	2293	2294	rBV2	784	445	0.02%	0.002%
53	8.580	2342	2345	2348	rBV3	322	274	0.01%	0.001%
54	8.606	2351	2353	2355	rBV	560	343	0.01%	0.002%
55	8.661	2367	2370	2373	rVB3	514	327	0.01%	0.002%
56	8.680	2373	2376	2379	rVB2	537	384	0.01%	0.002%
57	8.706	2379	2384	2388	rBV2	530	579	0.02%	0.003%
58	8.735	2391	2393	2397	rVB3	469	274	0.01%	0.001%
59	8.850	2416	2429	2467	rBV	1011696	1696447	57.34%	7.900%
60	9.050	2489	2491	2498	rVB3	479	403	0.01%	0.002%
61	9.143	2515	2520	2525	rBV5	944	1125	0.04%	0.005%
62	9.252	2551	2554	2560	rVB2	427	402	0.01%	0.002%
63	9.288	2560	2565	2568	rBV2	420	474	0.02%	0.002%
64	9.313	2570	2573	2578	rVV2	368	355	0.01%	0.002%
65	9.516	2631	2636	2638	rVV4	428	346	0.01%	0.002%
66	9.542	2642	2644	2650	rVB4	500	512	0.02%	0.002%
67	9.779	2714	2718	2721	rBV2	404	347	0.01%	0.002%
68	10.091	2813	2815	2820	rVB4	613	546	0.02%	0.003%
69	10.127	2820	2826	2831	rBV2	413	417	0.01%	0.002%
70	10.214	2840	2853	2874	rBV	817742	1298576	43.89%	6.047%
71	10.416	2913	2916	2920	rBV3	617	482	0.02%	0.002%
72	10.516	2942	2947	2951	rBV4	451	350	0.01%	0.002%
73	10.590	2964	2970	2976	rVB4	746	827	0.03%	0.004%
74	10.651	2983	2989	2992	rBV3	272	287	0.01%	0.001%
75	10.844	3044	3049	3050	rBV2	488	405	0.01%	0.002%
76	10.853	3050	3052	3055	rVB2	766	521	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027153.D
 Acq On : 02 Aug 2022 02:35
 Operator : SY/MD
 Sample : N3880-16 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	10.960	3083	3085	3089	rBV2	353	318	0.01%	0.001%
78	11.021	3100	3104	3107	rBV3	321	261	0.01%	0.001%
79	11.069	3114	3119	3122	rBV3	388	376	0.01%	0.002%
80	11.246	3161	3174	3204	rBV	920079	1420274	48.01%	6.614%
81	11.419	3226	3228	3232	rVB2	760	362	0.01%	0.002%
82	11.461	3238	3241	3243	rBV3	475	270	0.01%	0.001%
83	11.622	3279	3291	3312	rBV	1047180	1638002	55.37%	7.627%
84	12.239	3479	3483	3488	rBV2	522	488	0.02%	0.002%
85	12.410	3533	3536	3543	rVB3	651	770	0.03%	0.004%
86	12.480	3555	3558	3561	rVB3	450	298	0.01%	0.001%
87	13.410	3844	3847	3851	rBV3	673	541	0.02%	0.003%
88	13.580	3895	3900	3903	rBV3	624	530	0.02%	0.002%
89	13.908	3995	4002	4010	rBV8	2789	3728	0.13%	0.017%
90	13.988	4024	4027	4030	rVB2	433	290	0.01%	0.001%
91	14.056	4046	4048	4052	rVB4	657	429	0.01%	0.002%
92	14.104	4060	4063	4068	rVB3	444	329	0.01%	0.002%
93	14.397	4151	4154	4159	rBV3	526	452	0.02%	0.002%
94	14.901	4309	4311	4314	rVB2	539	346	0.01%	0.002%
95	14.921	4314	4317	4319	rBV2	563	310	0.01%	0.001%
96	14.963	4327	4330	4338	rBV8	1824	2071	0.07%	0.010%
97	15.130	4380	4382	4384	rBV2	688	396	0.01%	0.002%
98	15.268	4423	4425	4427	rBV3	618	320	0.01%	0.001%
99	15.686	4552	4555	4560	rVB4	1092	941	0.03%	0.004%
100	15.773	4580	4582	4585	rBV3	808	312	0.01%	0.001%




Sum of corrected areas: 21475023

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027153.D
Acq On : 02 Aug 2022 02:35
Operator : SY/MD
Sample : N3880-16 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

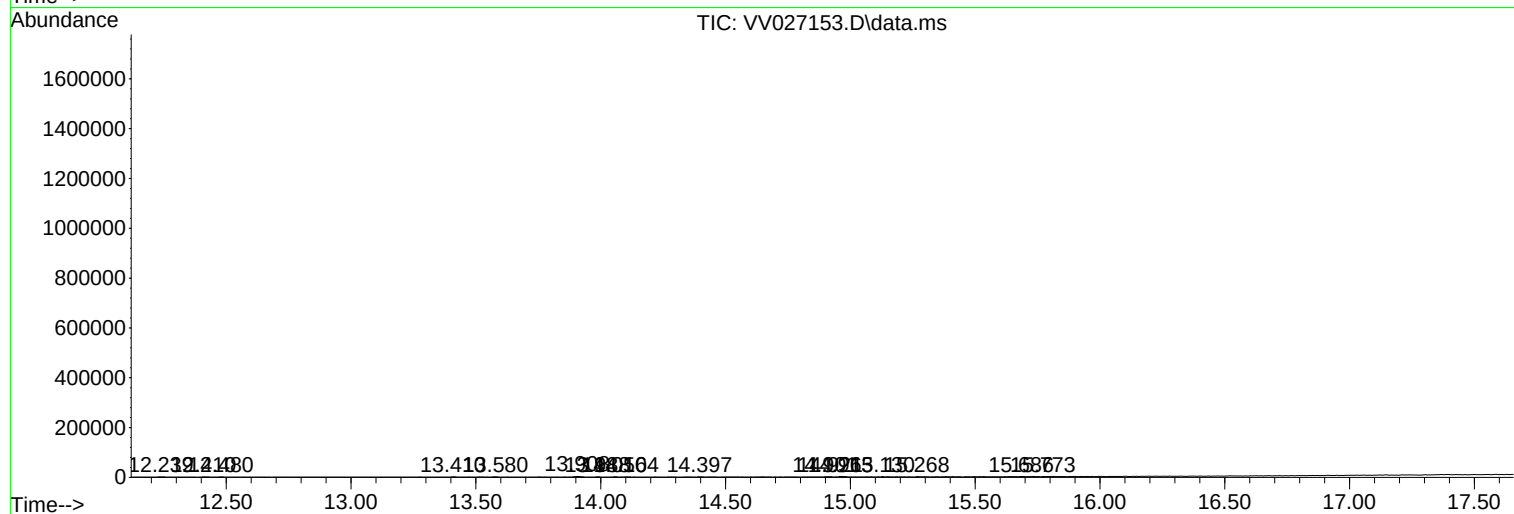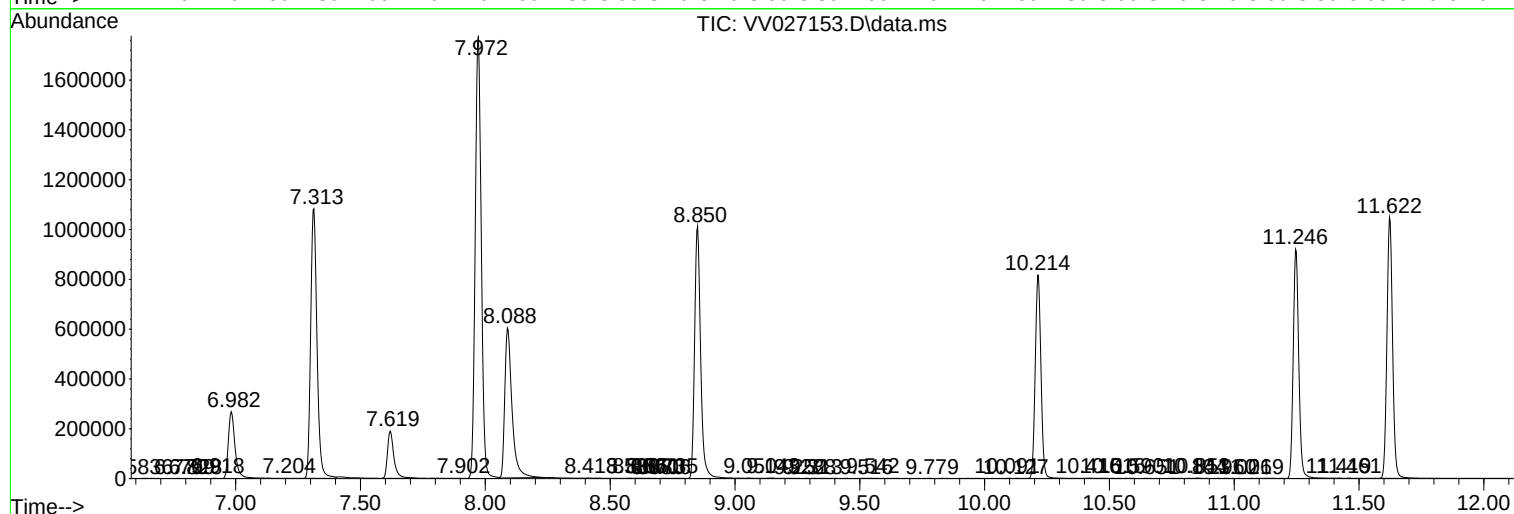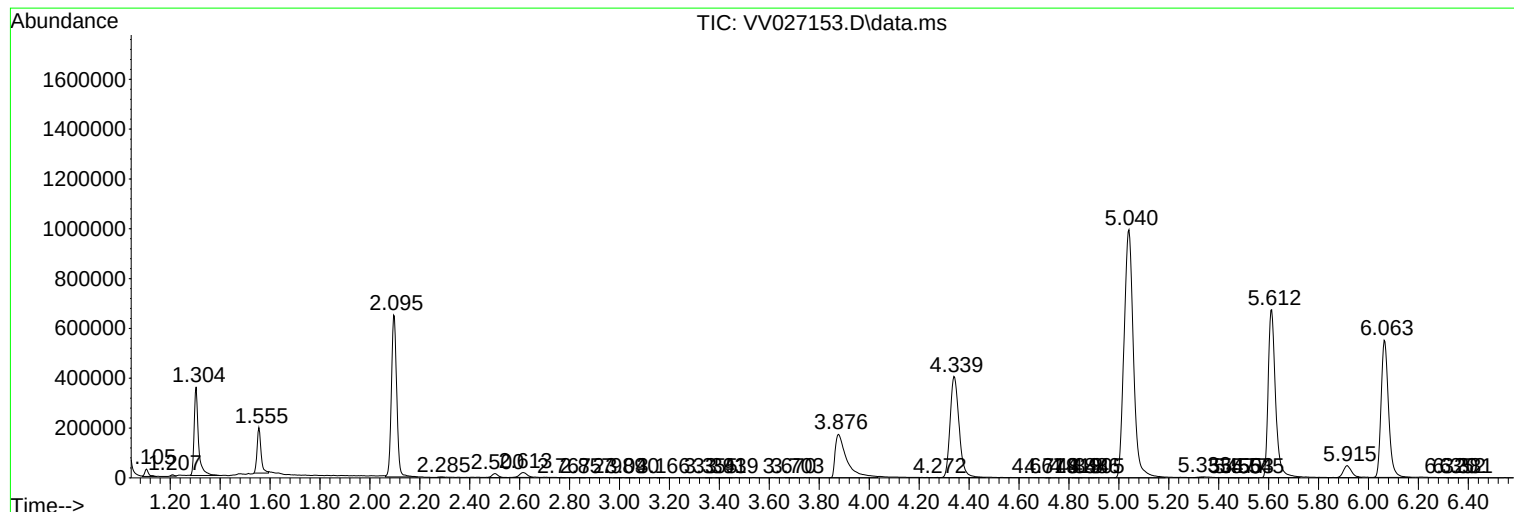

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027153.D
Acq On : 02 Aug 2022 02:35
Operator : SY/MD
Sample : N3880-16 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027153.D
Acq On : 02 Aug 2022 02:35
Operator : SY/MD
Sample : N3880-16 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc