

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027154.D
 Acq On : 02 Aug 2022 03:00
 Operator : SY/MD
 Sample : N3880-18 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027154.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	17	20	26	rVB3	5345	4066	0.12%	0.018%
2	1.208	49	52	56	rBV	4412	3769	0.11%	0.017%
3	1.304	75	82	111	rVB	379961	442746	13.05%	1.965%
4	1.555	154	160	172	rBV	189883	215712	6.36%	0.957%
5	2.098	318	329	351	rBV	696670	991708	29.24%	4.401%
6	2.282	382	386	389	rBV4	1503	1429	0.04%	0.006%
7	2.500	444	454	467	rVB3	12174	19623	0.58%	0.087%
8	2.561	471	473	476	rBV2	506	314	0.01%	0.001%
9	2.616	476	490	505	rBV	23090	49881	1.47%	0.221%
10	2.822	551	554	557	rVB2	481	303	0.01%	0.001%
11	2.847	557	562	565	rBV3	482	360	0.01%	0.002%
12	3.031	616	619	620	rBV	643	295	0.01%	0.001%
13	3.111	639	644	646	rBV3	465	390	0.01%	0.002%
14	3.600	790	796	799	rBV3	308	379	0.01%	0.002%
15	3.677	817	820	824	rVB3	423	284	0.01%	0.001%
16	3.831	864	868	872	rVB3	348	260	0.01%	0.001%
17	3.876	872	882	932	rBV	172192	572172	16.87%	2.539%
18	4.285	1007	1009	1010	rBV	531	281	0.01%	0.001%
19	4.339	1010	1026	1062	rVV	419612	1044688	30.80%	4.636%
20	4.751	1151	1154	1160	rVB3	348	361	0.01%	0.002%
21	4.822	1174	1176	1180	rVB3	488	263	0.01%	0.001%
22	4.892	1196	1198	1203	rVB3	429	263	0.01%	0.001%
23	5.040	1226	1244	1294	rBV2	1019343	2638973	77.81%	11.712%
24	5.230	1301	1303	1310	rVB5	959	724	0.02%	0.003%
25	5.330	1329	1334	1336	rBV4	2143	2315	0.07%	0.010%
26	5.417	1359	1361	1367	rVB4	733	697	0.02%	0.003%
27	5.490	1382	1384	1389	rVV3	576	383	0.01%	0.002%
28	5.613	1409	1422	1460	rBV	715284	1475676	43.51%	6.549%
29	5.908	1503	1514	1530	rBV8	13796	32802	0.97%	0.146%
30	5.986	1535	1538	1539	rBV2	686	401	0.01%	0.002%
31	6.063	1549	1562	1587	rBV	563850	1165590	34.37%	5.173%
32	6.310	1637	1639	1645	rVB4	592	458	0.01%	0.002%
33	6.349	1649	1651	1656	rVB3	649	545	0.02%	0.002%
34	6.378	1657	1660	1663	rBV2	482	297	0.01%	0.001%
35	6.420	1669	1673	1675	rBV2	343	330	0.01%	0.001%
36	6.619	1729	1735	1736	rBV2	377	327	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027154.D
 Acq On : 02 Aug 2022 03:00
 Operator : SY/MD
 Sample : N3880-18 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.645	1740	1743	1745	rBV2	613	340	0.01%	0.002%
38	6.757	1773	1778	1784	rVB3	342	425	0.01%	0.002%
39	6.982	1837	1848	1874	rBV	270724	507100	14.95%	2.250%
40	7.217	1916	1921	1925	rVB4	530	416	0.01%	0.002%
41	7.240	1925	1928	1932	rBV4	519	328	0.01%	0.001%
42	7.314	1938	1951	1979	rBV	1169523	2043319	60.25%	9.068%
43	7.619	2036	2046	2074	rBV	189033	342664	10.10%	1.521%
44	7.773	2093	2094	2098	rBV3	440	329	0.01%	0.001%
45	7.873	2121	2125	2129	rVB3	464	273	0.01%	0.001%
46	7.905	2133	2135	2139	rVB3	549	382	0.01%	0.002%
47	7.973	2142	2156	2182	rBV	2013966	3391606	100.00%	15.052%
48	8.088	2182	2192	2230	rVV	599417	1172462	34.57%	5.203%
49	8.381	2281	2283	2286	rVB3	589	288	0.01%	0.001%
50	8.490	2315	2317	2319	rBV	445	277	0.01%	0.001%
51	8.699	2379	2382	2385	rBV2	375	280	0.01%	0.001%
52	8.719	2385	2388	2392	rVB3	359	277	0.01%	0.001%
53	8.764	2399	2402	2406	rVB2	532	458	0.01%	0.002%
54	8.786	2406	2409	2414	rBV3	569	565	0.02%	0.003%
55	8.850	2414	2429	2458	rBV	1089655	1785700	52.65%	7.925%
56	9.101	2505	2507	2512	rVB3	595	269	0.01%	0.001%
57	9.130	2512	2516	2521	rVB4	549	483	0.01%	0.002%
58	9.233	2545	2548	2552	rVB3	523	482	0.01%	0.002%
59	9.452	2612	2616	2620	rBV3	391	358	0.01%	0.002%
60	9.522	2633	2638	2643	rVB3	428	436	0.01%	0.002%
61	9.564	2645	2651	2655	rBV2	727	639	0.02%	0.003%
62	9.812	2721	2728	2732	rBV2	545	751	0.02%	0.003%
63	9.883	2745	2750	2753	rBV2	638	562	0.02%	0.002%
64	9.963	2773	2775	2781	rVB3	300	296	0.01%	0.001%
65	10.079	2806	2811	2813	rBV	551	473	0.01%	0.002%
66	10.149	2829	2833	2836	rBV2	404	408	0.01%	0.002%
67	10.214	2841	2853	2876	rBV	829201	1304430	38.46%	5.789%
68	10.481	2932	2936	2939	rVB2	340	276	0.01%	0.001%
69	10.635	2980	2984	2985	rBV	502	281	0.01%	0.001%
70	10.670	2991	2995	2998	rBV2	369	301	0.01%	0.001%
71	10.725	3009	3012	3017	rVB3	444	422	0.01%	0.002%
72	10.821	3036	3042	3045	rBV3	354	425	0.01%	0.002%
73	10.860	3045	3054	3058	rBV4	1310	1537	0.05%	0.007%
74	10.969	3085	3088	3091	rVB2	454	305	0.01%	0.001%
75	11.034	3105	3108	3115	rVB2	561	589	0.02%	0.003%
76	11.146	3141	3143	3148	rBV2	524	576	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027154.D
 Acq On : 02 Aug 2022 03:00
 Operator : SY/MD
 Sample : N3880-18 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	11.246	3160	3174	3204	rBV	1006227	1551308	45.74%	6.885%
78	11.622	3278	3291	3313	rBV	1104689	1740684	51.32%	7.725%
79	11.792	3342	3344	3352	rVB4	836	689	0.02%	0.003%
80	12.001	3408	3409	3414	rBV3	329	301	0.01%	0.001%
81	12.175	3459	3463	3466	rBV	331	312	0.01%	0.001%
82	12.194	3467	3469	3472	rVV3	449	304	0.01%	0.001%
83	12.210	3472	3474	3477	rVB2	459	263	0.01%	0.001%
84	12.583	3586	3590	3592	rBV2	504	348	0.01%	0.002%
85	12.944	3697	3702	3704	rBV3	305	306	0.01%	0.001%
86	13.207	3782	3784	3788	rVB2	518	316	0.01%	0.001%
87	13.365	3829	3833	3836	rBV	484	333	0.01%	0.001%
88	13.693	3930	3935	3936	rBV2	584	477	0.01%	0.002%
89	13.757	3952	3955	3959	rBV2	544	392	0.01%	0.002%
90	13.805	3966	3970	3973	rBV3	468	423	0.01%	0.002%
91	13.828	3973	3977	3980	rVB2	442	317	0.01%	0.001%
92	13.908	4000	4002	4005	rVB2	719	397	0.01%	0.002%
93	13.972	4018	4022	4031	rVB4	905	1059	0.03%	0.005%
94	14.146	4069	4076	4077	rBV3	523	590	0.02%	0.003%
95	14.516	4187	4191	4194	rBV2	477	350	0.01%	0.002%
96	14.879	4301	4304	4305	rBV	568	312	0.01%	0.001%
97	14.963	4327	4330	4333	rBV3	1099	830	0.02%	0.004%
98	15.082	4364	4367	4368	rBV2	761	431	0.01%	0.002%
99	15.278	4425	4428	4432	rVB4	817	556	0.02%	0.002%
100	15.400	4463	4466	4469	rBV4	1219	1014	0.03%	0.005%




Sum of corrected areas: 22533165

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027154.D
Acq On : 02 Aug 2022 03:00
Operator : SY/MD
Sample : N3880-18 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

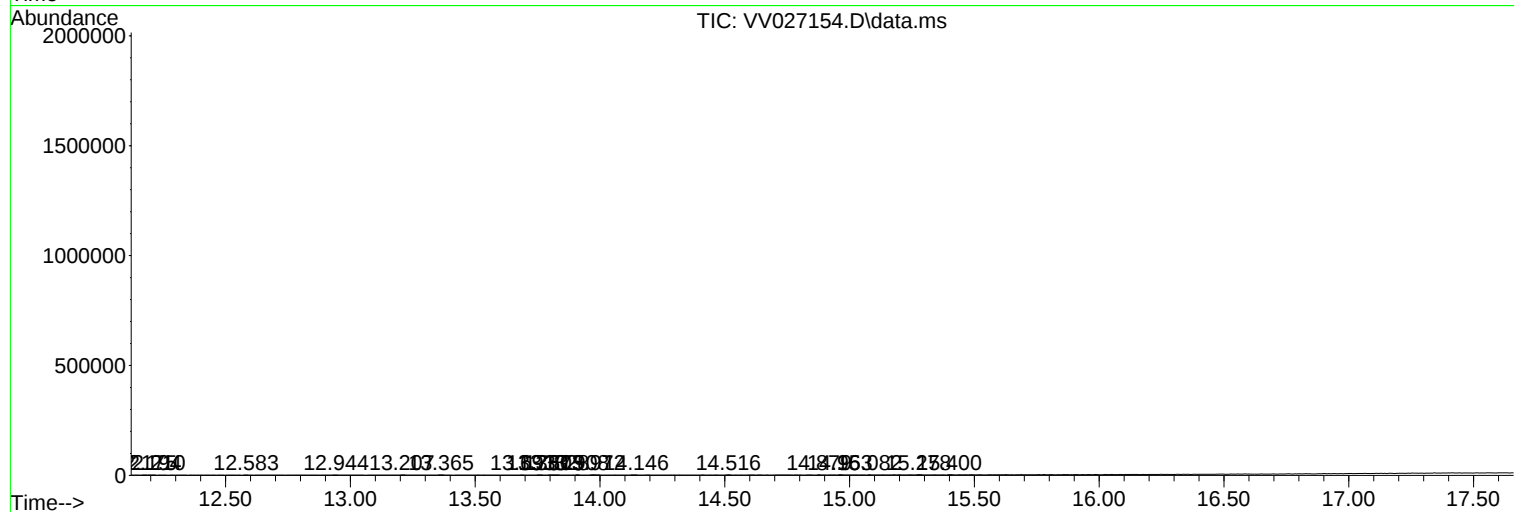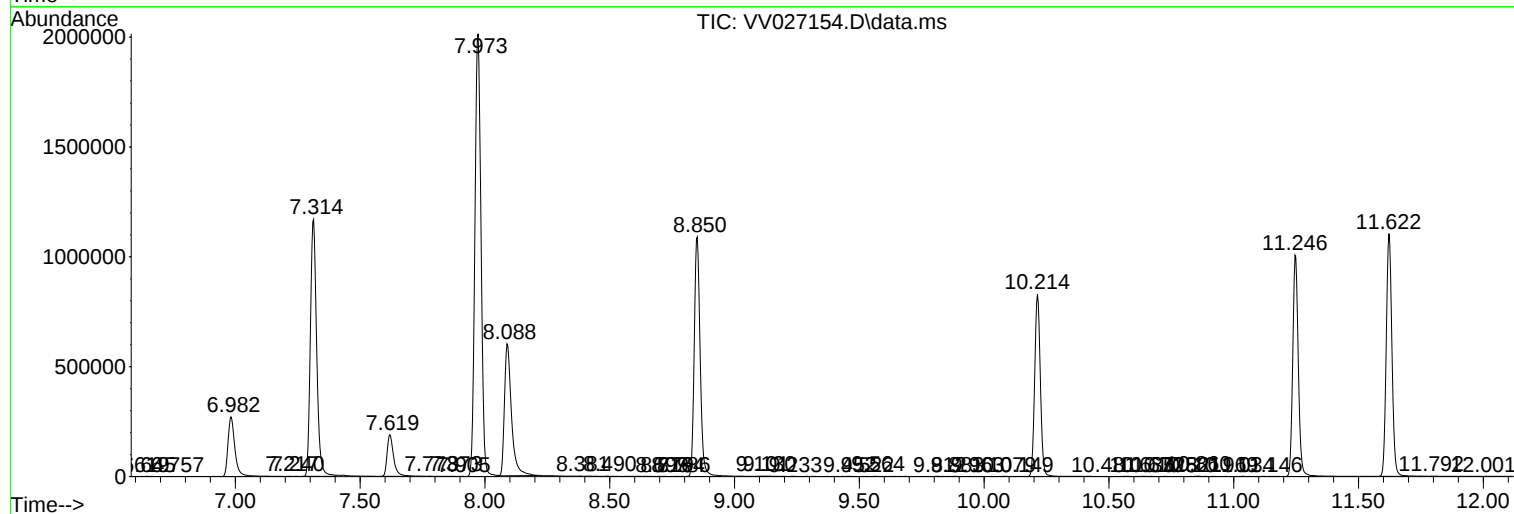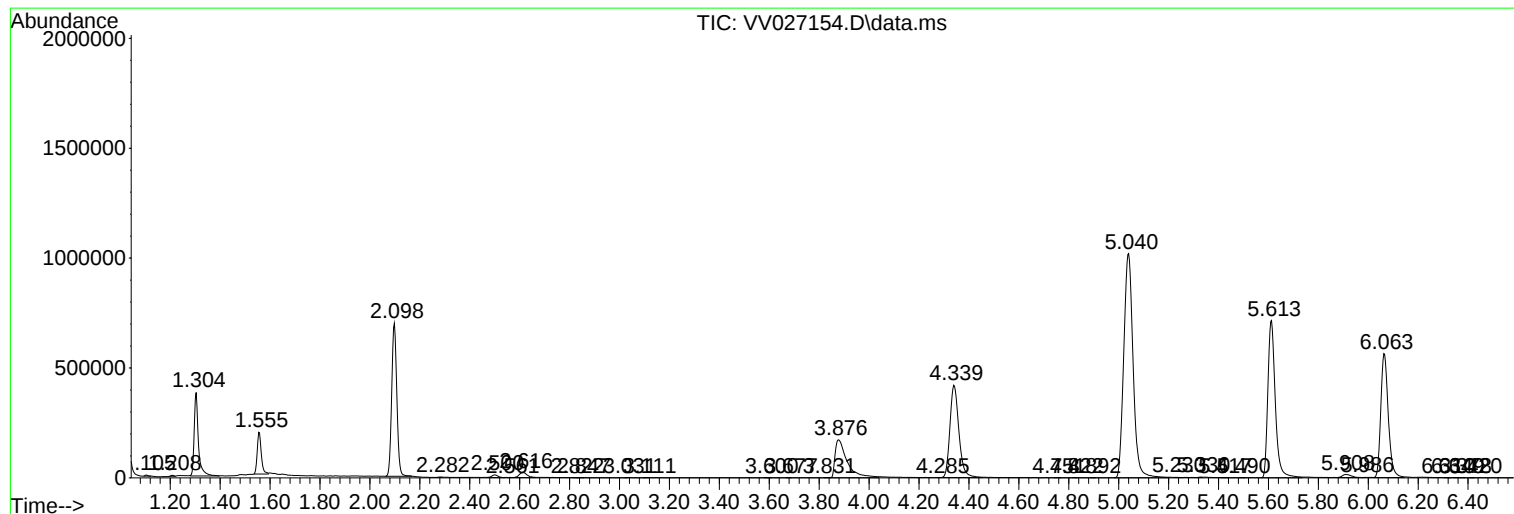

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027154.D
Acq On : 02 Aug 2022 03:00
Operator : SY/MD
Sample : N3880-18 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027154.D
Acq On : 02 Aug 2022 03:00
Operator : SY/MD
Sample : N3880-18 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc