

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027156.D
 Acq On : 02 Aug 2022 05:01
 Operator : SY/MD
 Sample : VV0801WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK246

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027156.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rBV	269880	282749	13.18%	1.793%
2	1.561	156	162	177	rVB	242945	277451	12.93%	1.759%
3	2.105	322	331	357	rVB	502143	724813	33.78%	4.595%
4	2.503	446	455	470	rBV	9792	17101	0.80%	0.108%
5	3.243	681	685	690	rBV2	420	535	0.02%	0.003%
6	3.510	767	768	773	rBV	278	260	0.01%	0.002%
7	3.574	782	788	795	rVB2	335	431	0.02%	0.003%
8	3.619	798	802	803	rBV2	385	241	0.01%	0.002%
9	3.735	835	838	840	rVB2	263	166	0.01%	0.001%
10	3.754	840	844	848	rBV2	384	422	0.02%	0.003%
11	3.806	857	860	863	rVB	484	261	0.01%	0.002%
12	3.835	867	869	870	rBV	190	87	0.00%	0.001%
13	3.876	872	882	919	rBV	155767	452303	21.08%	2.868%
14	4.005	919	922	926	rVB	14721	8630	0.40%	0.055%
15	4.343	1011	1027	1064	rBV	344464	864885	40.31%	5.484%
16	4.754	1149	1155	1161	rBV4	853	938	0.04%	0.006%
17	4.822	1173	1176	1179	rBV2	677	561	0.03%	0.004%
18	4.915	1204	1205	1206	rVB	292	56	0.00%	0.000%
19	4.925	1206	1208	1210	rBV3	352	159	0.01%	0.001%
20	5.043	1227	1245	1293	rBV2	817194	2145681	100.00%	13.604%
21	5.378	1347	1349	1353	rVB2	569	288	0.01%	0.002%
22	5.613	1406	1422	1457	rBV	647825	1344231	62.65%	8.523%
23	5.908	1504	1514	1529	rBV6	10098	22376	1.04%	0.142%
24	6.066	1549	1563	1595	rBV	477106	982923	45.81%	6.232%
25	6.362	1653	1655	1658	rBV2	590	315	0.01%	0.002%
26	6.420	1670	1673	1677	rBV2	428	259	0.01%	0.002%
27	6.449	1680	1682	1684	rVV2	266	87	0.00%	0.001%
28	6.458	1684	1685	1688	rVV	174	118	0.01%	0.001%
29	6.478	1690	1691	1695	rVB	548	214	0.01%	0.001%
30	6.584	1718	1724	1726	rBV	294	315	0.01%	0.002%
31	6.609	1730	1732	1735	rVB2	320	168	0.01%	0.001%
32	6.645	1740	1743	1744	rBV2	530	293	0.01%	0.002%
33	6.719	1764	1766	1770	rBV	427	259	0.01%	0.002%
34	6.738	1770	1772	1775	rBV2	167	66	0.00%	0.000%
35	6.822	1795	1798	1799	rBV2	103	57	0.00%	0.000%
36	6.834	1799	1802	1806	rVB3	628	436	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027156.D
 Acq On : 02 Aug 2022 05:01
 Operator : SY/MD
 Sample : VV0801WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK246

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.870	1809	1813	1814	rBV2	289	220	0.01%	0.001%
38	6.937	1832	1834	1835	rBV	154	79	0.00%	0.001%
39	6.986	1836	1849	1876	rBV	212946	408013	19.02%	2.587%
40	7.191	1911	1913	1917	rBV3	683	638	0.03%	0.004%
41	7.313	1938	1951	1979	rBV	911980	1593568	74.27%	10.104%
42	7.619	2035	2046	2077	rBV	150746	273987	12.77%	1.737%
43	7.902	2128	2134	2139	rBV4	697	643	0.03%	0.004%
44	7.928	2139	2142	2145	rBV2	371	224	0.01%	0.001%
45	7.979	2151	2158	2169	rVB5	2526	4127	0.19%	0.026%
46	8.018	2169	2170	2171	rBV	277	66	0.00%	0.000%
47	8.088	2181	2192	2230	rBV	488974	935858	43.62%	5.934%
48	8.590	2345	2348	2349	rVB3	404	178	0.01%	0.001%
49	8.654	2365	2368	2372	rVB	551	322	0.02%	0.002%
50	8.670	2372	2373	2374	rBV	330	97	0.00%	0.001%
51	8.728	2388	2391	2393	rBV2	419	305	0.01%	0.002%
52	8.850	2416	2429	2455	rBV	988318	1591636	74.18%	10.091%
53	9.217	2540	2543	2547	rVB4	506	302	0.01%	0.002%
54	9.281	2560	2563	2566	rBV2	570	291	0.01%	0.002%
55	9.304	2568	2570	2574	rVB2	392	224	0.01%	0.001%
56	9.326	2574	2577	2582	rBV2	307	296	0.01%	0.002%
57	9.381	2592	2594	2595	rVB2	425	88	0.00%	0.001%
58	9.754	2702	2710	2715	rBV4	535	621	0.03%	0.004%
59	9.783	2715	2719	2724	rVV2	389	376	0.02%	0.002%
60	9.805	2724	2726	2728	rVB2	249	102	0.00%	0.001%
61	9.873	2744	2747	2749	rBV2	261	188	0.01%	0.001%
62	10.111	2818	2821	2822	rBV	140	90	0.00%	0.001%
63	10.140	2828	2830	2832	rBV	260	125	0.01%	0.001%
64	10.214	2838	2853	2880	rBV	703900	1105470	51.52%	7.009%
65	10.374	2899	2903	2908	rBV4	446	545	0.03%	0.003%
66	10.458	2928	2929	2930	rBV	488	104	0.00%	0.001%
67	10.471	2930	2933	2936	rBV3	479	410	0.02%	0.003%
68	10.545	2944	2956	2959	rBV4	838	1308	0.06%	0.008%
69	10.577	2964	2966	2970	rVB	386	213	0.01%	0.001%
70	10.596	2970	2972	2977	rVB2	376	313	0.01%	0.002%
71	10.622	2977	2980	2983	rBV	487	334	0.02%	0.002%
72	10.786	3028	3031	3032	rBV	239	109	0.01%	0.001%
73	10.850	3049	3051	3052	rBV	401	168	0.01%	0.001%
74	10.918	3069	3072	3076	rBV4	518	445	0.02%	0.003%
75	10.966	3085	3087	3090	rBV	344	243	0.01%	0.002%
76	11.133	3136	3139	3142	rBV	388	246	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027156.D
 Acq On : 02 Aug 2022 05:01
 Operator : SY/MD
 Sample : VV0801WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK246

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M

Title : VOC Analysis

77	11.246	3163	3174	3200	rBV	843130	1332140	62.08%	8.446%
78	11.622	3279	3291	3316	rBV	870006	1365153	63.62%	8.655%
79	12.304	3501	3503	3504	rBV	262	97	0.00%	0.001%
80	12.329	3508	3511	3515	rVB3	536	331	0.02%	0.002%
81	12.471	3553	3555	3557	rBV2	269	142	0.01%	0.001%
82	13.268	3798	3803	3813	rVB6	2869	4083	0.19%	0.026%
83	13.509	3871	3878	3889	rVB2	7842	11889	0.55%	0.075%
84	13.744	3945	3951	3962	rBV5	4285	5797	0.27%	0.037%




Sum of corrected areas: 15772339

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027156.D
Acq On : 02 Aug 2022 05:01
Operator : SY/MD
Sample : VV0801WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK246

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

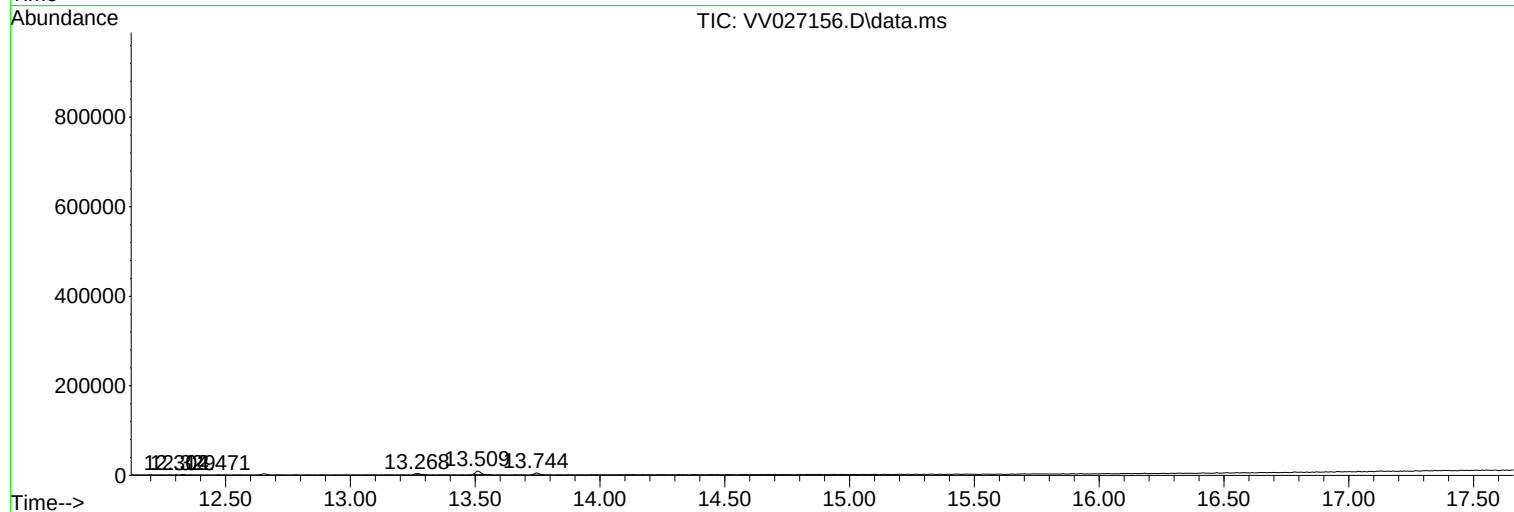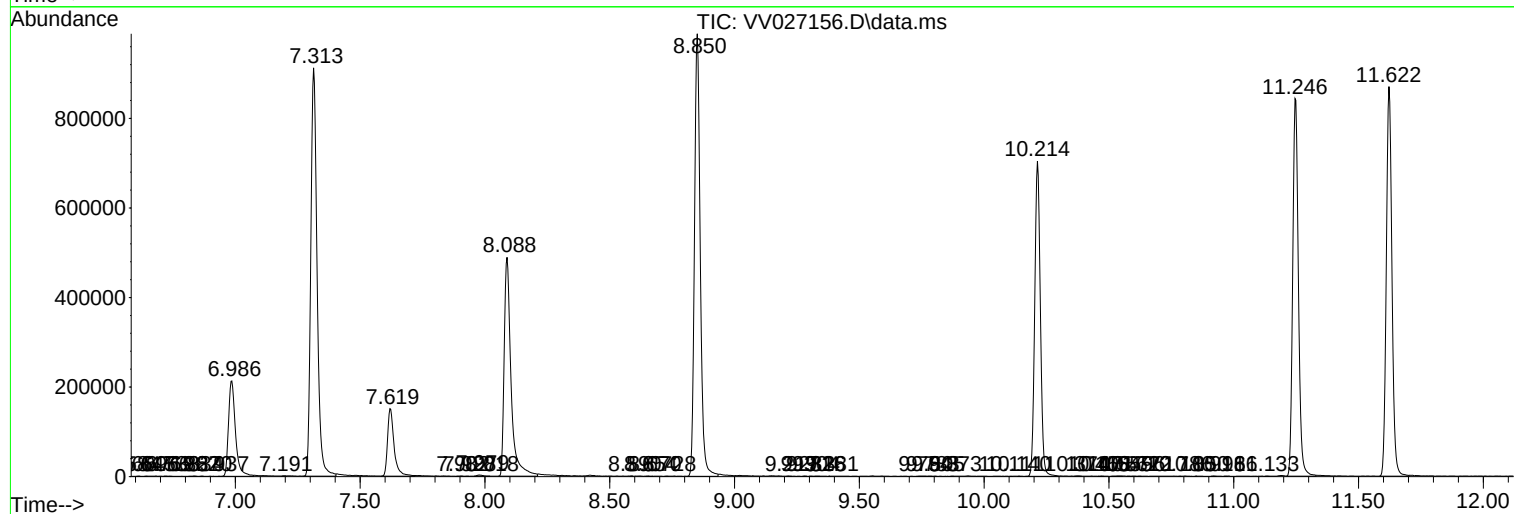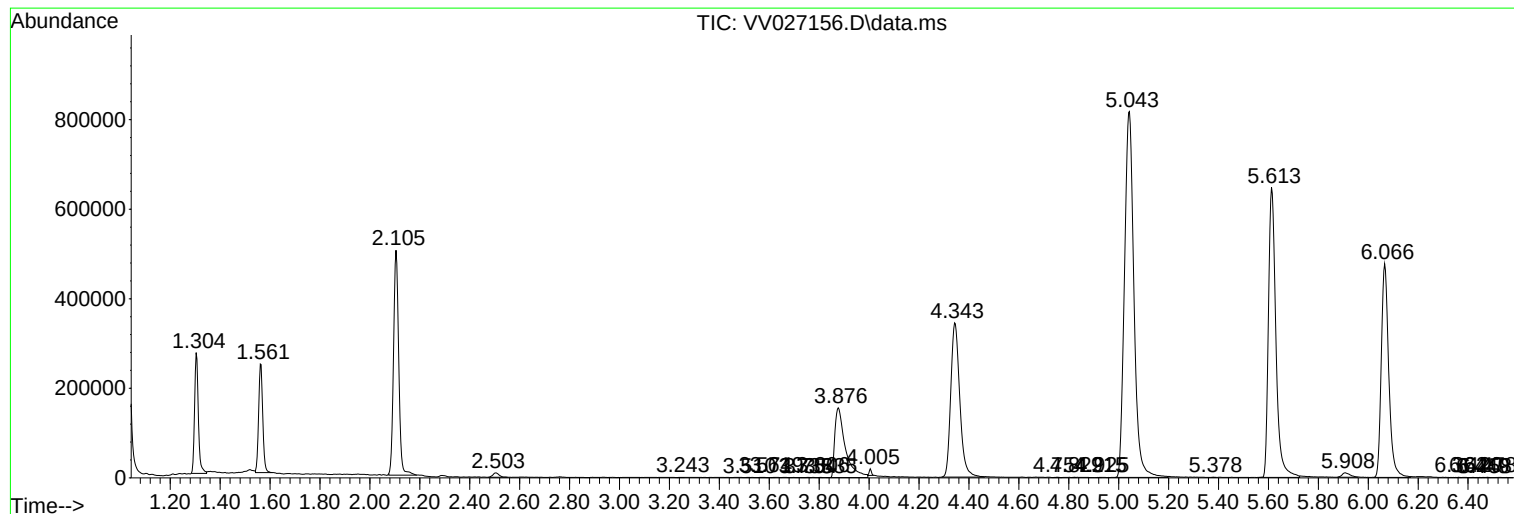

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027156.D
Acq On : 02 Aug 2022 05:01
Operator : SY/MD
Sample : VV0801WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK246

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027156.D
Acq On : 02 Aug 2022 05:01
Operator : SY/MD
Sample : VV0801WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK246

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc