

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027157.D
 Acq On : 02 Aug 2022 07:59
 Operator : SY/MD
 Sample : N3955-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027157.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB	264597	283053	13.29%	1.694%
2	1.564	157	163	175	rVB	234717	263619	12.38%	1.577%
3	2.105	321	331	348	rVB	515623	737760	34.64%	4.415%
4	2.831	554	557	561	rBV2	339	273	0.01%	0.002%
5	2.870	567	569	572	rBV2	352	217	0.01%	0.001%
6	2.928	585	587	590	rBV	438	271	0.01%	0.002%
7	2.963	594	598	601	rVB3	445	289	0.01%	0.002%
8	3.047	622	624	628	rVB	654	275	0.01%	0.002%
9	3.092	632	638	642	rBV2	401	436	0.02%	0.003%
10	3.220	674	678	681	rVB3	568	249	0.01%	0.001%
11	3.236	681	683	686	rVV2	217	125	0.01%	0.001%
12	3.252	686	688	699	rVB2	420	439	0.02%	0.003%
13	3.297	699	702	704	rBV2	212	127	0.01%	0.001%
14	3.336	706	714	720	rBV3	336	417	0.02%	0.002%
15	3.371	722	725	728	rVB	372	166	0.01%	0.001%
16	3.407	733	736	740	rVB2	334	183	0.01%	0.001%
17	3.445	745	748	752	rBV2	284	218	0.01%	0.001%
18	3.539	774	777	780	rBV2	359	241	0.01%	0.001%
19	3.555	780	782	785	rBV3	252	174	0.01%	0.001%
20	3.664	813	816	819	rBV	324	157	0.01%	0.001%
21	3.722	833	834	841	rVB2	263	218	0.01%	0.001%
22	3.783	849	853	857	rBV2	335	280	0.01%	0.002%
23	3.879	872	883	922	rBV2	153923	510578	23.97%	3.055%
24	4.339	1009	1026	1055	rBV	350037	876692	41.16%	5.246%
25	4.600	1105	1107	1111	rBV3	489	319	0.01%	0.002%
26	4.783	1161	1164	1167	rVB2	400	213	0.01%	0.001%
27	4.822	1172	1176	1180	rBV3	482	388	0.02%	0.002%
28	4.870	1188	1191	1194	rBV	218	157	0.01%	0.001%
29	4.895	1198	1199	1204	rVB	258	127	0.01%	0.001%
30	4.940	1211	1213	1216	rBV2	376	265	0.01%	0.002%
31	5.037	1226	1243	1277	rBV2	821915	2130063	100.00%	12.746%
32	5.342	1336	1338	1341	rVB	750	315	0.01%	0.002%
33	5.477	1377	1380	1382	rBV3	489	350	0.02%	0.002%
34	5.526	1390	1395	1396	rBV3	315	227	0.01%	0.001%
35	5.609	1408	1421	1451	rBV	732086	1491345	70.01%	8.924%
36	5.902	1502	1512	1530	rBV3	10119	22730	1.07%	0.136%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027157.D
 Acq On : 02 Aug 2022 07:59
 Operator : SY/MD
 Sample : N3955-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	5.989	1536	1539	1541	rVB3	379	198	0.01%	0.001%
38	6.063	1546	1562	1598	rBV	475118	984789	46.23%	5.893%
39	6.320	1641	1642	1644	rBV	282	154	0.01%	0.001%
40	6.429	1673	1676	1681	rVB3	430	327	0.02%	0.002%
41	6.452	1681	1683	1686	rBV	277	137	0.01%	0.001%
42	6.474	1686	1690	1693	rBV2	346	240	0.01%	0.001%
43	6.529	1704	1707	1709	rBV	212	155	0.01%	0.001%
44	6.583	1720	1724	1727	rVB3	178	131	0.01%	0.001%
45	6.635	1738	1740	1743	rBV	377	292	0.01%	0.002%
46	6.719	1762	1766	1768	rBV2	145	126	0.01%	0.001%
47	6.735	1768	1771	1776	rVB2	313	248	0.01%	0.001%
48	6.805	1791	1793	1796	rVB2	387	210	0.01%	0.001%
49	6.886	1813	1818	1821	rBV2	214	168	0.01%	0.001%
50	6.979	1836	1847	1882	rBV	230499	435727	20.46%	2.607%
51	7.310	1936	1950	1977	rBV	944381	1654907	77.69%	9.903%
52	7.616	2036	2045	2073	rBV	162012	287260	13.49%	1.719%
53	7.876	2124	2126	2129	rVB2	401	238	0.01%	0.001%
54	7.892	2129	2131	2134	rBV2	238	190	0.01%	0.001%
55	7.973	2150	2156	2157	rBV3	1609	1370	0.06%	0.008%
56	8.021	2168	2171	2174	rBV3	480	365	0.02%	0.002%
57	8.040	2174	2177	2179	rBV2	372	219	0.01%	0.001%
58	8.085	2181	2191	2230	rBV	461025	904079	42.44%	5.410%
59	8.487	2312	2316	2319	rBV2	536	464	0.02%	0.003%
60	8.564	2338	2340	2348	rVB3	480	497	0.02%	0.003%
61	8.609	2348	2354	2358	rBV3	669	923	0.04%	0.006%
62	8.657	2367	2369	2372	rBV2	404	256	0.01%	0.002%
63	8.696	2379	2381	2386	rVB2	434	333	0.02%	0.002%
64	8.747	2393	2397	2400	rBV2	346	309	0.01%	0.002%
65	8.767	2400	2403	2408	rVB3	573	479	0.02%	0.003%
66	8.847	2416	2428	2471	rBV	1112457	1820723	85.48%	10.895%
67	9.326	2575	2577	2581	rBV2	234	129	0.01%	0.001%
68	9.358	2585	2587	2589	rBV2	349	137	0.01%	0.001%
69	9.487	2622	2627	2631	rBV2	498	369	0.02%	0.002%
70	9.525	2637	2639	2642	rBV	321	217	0.01%	0.001%
71	9.709	2694	2696	2698	rBV	293	148	0.01%	0.001%
72	9.870	2743	2746	2749	rBV	274	191	0.01%	0.001%
73	9.902	2754	2756	2761	rVB	341	235	0.01%	0.001%
74	9.931	2761	2765	2768	rBV2	563	444	0.02%	0.003%
75	10.043	2797	2800	2804	rBV2	340	291	0.01%	0.002%
76	10.140	2827	2830	2833	rVB3	180	133	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027157.D
 Acq On : 02 Aug 2022 07:59
 Operator : SY/MD
 Sample : N3955-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	10.210	2839	2852	2877	rBV	706400	1110718	52.14%	6.646%
78	10.413	2913	2915	2918	rBV2	270	156	0.01%	0.001%
79	10.477	2933	2935	2938	rVB3	352	216	0.01%	0.001%
80	10.509	2941	2945	2947	rBV2	210	186	0.01%	0.001%
81	10.599	2969	2973	2974	rBV2	294	219	0.01%	0.001%
82	10.628	2980	2982	2985	rVB	433	163	0.01%	0.001%
83	10.648	2985	2988	2991	rBV2	314	246	0.01%	0.001%
84	10.824	3041	3043	3045	rBV	209	127	0.01%	0.001%
85	10.844	3047	3049	3051	rBV	337	244	0.01%	0.001%
86	10.879	3058	3060	3062	rBV2	306	157	0.01%	0.001%
87	11.143	3136	3142	3143	rBV	216	160	0.01%	0.001%
88	11.188	3145	3156	3163	rBV4	1227	2324	0.11%	0.014%
89	11.246	3163	3174	3210	rBV	1046092	1632956	76.66%	9.771%
90	11.532	3258	3263	3264	rBV3	1001	613	0.03%	0.004%
91	11.622	3279	3291	3313	rBV	974744	1529725	71.82%	9.154%
92	11.873	3367	3369	3373	rBV3	272	199	0.01%	0.001%
93	12.213	3472	3475	3479	rBV	344	297	0.01%	0.002%
94	12.651	3602	3611	3618	rBV5	1539	2232	0.10%	0.013%
95	12.728	3631	3635	3637	rBV2	528	380	0.02%	0.002%
96	12.795	3653	3656	3659	rBV	387	210	0.01%	0.001%
97	12.988	3712	3716	3719	rBV	420	360	0.02%	0.002%
98	13.262	3796	3801	3812	rVB5	1640	2499	0.12%	0.015%
99	13.509	3873	3878	3886	rBV3	3063	3817	0.18%	0.023%
100	13.744	3945	3951	3959	rVB5	2101	2563	0.12%	0.015%




Sum of corrected areas: 16711531

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027157.D
Acq On : 02 Aug 2022 07:59
Operator : SY/MD
Sample : N3955-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

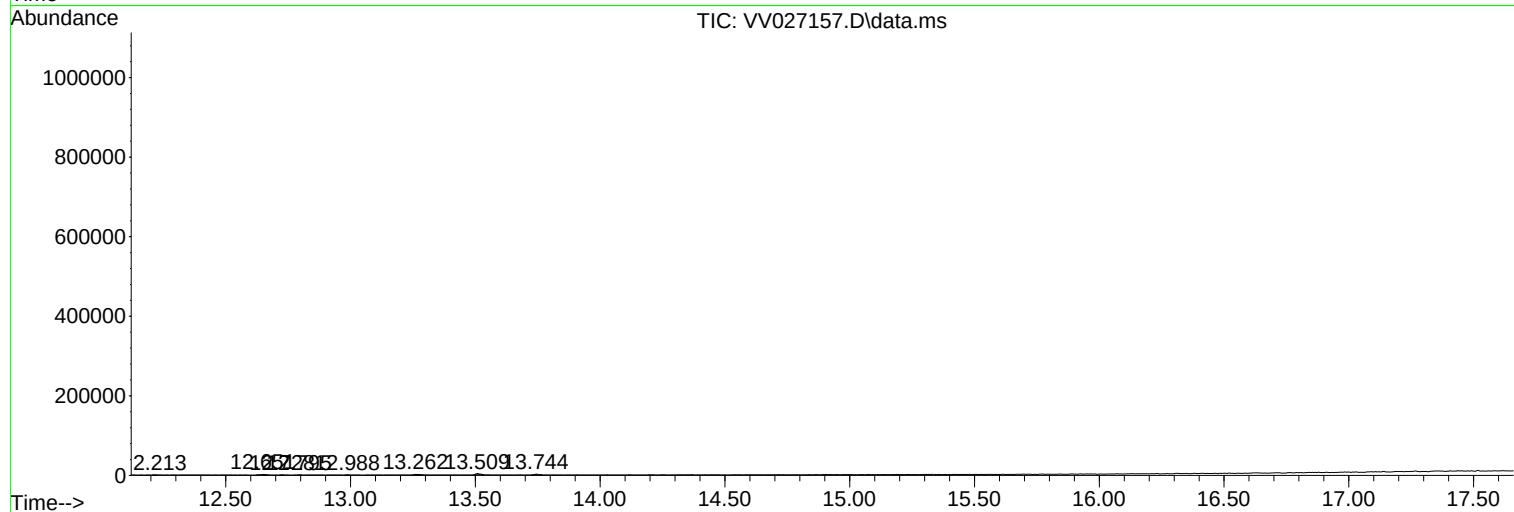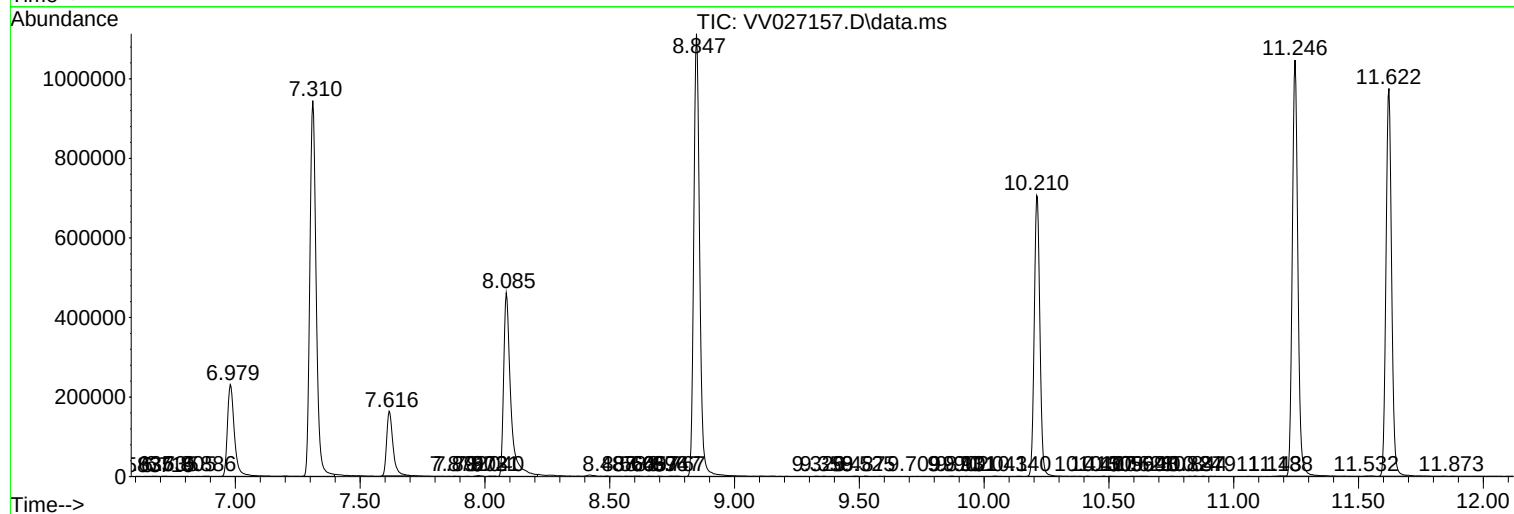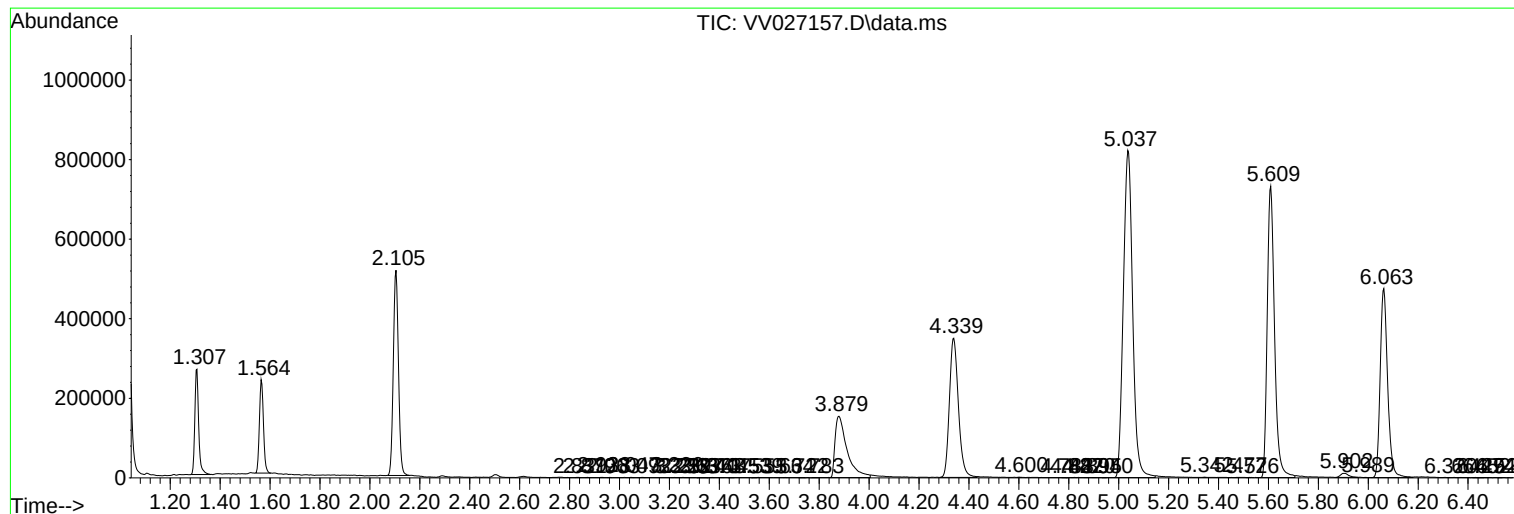

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027157.D
Acq On : 02 Aug 2022 07:59
Operator : SY/MD
Sample : N3955-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027157.D
Acq On : 02 Aug 2022 07:59
Operator : SY/MD
Sample : N3955-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc