

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027159.D
 Acq On : 02 Aug 2022 08:48
 Operator : SY/MD
 Sample : VIBLK265
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK265

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027159.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.208	49	52	56	rBV2	2974	2235	0.10%	0.013%
2	1.301	74	81	95	rBV	334213	350029	16.05%	2.086%
3	1.561	155	162	181	rVB	270325	303353	13.91%	1.808%
4	2.101	320	330	352	rVB	560449	800388	36.71%	4.770%
5	2.285	385	387	388	rBV3	901	403	0.02%	0.002%
6	2.362	408	411	412	rBV2	467	290	0.01%	0.002%
7	2.436	431	434	436	rBV2	640	357	0.02%	0.002%
8	2.500	447	454	466	rVB3	6497	10478	0.48%	0.062%
9	2.616	480	490	499	rBV	2917	4902	0.22%	0.029%
10	2.687	510	512	518	rVB3	254	259	0.01%	0.002%
11	3.056	622	627	630	rVB2	318	298	0.01%	0.002%
12	3.079	630	634	638	rBV2	359	333	0.02%	0.002%
13	3.285	692	698	704	rVB3	410	575	0.03%	0.003%
14	3.545	775	779	784	rVB2	312	308	0.01%	0.002%
15	3.597	792	795	798	rBV2	400	268	0.01%	0.002%
16	3.783	851	853	862	rVB2	363	449	0.02%	0.003%
17	3.880	868	883	925	rBV2	165156	565538	25.94%	3.370%
18	4.339	1010	1026	1058	rBV	354587	886665	40.67%	5.284%
19	4.658	1122	1125	1129	rBV3	326	264	0.01%	0.002%
20	4.786	1161	1165	1169	rBV2	358	351	0.02%	0.002%
21	5.040	1227	1244	1282	rBV2	834098	2180287	100.00%	12.993%
22	5.394	1349	1354	1357	rVV5	602	548	0.03%	0.003%
23	5.416	1357	1361	1362	rVV3	552	380	0.02%	0.002%
24	5.429	1363	1365	1370	rVB2	708	359	0.02%	0.002%
25	5.613	1409	1422	1451	rBV	669433	1379054	63.25%	8.218%
26	5.912	1504	1515	1526	rBV2	8962	18857	0.86%	0.112%
27	6.066	1548	1563	1590	rBV	476348	991884	45.49%	5.911%
28	6.275	1623	1628	1633	rBV3	783	973	0.04%	0.006%
29	6.326	1639	1644	1648	rVB4	695	697	0.03%	0.004%
30	6.346	1648	1650	1654	rVB2	566	397	0.02%	0.002%
31	6.397	1664	1666	1669	rVB	433	258	0.01%	0.002%
32	6.577	1720	1722	1727	rVB	533	332	0.02%	0.002%
33	6.603	1727	1730	1732	rBV	409	300	0.01%	0.002%
34	6.625	1735	1737	1743	rVB3	560	390	0.02%	0.002%
35	6.667	1743	1750	1756	rVB2	366	519	0.02%	0.003%
36	6.982	1834	1848	1882	rBV	235087	445270	20.42%	2.654%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027159.D
 Acq On : 02 Aug 2022 08:48
 Operator : SY/MD
 Sample : VIBLK265
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK265

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	7.169	1903	1906	1912	rVB4	881	814	0.04%	0.005%
38	7.204	1912	1917	1918	rBV3	462	354	0.02%	0.002%
39	7.246	1926	1930	1934	rVB4	409	299	0.01%	0.002%
40	7.313	1938	1951	1980	rBV	934766	1654184	75.87%	9.858%
41	7.619	2036	2046	2069	rBV	167999	296052	13.58%	1.764%
42	7.741	2081	2084	2091	rVB6	972	972	0.04%	0.006%
43	7.924	2137	2141	2142	rBV	501	318	0.01%	0.002%
44	7.979	2149	2158	2173	rVB5	8774	16886	0.77%	0.101%
45	8.034	2173	2175	2178	rBV2	461	307	0.01%	0.002%
46	8.088	2181	2192	2239	rBV	541990	1070129	49.08%	6.377%
47	8.420	2292	2295	2298	rBV2	1085	792	0.04%	0.005%
48	8.609	2350	2354	2355	rBV	430	316	0.01%	0.002%
49	8.850	2413	2429	2456	rBV	1038918	1688421	77.44%	10.062%
50	9.114	2509	2511	2516	rVB3	431	274	0.01%	0.002%
51	9.191	2532	2535	2540	rVB6	427	361	0.02%	0.002%
52	9.230	2544	2547	2554	rBV4	349	304	0.01%	0.002%
53	9.294	2564	2567	2571	rBV3	357	272	0.01%	0.002%
54	9.526	2635	2639	2642	rVB2	332	296	0.01%	0.002%
55	9.693	2684	2691	2695	rVB2	236	341	0.02%	0.002%
56	9.715	2695	2698	2702	rBV3	331	312	0.01%	0.002%
57	9.767	2708	2714	2717	rBV2	382	369	0.02%	0.002%
58	9.985	2779	2782	2786	rVB2	404	285	0.01%	0.002%
59	10.214	2840	2853	2874	rBV	744125	1162490	53.32%	6.928%
60	10.510	2941	2945	2947	rBV2	317	264	0.01%	0.002%
61	10.545	2953	2956	2962	rBV3	383	339	0.02%	0.002%
62	10.574	2962	2965	2970	rBV	366	415	0.02%	0.002%
63	10.664	2990	2993	2997	rBV2	346	285	0.01%	0.002%
64	10.744	3013	3018	3022	rBV3	272	287	0.01%	0.002%
65	10.815	3037	3040	3045	rBV3	266	256	0.01%	0.002%
66	10.854	3049	3052	3055	rBV3	573	382	0.02%	0.002%
67	10.927	3071	3075	3077	rBV2	301	268	0.01%	0.002%
68	11.079	3117	3122	3127	rBV2	209	281	0.01%	0.002%
69	11.104	3127	3130	3136	rVB3	411	397	0.02%	0.002%
70	11.140	3136	3141	3143	rBV2	352	324	0.01%	0.002%
71	11.246	3163	3174	3199	rBV	913099	1445245	66.29%	8.613%
72	11.542	3262	3266	3271	rBV4	957	878	0.04%	0.005%
73	11.577	3274	3277	3279	rBV2	328	272	0.01%	0.002%
74	11.622	3279	3291	3313	rBV	943288	1474575	67.63%	8.788%
75	11.918	3382	3383	3389	rVB3	355	274	0.01%	0.002%
76	11.966	3396	3398	3403	rVB2	416	268	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027159.D
 Acq On : 02 Aug 2022 08:48
 Operator : SY/MD
 Sample : VIBLK265
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK265

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	12.066	3427	3429	3436	rVB3	460	444	0.02%	0.003%
78	12.181	3462	3465	3468	rBV	454	339	0.02%	0.002%
79	12.349	3514	3517	3520	rVB	620	427	0.02%	0.003%
80	12.625	3598	3603	3607	rBV2	386	458	0.02%	0.003%
81	12.654	3609	3612	3620	rVB2	703	768	0.04%	0.005%
82	12.882	3680	3683	3688	rVB	470	400	0.02%	0.002%
83	13.005	3717	3721	3725	rBV3	324	270	0.01%	0.002%
84	13.268	3798	3803	3806	rBV4	594	631	0.03%	0.004%
85	13.281	3806	3807	3813	rVB4	767	564	0.03%	0.003%
86	13.480	3864	3869	3873	rBV2	483	730	0.03%	0.004%
87	13.574	3896	3898	3902	rBV2	461	348	0.02%	0.002%
88	13.706	3935	3939	3942	rBV3	667	424	0.02%	0.003%
89	13.760	3952	3956	3961	rBV4	335	350	0.02%	0.002%
90	13.985	4020	4026	4027	rBV3	555	457	0.02%	0.003%
91	14.024	4036	4038	4040	rBV	493	260	0.01%	0.002%
92	14.095	4056	4060	4062	rBV3	601	391	0.02%	0.002%
93	14.435	4159	4166	4169	rBV4	571	702	0.03%	0.004%
94	14.513	4188	4190	4193	rBV3	551	288	0.01%	0.002%
95	14.548	4198	4201	4205	rVB3	589	383	0.02%	0.002%
96	14.943	4320	4324	4331	rVB6	714	881	0.04%	0.005%
97	14.982	4334	4336	4341	rBV4	607	496	0.02%	0.003%
98	15.024	4347	4349	4353	rVB3	870	408	0.02%	0.002%
99	15.143	4383	4386	4389	rBV3	616	492	0.02%	0.003%
100	15.233	4410	4414	4417	rBV4	907	694	0.03%	0.004%




Sum of corrected areas: 16780011

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027159.D
Acq On : 02 Aug 2022 08:48
Operator : SY/MD
Sample : VIBLK265
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK265

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

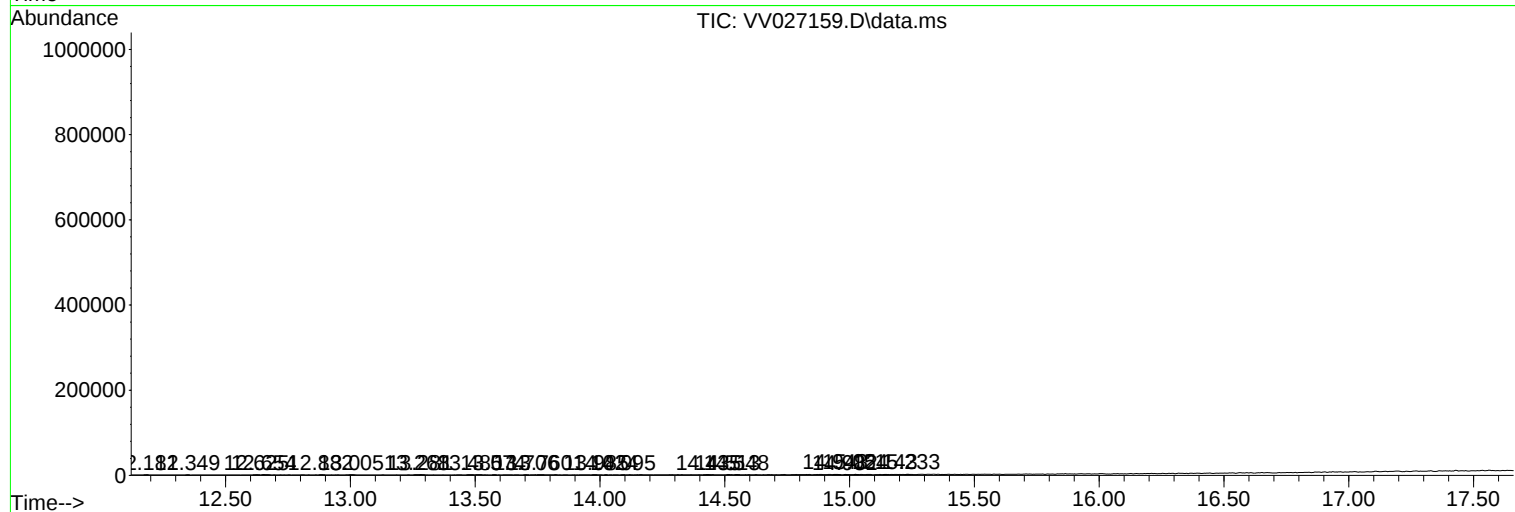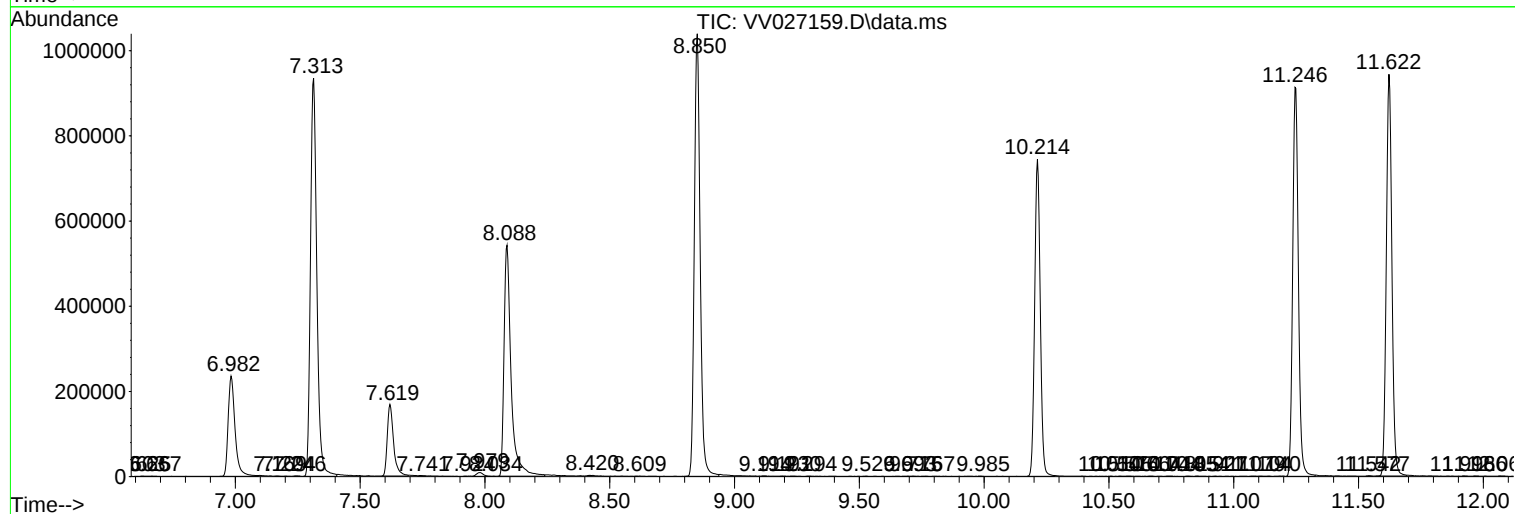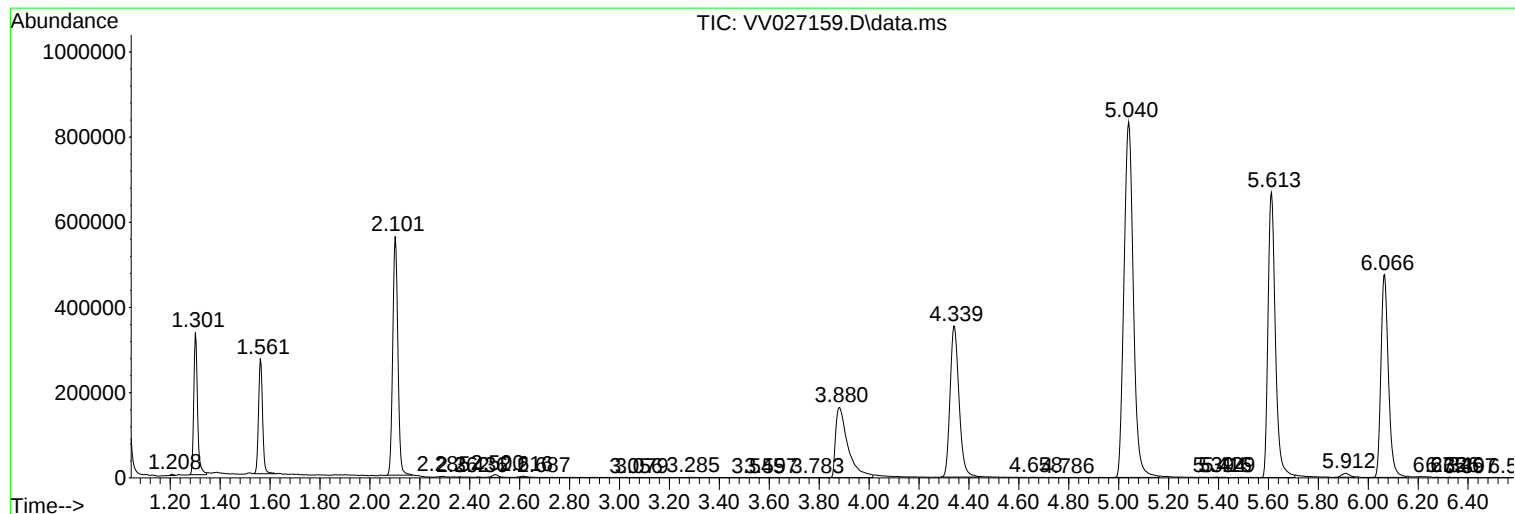

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027159.D
Acq On : 02 Aug 2022 08:48
Operator : SY/MD
Sample : VIBLK265
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK265

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027159.D
Acq On : 02 Aug 2022 08:48
Operator : SY/MD
Sample : VIBLK265
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK265

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc