

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027160.D
 Acq On : 02 Aug 2022 09:16
 Operator : SY/MD
 Sample : N3880-17DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUH1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027160.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rBV	251214	266461	13.20%	1.565%
2	1.564	156	163	175	rVB	223608	248222	12.30%	1.457%
3	2.105	320	331	350	rBV	474777	685900	33.99%	4.027%
4	2.291	384	389	397	rVV3	1769	2418	0.12%	0.014%
5	2.416	426	428	432	rVB4	571	278	0.01%	0.002%
6	2.503	447	455	470	rVB3	6466	11627	0.58%	0.068%
7	2.558	470	472	475	rBV	322	230	0.01%	0.001%
8	2.622	479	492	498	rBV2	2197	4356	0.22%	0.026%
9	2.728	523	525	529	rVB3	308	232	0.01%	0.001%
10	2.770	532	538	545	rBV3	276	413	0.02%	0.002%
11	2.809	545	550	552	rBV3	377	375	0.02%	0.002%
12	2.844	558	561	565	rBV2	337	242	0.01%	0.001%
13	3.034	617	620	623	rBV	397	243	0.01%	0.001%
14	3.336	709	714	719	rBV3	407	430	0.02%	0.003%
15	3.606	795	798	802	rVB2	391	300	0.01%	0.002%
16	3.629	802	805	809	rBV2	291	284	0.01%	0.002%
17	3.879	871	883	924	rBV2	146093	491561	24.36%	2.886%
18	4.246	996	997	1002	rVB	831	358	0.02%	0.002%
19	4.342	1009	1027	1063	rBV	327717	830270	41.14%	4.875%
20	4.616	1110	1112	1116	rVB3	508	282	0.01%	0.002%
21	4.657	1120	1125	1129	rBV3	538	571	0.03%	0.003%
22	4.725	1142	1146	1148	rBV2	534	444	0.02%	0.003%
23	4.783	1160	1164	1166	rVV2	451	323	0.02%	0.002%
24	4.812	1170	1173	1177	rVB3	383	287	0.01%	0.002%
25	4.838	1177	1181	1184	rBV2	495	501	0.02%	0.003%
26	4.931	1203	1210	1213	rBV4	406	470	0.02%	0.003%
27	5.040	1227	1244	1279	rBV2	770714	2017958	100.00%	11.848%
28	5.397	1351	1355	1356	rBV2	631	378	0.02%	0.002%
29	5.612	1409	1422	1454	rBV	673107	1394375	69.10%	8.187%
30	5.911	1502	1515	1529	rBV8	11255	27968	1.39%	0.164%
31	5.973	1532	1534	1539	rVB4	985	637	0.03%	0.004%
32	6.066	1549	1563	1592	rBV	443625	924440	45.81%	5.428%
33	6.419	1671	1673	1677	rVB2	805	485	0.02%	0.003%
34	6.445	1677	1681	1683	rBV3	425	324	0.02%	0.002%
35	6.593	1725	1727	1733	rVB2	270	236	0.01%	0.001%
36	6.622	1733	1736	1741	rBV2	334	253	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027160.D
 Acq On : 02 Aug 2022 09:16
 Operator : SY/MD
 Sample : N3880-17DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUH1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.657	1741	1747	1749	rBV3	682	665	0.03%	0.004%
38	6.747	1773	1775	1778	rVV4	411	319	0.02%	0.002%
39	6.825	1794	1799	1802	rVB3	453	394	0.02%	0.002%
40	6.982	1834	1848	1871	rBV	217995	407112	20.17%	2.390%
41	7.191	1910	1913	1915	rBV2	591	444	0.02%	0.003%
42	7.226	1921	1924	1926	rBV3	433	241	0.01%	0.001%
43	7.262	1934	1935	1938	rBV3	475	232	0.01%	0.001%
44	7.313	1939	1951	1987	rVV	866526	1549445	76.78%	9.097%
45	7.619	2035	2046	2066	rBV	154254	275993	13.68%	1.620%
46	7.844	2114	2116	2122	rVB3	597	482	0.02%	0.003%
47	7.905	2133	2135	2138	rVB	415	239	0.01%	0.001%
48	7.972	2140	2156	2182	rBV	788520	1338252	66.32%	7.857%
49	8.088	2182	2192	2235	rVV	454853	876450	43.43%	5.146%
50	8.410	2290	2292	2296	rVB3	607	439	0.02%	0.003%
51	8.448	2301	2304	2308	rVB3	436	286	0.01%	0.002%
52	8.548	2332	2335	2342	rVB3	352	308	0.02%	0.002%
53	8.606	2351	2353	2356	rBV4	426	270	0.01%	0.002%
54	8.696	2377	2381	2384	rBV3	268	296	0.01%	0.002%
55	8.850	2416	2429	2463	rBV	1045619	1710141	84.75%	10.041%
56	9.075	2497	2499	2505	rVB2	603	419	0.02%	0.002%
57	9.188	2529	2534	2544	rVB6	1922	3012	0.15%	0.018%
58	9.622	2666	2669	2674	rVB2	298	259	0.01%	0.002%
59	9.664	2678	2682	2684	rBV	409	246	0.01%	0.001%
60	9.709	2690	2696	2700	rBV	215	251	0.01%	0.001%
61	9.770	2712	2715	2718	rBV	397	235	0.01%	0.001%
62	9.805	2722	2726	2730	rVB3	373	312	0.02%	0.002%
63	9.857	2739	2742	2745	rVB3	444	296	0.01%	0.002%
64	10.214	2839	2853	2881	rBV	682925	1063363	52.70%	6.243%
65	10.361	2896	2899	2901	rBV3	461	297	0.01%	0.002%
66	10.648	2985	2988	2992	rVB2	597	483	0.02%	0.003%
67	10.670	2992	2995	2996	rBV2	543	255	0.01%	0.001%
68	10.844	3046	3049	3051	rBV	392	248	0.01%	0.001%
69	10.889	3059	3063	3064	rBV2	573	383	0.02%	0.002%
70	10.969	3085	3088	3091	rBV2	336	251	0.01%	0.001%
71	11.008	3097	3100	3105	rBV3	224	236	0.01%	0.001%
72	11.088	3122	3125	3127	rBV2	488	288	0.01%	0.002%
73	11.130	3135	3138	3141	rBV2	385	260	0.01%	0.002%
74	11.165	3144	3149	3152	rBV3	393	374	0.02%	0.002%
75	11.246	3163	3174	3197	rBV	962711	1486058	73.64%	8.725%
76	11.548	3260	3268	3272	rBV5	669	951	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027160.D
 Acq On : 02 Aug 2022 09:16
 Operator : SY/MD
 Sample : N3880-17DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUH1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	11.622	3279	3291	3315	rBV	877487	1388286	68.80%	8.151%
78	11.840	3357	3359	3364	rVB2	444	275	0.01%	0.002%
79	11.937	3387	3389	3393	rBV3	391	273	0.01%	0.002%
80	12.802	3656	3658	3662	rVV3	418	260	0.01%	0.002%
81	12.995	3714	3718	3721	rBV2	343	300	0.01%	0.002%
82	13.172	3770	3773	3779	rVB3	549	605	0.03%	0.004%
83	13.271	3801	3804	3807	rBV	631	479	0.02%	0.003%
84	13.329	3819	3822	3824	rBV	426	288	0.01%	0.002%
85	13.390	3839	3841	3844	rVB2	497	232	0.01%	0.001%
86	13.480	3867	3869	3871	rBV2	392	233	0.01%	0.001%
87	13.519	3877	3881	3886	rBV3	822	760	0.04%	0.004%
88	13.651	3919	3922	3924	rBV2	539	340	0.02%	0.002%
89	13.725	3941	3945	3948	rBV3	369	304	0.02%	0.002%
90	13.744	3948	3951	3955	rBV2	823	711	0.04%	0.004%
91	13.779	3959	3962	3966	rBV3	434	419	0.02%	0.002%
92	14.223	4098	4100	4109	rBV4	539	464	0.02%	0.003%
93	14.506	4186	4188	4192	rVV3	609	377	0.02%	0.002%
94	14.689	4243	4245	4249	rBV4	461	261	0.01%	0.002%
95	14.834	4288	4290	4294	rBV4	549	431	0.02%	0.003%
96	14.921	4314	4317	4318	rBV2	565	287	0.01%	0.002%
97	14.975	4332	4334	4337	rBV3	764	408	0.02%	0.002%
98	15.181	4397	4398	4400	rBV	797	227	0.01%	0.001%
99	15.409	4467	4469	4475	rVB6	727	395	0.02%	0.002%
100	15.509	4498	4500	4501	rBV	835	344	0.02%	0.002%




Sum of corrected areas: 17031576

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027160.D
Acq On : 02 Aug 2022 09:16
Operator : SY/MD
Sample : N3880-17DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUH1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

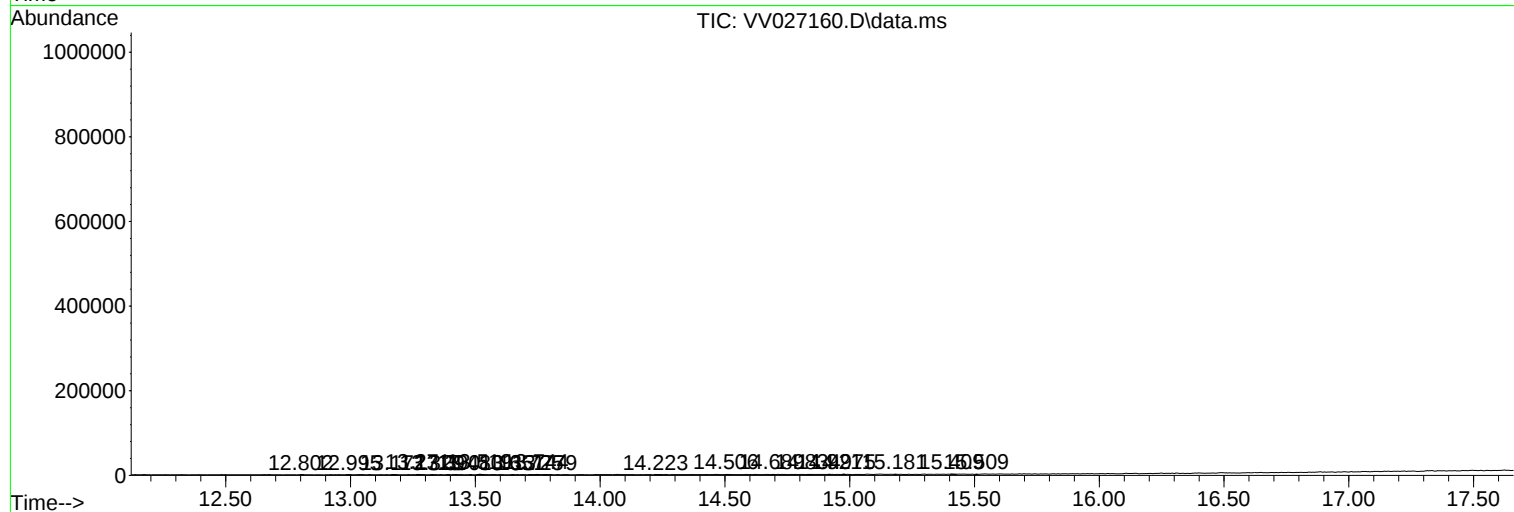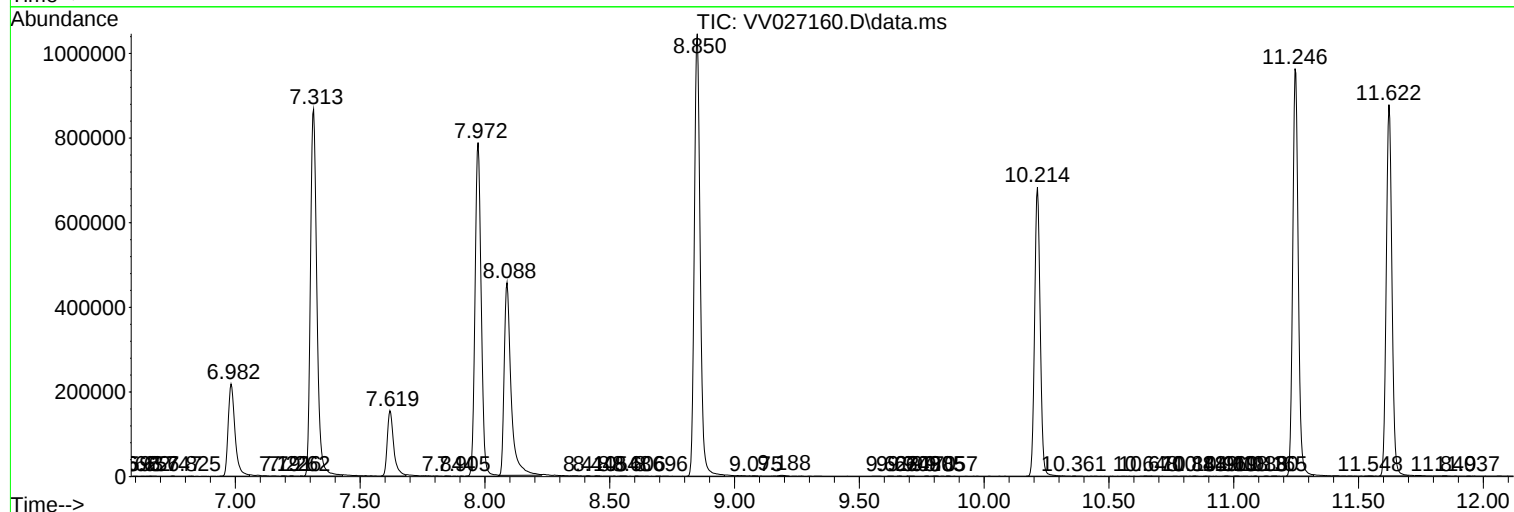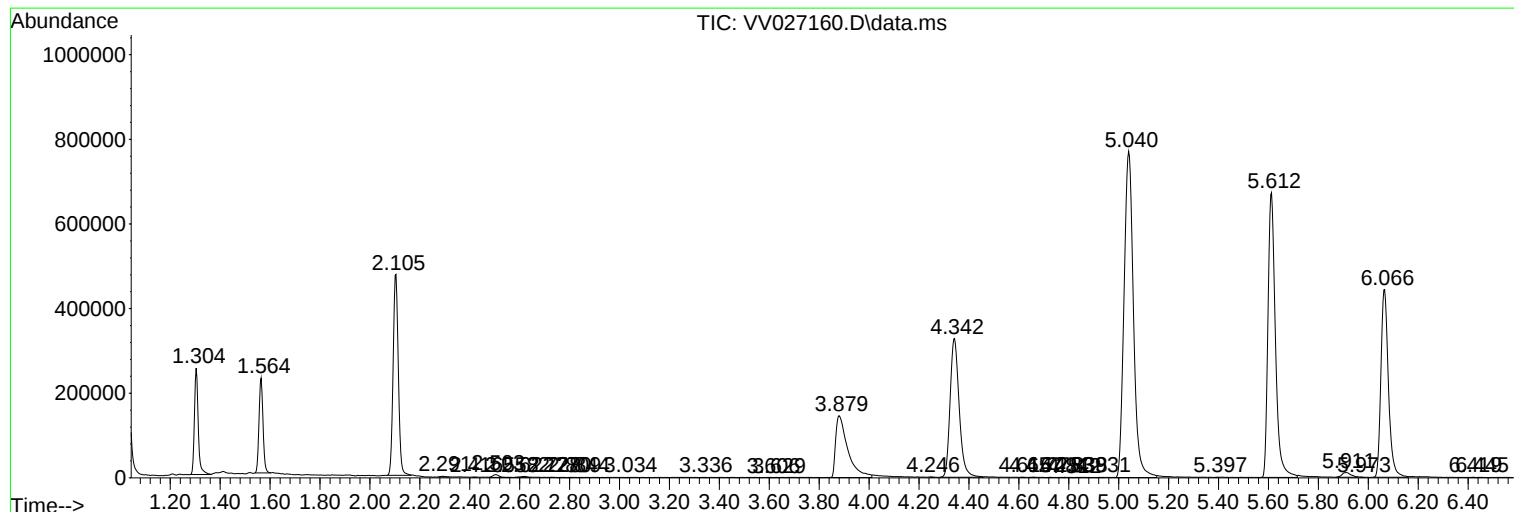

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027160.D
Acq On : 02 Aug 2022 09:16
Operator : SY/MD
Sample : N3880-17DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUH1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027160.D
Acq On : 02 Aug 2022 09:16
Operator : SY/MD
Sample : N3880-17DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUH1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc