

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027163.D
 Acq On : 02 Aug 2022 10:39
 Operator : SY/MD
 Sample : VIBLK266
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK266

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027163.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	34	rVB	40396	41327	1.84%	0.242%
2	1.304	76	82	102	rVB	327724	343205	15.27%	2.008%
3	1.565	156	163	175	rBV	267436	295739	13.16%	1.730%
4	2.105	322	331	343	rBV	555404	777680	34.60%	4.550%
5	2.812	550	551	554	rBV	458	136	0.01%	0.001%
6	2.883	570	573	574	rBV	360	213	0.01%	0.001%
7	3.008	610	612	613	rBV	310	126	0.01%	0.001%
8	3.146	651	655	656	rBV2	221	182	0.01%	0.001%
9	3.243	678	685	687	rBV3	406	373	0.02%	0.002%
10	3.275	692	695	699	rBV2	436	348	0.02%	0.002%
11	3.320	704	709	712	rBV2	407	365	0.02%	0.002%
12	3.417	735	739	741	rBV2	314	194	0.01%	0.001%
13	3.478	752	758	760	rBV2	561	368	0.02%	0.002%
14	3.507	765	767	770	rBV	221	130	0.01%	0.001%
15	3.590	791	793	797	rBV2	320	266	0.01%	0.002%
16	3.635	803	807	814	rVB2	327	372	0.02%	0.002%
17	3.680	818	821	824	rBV	368	227	0.01%	0.001%
18	3.716	830	832	837	rBV2	326	279	0.01%	0.002%
19	3.744	837	841	847	rVV3	333	401	0.02%	0.002%
20	3.880	870	883	926	rBV2	173187	576811	25.66%	3.374%
21	4.343	1011	1027	1059	rBV	362032	914450	40.69%	5.350%
22	4.744	1150	1152	1155	rBV	367	306	0.01%	0.002%
23	4.822	1172	1176	1178	rBV2	252	172	0.01%	0.001%
24	4.931	1206	1210	1211	rVB2	245	129	0.01%	0.001%
25	4.944	1211	1214	1219	rBV3	444	430	0.02%	0.003%
26	4.966	1219	1221	1225	rVB2	310	150	0.01%	0.001%
27	5.043	1228	1245	1293	rBV2	842483	2247571	100.00%	13.149%
28	5.404	1355	1357	1361	rBV3	822	647	0.03%	0.004%
29	5.458	1372	1374	1377	rVB2	413	174	0.01%	0.001%
30	5.551	1401	1403	1405	rVB2	372	143	0.01%	0.001%
31	5.613	1409	1422	1453	rBV	657944	1376849	61.26%	8.055%
32	6.066	1549	1563	1589	rBV	489733	1020572	45.41%	5.970%
33	6.365	1653	1656	1657	rBV2	705	411	0.02%	0.002%
34	6.490	1692	1695	1698	rBV2	202	177	0.01%	0.001%
35	6.526	1704	1706	1707	rBV	252	114	0.01%	0.001%
36	6.555	1713	1715	1717	rVB2	502	232	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027163.D
 Acq On : 02 Aug 2022 10:39
 Operator : SY/MD
 Sample : VIBLK266
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK266

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.587	1723	1725	1729	rVB	276	131	0.01%	0.001%
38	6.613	1729	1733	1737	rVB2	272	228	0.01%	0.001%
39	6.661	1745	1748	1752	rBV3	199	160	0.01%	0.001%
40	6.680	1752	1754	1757	rVB3	284	138	0.01%	0.001%
41	6.809	1791	1794	1797	rBV2	244	171	0.01%	0.001%
42	6.838	1800	1803	1806	rVB3	233	137	0.01%	0.001%
43	6.883	1813	1817	1819	rBV2	416	322	0.01%	0.002%
44	6.912	1819	1826	1833	rBV5	2536	3273	0.15%	0.019%
45	6.982	1838	1848	1877	rBV	242274	459115	20.43%	2.686%
46	7.220	1918	1922	1924	rBV3	589	435	0.02%	0.003%
47	7.313	1939	1951	1981	rBV	956708	1691365	75.25%	9.895%
48	7.619	2036	2046	2068	rBV	178604	316785	14.09%	1.853%
49	8.018	2161	2170	2182	rBV	29192	50879	2.26%	0.298%
50	8.088	2182	2192	2224	rBV	579263	1092410	48.60%	6.391%
51	8.600	2348	2351	2352	rBV	280	135	0.01%	0.001%
52	8.683	2373	2377	2379	rBV	368	229	0.01%	0.001%
53	8.744	2394	2396	2400	rVB	430	242	0.01%	0.001%
54	8.776	2404	2406	2409	rVB2	257	114	0.01%	0.001%
55	8.850	2417	2429	2451	rBV	1034981	1682458	74.86%	9.843%
56	9.098	2502	2506	2509	rBV4	470	462	0.02%	0.003%
57	9.153	2521	2523	2526	rBV2	544	350	0.02%	0.002%
58	9.239	2548	2550	2551	rBV2	478	156	0.01%	0.001%
59	9.317	2571	2574	2578	rVB3	380	315	0.01%	0.002%
60	9.346	2578	2583	2586	rBV3	413	387	0.02%	0.002%
61	9.374	2590	2592	2595	rVB	346	186	0.01%	0.001%
62	9.397	2595	2599	2604	rBV3	623	675	0.03%	0.004%
63	9.493	2625	2629	2632	rBV	442	363	0.02%	0.002%
64	9.535	2640	2642	2645	rVB2	373	172	0.01%	0.001%
65	9.555	2645	2648	2649	rBV	264	141	0.01%	0.001%
66	9.577	2653	2655	2657	rVB	297	134	0.01%	0.001%
67	9.593	2657	2660	2663	rBV2	335	264	0.01%	0.002%
68	9.641	2672	2675	2677	rBV2	309	223	0.01%	0.001%
69	9.693	2686	2691	2695	rBV2	346	431	0.02%	0.003%
70	9.731	2700	2703	2708	rVB2	340	283	0.01%	0.002%
71	9.757	2708	2711	2712	rBV	224	133	0.01%	0.001%
72	9.873	2744	2747	2749	rBV2	326	235	0.01%	0.001%
73	9.947	2768	2770	2773	rBV2	240	143	0.01%	0.001%
74	9.979	2777	2780	2782	rBV	291	195	0.01%	0.001%
75	10.021	2790	2793	2795	rBV2	225	142	0.01%	0.001%
76	10.072	2805	2809	2811	rBV2	216	142	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027163.D
 Acq On : 02 Aug 2022 10:39
 Operator : SY/MD
 Sample : VIBLK266
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK266

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	10.088	2811	2814	2821	rVB2	336	436	0.02%	0.003%
78	10.124	2821	2825	2828	rVB2	386	246	0.01%	0.001%
79	10.140	2828	2830	2833	rBV	272	179	0.01%	0.001%
80	10.214	2840	2853	2886	rBV	760127	1205784	53.65%	7.054%
81	10.423	2914	2918	2920	rVB3	324	217	0.01%	0.001%
82	10.436	2920	2922	2925	rBV	214	142	0.01%	0.001%
83	10.458	2926	2929	2934	rVB4	370	359	0.02%	0.002%
84	10.484	2935	2937	2941	rVB	379	222	0.01%	0.001%
85	10.506	2941	2944	2946	rBV2	406	197	0.01%	0.001%
86	10.526	2947	2950	2953	rBV	414	276	0.01%	0.002%
87	10.728	3009	3013	3014	rBV	378	248	0.01%	0.001%
88	10.847	3046	3050	3057	rVB4	737	804	0.04%	0.005%
89	10.950	3079	3082	3085	rBV2	213	192	0.01%	0.001%
90	11.008	3098	3100	3105	rVB2	618	405	0.02%	0.002%
91	11.037	3105	3109	3111	rBV3	325	184	0.01%	0.001%
92	11.095	3123	3127	3131	rVB2	313	317	0.01%	0.002%
93	11.117	3131	3134	3137	rBV	356	181	0.01%	0.001%
94	11.178	3146	3153	3162	rBV6	2135	3052	0.14%	0.018%
95	11.246	3163	3174	3201	rBV	917307	1442525	64.18%	8.439%
96	11.622	3279	3291	3317	rBV	960061	1529327	68.04%	8.947%
97	11.921	3381	3384	3385	rBV2	421	262	0.01%	0.002%
98	12.995	3715	3718	3720	rBV2	361	244	0.01%	0.001%
99	13.664	3920	3926	3929	rBV4	504	548	0.02%	0.003%
100	13.902	3997	4000	4009	rVB4	1428	1786	0.08%	0.010%




Sum of corrected areas: 17093661

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027163.D
Acq On : 02 Aug 2022 10:39
Operator : SY/MD
Sample : VIBLK266
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK266

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

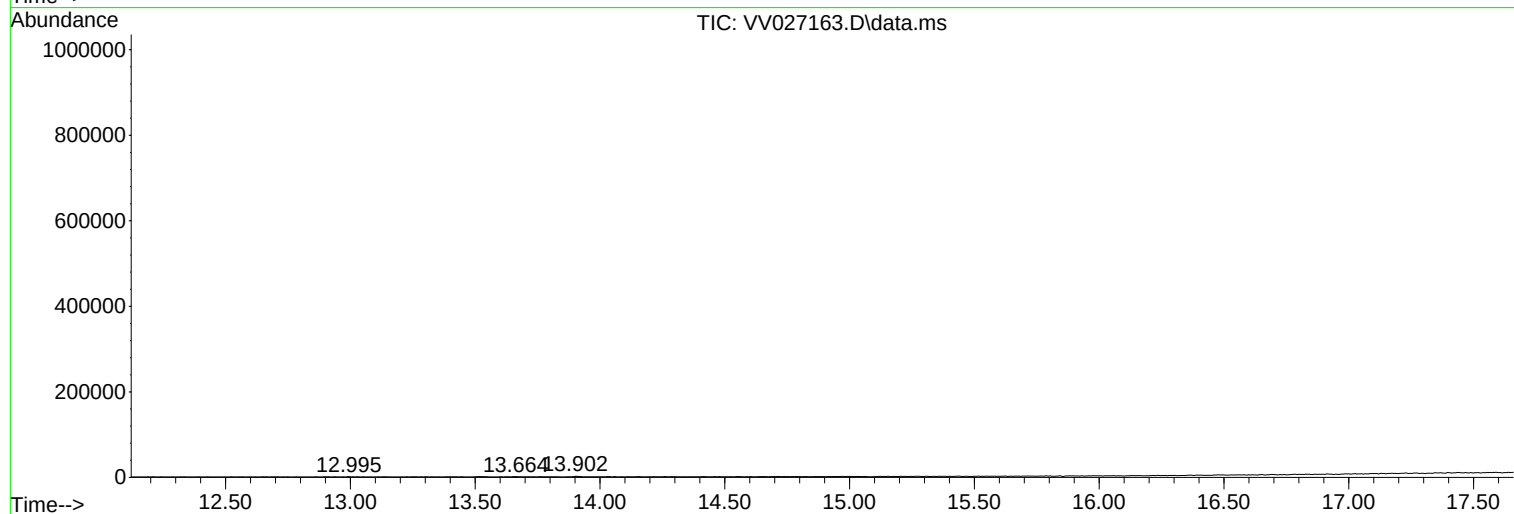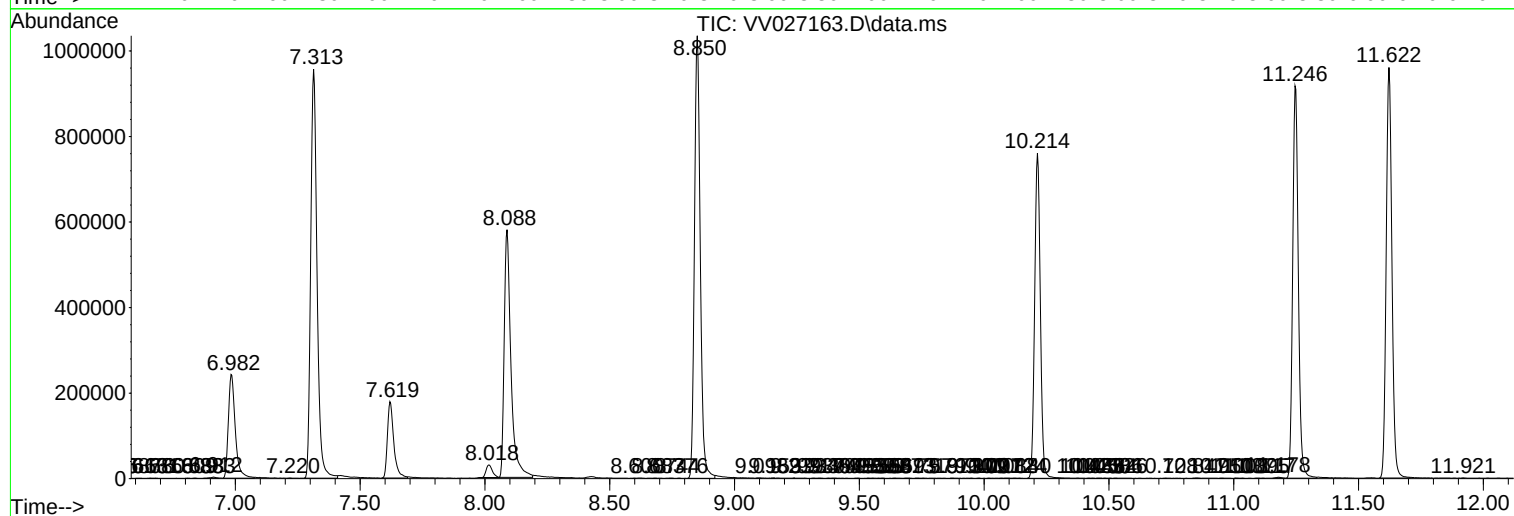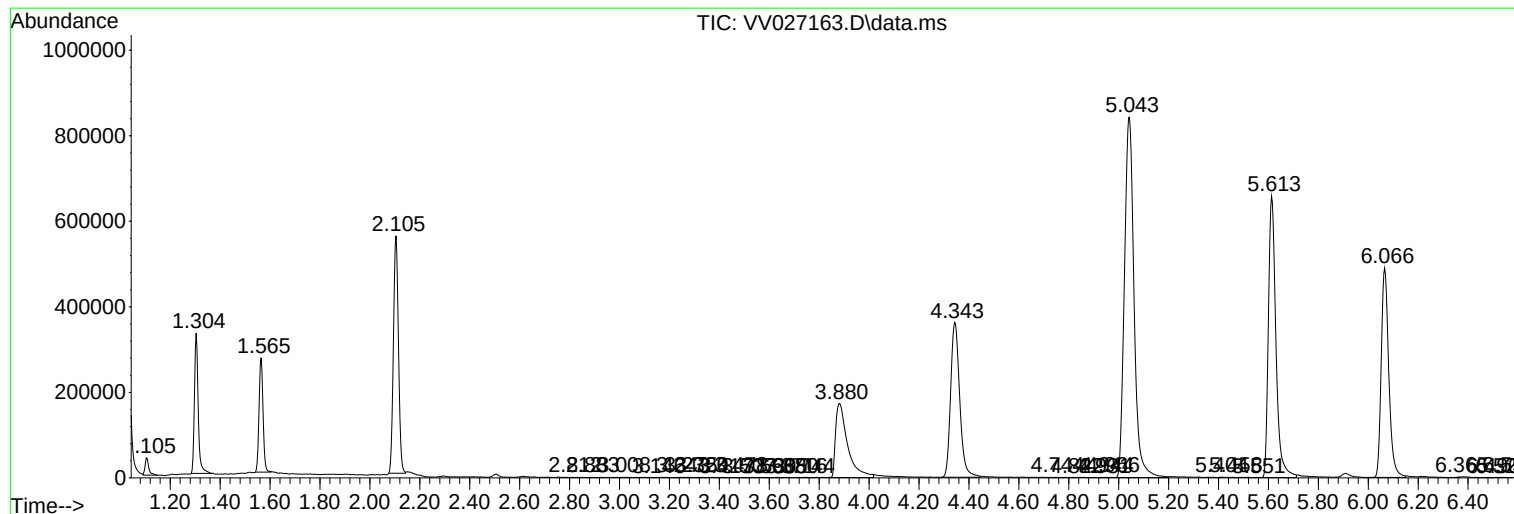

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027163.D
Acq On : 02 Aug 2022 10:39
Operator : SY/MD
Sample : VIBLK266
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK266

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027163.D
Acq On : 02 Aug 2022 10:39
Operator : SY/MD
Sample : VIBLK266
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK266

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------