

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027165.D
 Acq On : 02 Aug 2022 12:09
 Operator : SY/MD
 Sample : VIBLK267
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK267

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027165.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	103	rBV	276364	295262	14.19%	1.882%
2	1.561	156	162	173	rVB	237249	263068	12.65%	1.677%
3	2.101	321	330	343	rBV	490829	685718	32.96%	4.372%
4	2.503	445	455	465	rBV3	8041	13894	0.67%	0.089%
5	2.616	480	490	496	rBV5	2816	5105	0.25%	0.033%
6	2.992	603	607	610	rBV3	382	314	0.02%	0.002%
7	3.018	613	615	620	rBV2	288	262	0.01%	0.002%
8	3.162	659	660	666	rVB2	439	278	0.01%	0.002%
9	3.201	666	672	677	rBV2	283	366	0.02%	0.002%
10	3.230	677	681	683	rBV2	210	148	0.01%	0.001%
11	3.314	701	707	711	rBV2	387	465	0.02%	0.003%
12	3.333	711	713	715	rVB	359	169	0.01%	0.001%
13	3.365	721	723	727	rVB2	215	174	0.01%	0.001%
14	3.391	727	731	734	rBV2	253	238	0.01%	0.002%
15	3.423	735	741	744	rBV	238	299	0.01%	0.002%
16	3.497	761	764	769	rVB3	322	226	0.01%	0.001%
17	3.523	769	772	776	rVB2	311	224	0.01%	0.001%
18	3.548	776	780	783	rBV2	392	328	0.02%	0.002%
19	3.593	791	794	800	rVB3	270	293	0.01%	0.002%
20	3.625	800	804	808	rBV	417	326	0.02%	0.002%
21	3.793	849	856	860	rBV3	345	399	0.02%	0.003%
22	3.876	869	882	934	rBV2	171613	586010	28.17%	3.736%
23	4.339	1010	1026	1070	rBV	338240	848931	40.81%	5.412%
24	4.683	1131	1133	1135	rVB	390	147	0.01%	0.001%
25	4.712	1138	1142	1145	rVB2	490	351	0.02%	0.002%
26	4.828	1174	1178	1180	rBV2	337	264	0.01%	0.002%
27	4.844	1181	1183	1189	rVB4	574	500	0.02%	0.003%
28	4.873	1189	1192	1194	rBV2	577	362	0.02%	0.002%
29	4.908	1202	1203	1207	rBV	515	152	0.01%	0.001%
30	5.037	1225	1243	1283	rBV2	790326	2080384	100.00%	13.263%
31	5.368	1344	1346	1349	rBV2	335	260	0.01%	0.002%
32	5.455	1370	1373	1374	rBV2	297	180	0.01%	0.001%
33	5.522	1389	1394	1399	rBV3	450	434	0.02%	0.003%
34	5.609	1409	1421	1465	rBV	590808	1239403	59.58%	7.902%
35	5.902	1503	1512	1529	rBV3	9493	21164	1.02%	0.135%
36	5.995	1539	1541	1542	rBV	298	133	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027165.D
 Acq On : 02 Aug 2022 12:09
 Operator : SY/MD
 Sample : VIBLK267
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK267

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.063	1548	1562	1594	rBV	465213	963997	46.34%	6.146%
38	6.284	1629	1631	1637	rVB4	785	531	0.03%	0.003%
39	6.336	1645	1647	1649	rBV	466	240	0.01%	0.002%
40	6.371	1657	1658	1660	rBV	302	121	0.01%	0.001%
41	6.410	1668	1670	1673	rVB2	307	144	0.01%	0.001%
42	6.471	1686	1689	1693	rBV	246	192	0.01%	0.001%
43	6.497	1693	1697	1698	rBV	169	132	0.01%	0.001%
44	6.532	1706	1708	1710	rVB	301	119	0.01%	0.001%
45	6.567	1715	1719	1723	rBV2	300	256	0.01%	0.002%
46	6.629	1735	1738	1742	rVB2	237	163	0.01%	0.001%
47	6.651	1742	1745	1748	rBV	305	259	0.01%	0.002%
48	6.696	1755	1759	1760	rBV2	490	207	0.01%	0.001%
49	6.709	1761	1763	1764	rVV	375	169	0.01%	0.001%
50	6.731	1768	1770	1773	rVB	327	171	0.01%	0.001%
51	6.760	1773	1779	1780	rBV2	359	220	0.01%	0.001%
52	6.796	1784	1790	1796	rBV3	198	172	0.01%	0.001%
53	6.879	1812	1816	1821	rVB2	156	132	0.01%	0.001%
54	6.902	1821	1823	1824	rBV	308	125	0.01%	0.001%
55	6.911	1824	1826	1830	rBV	238	146	0.01%	0.001%
56	6.982	1836	1848	1876	rBV	226156	427868	20.57%	2.728%
57	7.310	1938	1950	1978	rBV	835509	1507269	72.45%	9.609%
58	7.616	2036	2045	2067	rBV	158548	289718	13.93%	1.847%
59	7.857	2117	2120	2122	rBV2	482	287	0.01%	0.002%
60	7.905	2133	2135	2140	rVB4	390	205	0.01%	0.001%
61	7.931	2140	2143	2146	rVB3	796	507	0.02%	0.003%
62	7.947	2146	2148	2149	rBV	339	162	0.01%	0.001%
63	7.956	2149	2151	2153	rBV2	326	161	0.01%	0.001%
64	8.018	2161	2170	2181	rBV3	8802	16467	0.79%	0.105%
65	8.085	2181	2191	2228	rBV	541338	1033592	49.68%	6.589%
66	8.423	2289	2296	2305	rVB2	5209	7955	0.38%	0.051%
67	8.673	2369	2374	2375	rBV2	372	276	0.01%	0.002%
68	8.741	2391	2395	2396	rBV2	418	284	0.01%	0.002%
69	8.847	2414	2428	2465	rBV	920612	1535631	73.81%	9.790%
70	9.188	2532	2534	2540	rBV3	377	237	0.01%	0.002%
71	9.246	2550	2552	2557	rVB2	360	262	0.01%	0.002%
72	9.387	2593	2596	2598	rBV2	223	135	0.01%	0.001%
73	9.426	2606	2608	2611	rBV2	394	257	0.01%	0.002%
74	9.506	2630	2633	2635	rVV3	300	162	0.01%	0.001%
75	9.522	2635	2638	2640	rBV	310	209	0.01%	0.001%
76	9.599	2658	2662	2664	rBV	195	167	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027165.D
 Acq On : 02 Aug 2022 12:09
 Operator : SY/MD
 Sample : VIBLK267
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK267

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	9.628	2670	2671	2675	rBV	210	115	0.01%	0.001%
78	9.715	2695	2698	2707	rVB2	390	559	0.03%	0.004%
79	9.754	2707	2710	2712	rBV2	194	134	0.01%	0.001%
80	9.943	2766	2769	2773	rBV	284	270	0.01%	0.002%
81	10.037	2797	2798	2803	rVB3	270	132	0.01%	0.001%
82	10.146	2829	2832	2834	rVB2	253	119	0.01%	0.001%
83	10.214	2840	2853	2878	rBV	736870	1157650	55.65%	7.380%
84	10.394	2907	2909	2914	rVB2	519	301	0.01%	0.002%
85	10.490	2935	2939	2942	rBV3	466	332	0.02%	0.002%
86	10.648	2986	2988	2989	rBV	237	115	0.01%	0.001%
87	10.831	3041	3045	3049	rBV2	572	628	0.03%	0.004%
88	10.853	3050	3052	3055	rVB3	464	279	0.01%	0.002%
89	10.931	3074	3076	3079	rBV2	327	206	0.01%	0.001%
90	11.124	3133	3136	3138	rBV2	221	131	0.01%	0.001%
91	11.178	3148	3153	3162	rBV5	1025	1136	0.05%	0.007%
92	11.246	3162	3174	3196	rBV	829957	1301505	62.56%	8.297%
93	11.622	3279	3291	3313	rBV	894569	1384197	66.54%	8.825%
94	12.098	3435	3439	3441	rBV2	473	360	0.02%	0.002%
95	12.651	3606	3611	3612	rBV2	447	415	0.02%	0.003%
96	12.911	3690	3692	3695	rBV2	332	241	0.01%	0.002%
97	12.959	3705	3707	3711	rBV2	350	277	0.01%	0.002%
98	13.024	3725	3727	3732	rVB2	429	254	0.01%	0.002%
99	13.323	3818	3820	3823	rBV2	616	379	0.02%	0.002%
100	13.844	3980	3982	3985	rBV2	448	301	0.01%	0.002%




Sum of corrected areas: 15685574

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027165.D
Acq On : 02 Aug 2022 12:09
Operator : SY/MD
Sample : VIBLK267
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK267

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

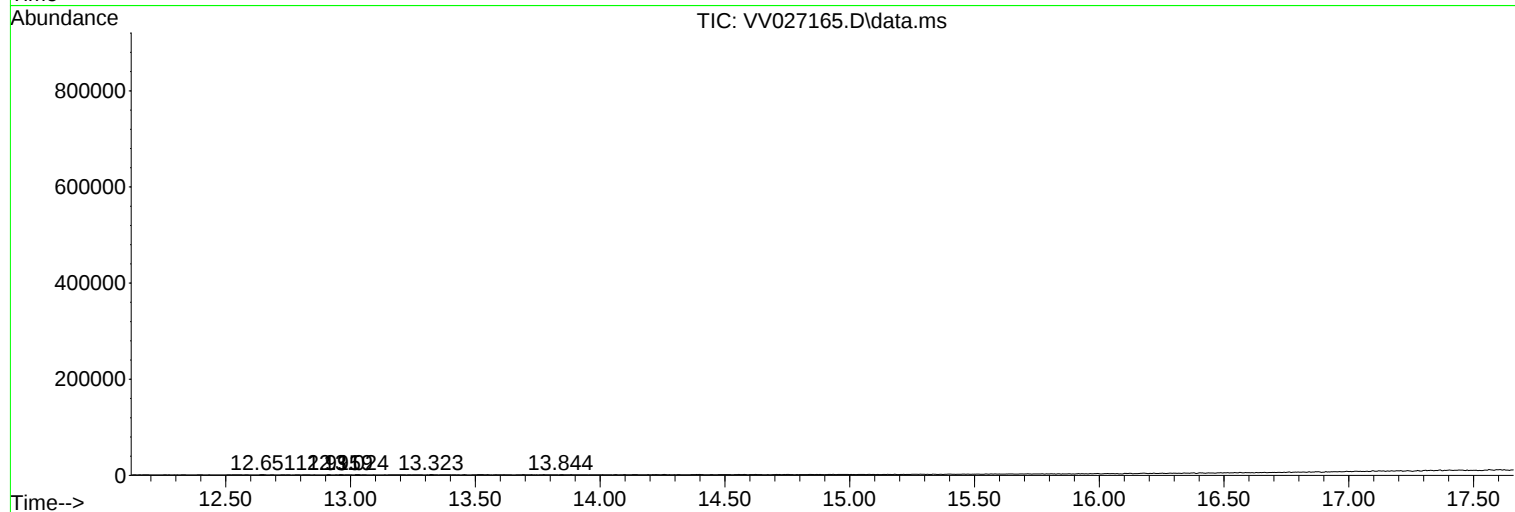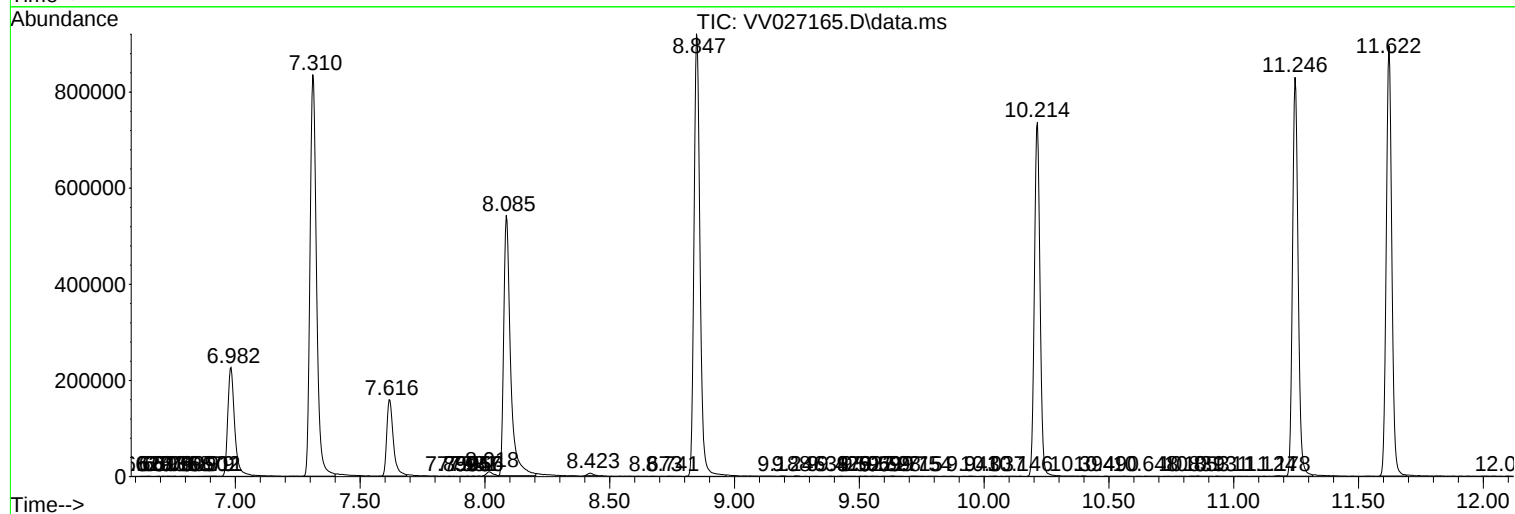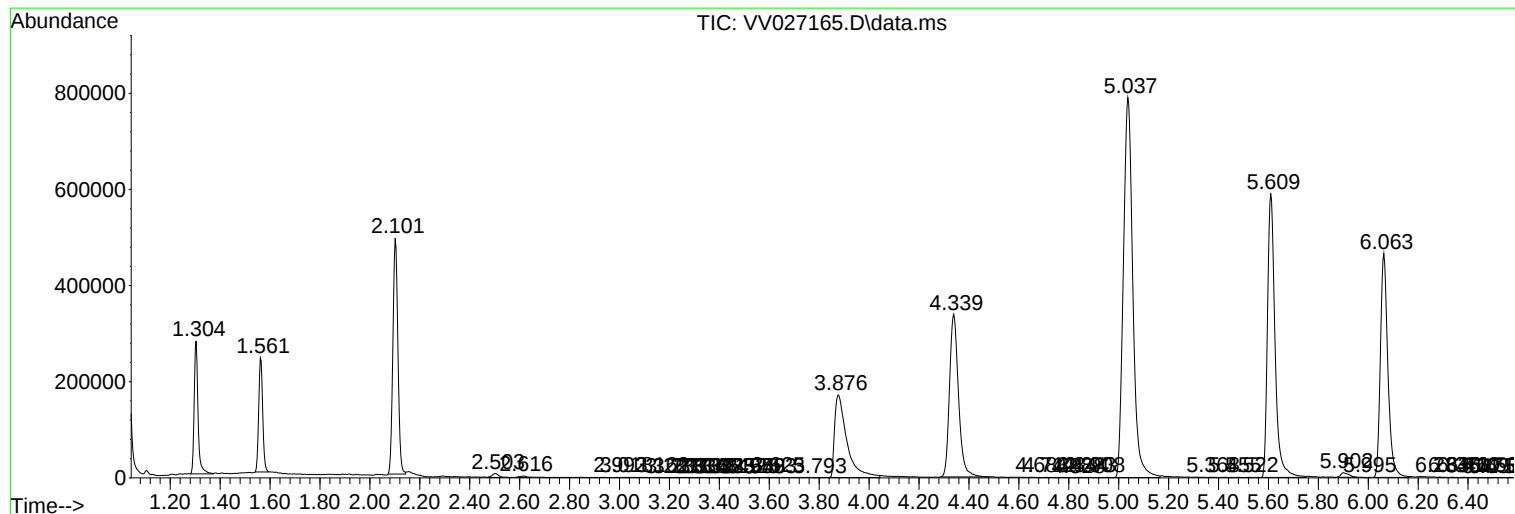

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027165.D
Acq On : 02 Aug 2022 12:09
Operator : SY/MD
Sample : VIBLK267
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK267

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027165.D
Acq On : 02 Aug 2022 12:09
Operator : SY/MD
Sample : VIBLK267
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK267

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------