

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027167.D
 Acq On : 02 Aug 2022 13:00
 Operator : SY/MD
 Sample : N3897-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027167.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	101	rBV	306464	328177	15.39%	2.029%
2	1.561	155	162	173	rVB	255706	281362	13.19%	1.739%
3	2.101	320	330	344	rBV	532651	754760	35.39%	4.666%
4	2.503	448	455	466	rVB2	6618	10108	0.47%	0.062%
5	2.616	485	490	493	rBV3	442	403	0.02%	0.002%
6	2.687	507	512	517	rBV3	414	484	0.02%	0.003%
7	2.854	561	564	568	rBV3	489	344	0.02%	0.002%
8	2.941	586	591	594	rBV2	314	281	0.01%	0.002%
9	3.182	661	666	668	rBV2	271	291	0.01%	0.002%
10	3.246	682	686	688	rBV2	335	255	0.01%	0.002%
11	3.320	706	709	712	rBV	492	367	0.02%	0.002%
12	3.876	870	882	925	rBV	162102	483889	22.69%	2.991%
13	4.227	987	991	993	rBV2	782	558	0.03%	0.003%
14	4.342	1009	1027	1068	rBV	352392	882616	41.38%	5.456%
15	4.519	1080	1082	1087	rVB4	447	313	0.01%	0.002%
16	4.593	1102	1105	1110	rVB3	445	291	0.01%	0.002%
17	4.706	1136	1140	1145	rBV	417	460	0.02%	0.003%
18	4.748	1150	1153	1158	rVB	344	287	0.01%	0.002%
19	4.854	1182	1186	1189	rBV2	527	312	0.01%	0.002%
20	4.879	1189	1194	1197	rVB4	404	319	0.01%	0.002%
21	4.960	1215	1219	1221	rBV	429	259	0.01%	0.002%
22	5.040	1227	1244	1285	rBV2	814716	2132784	100.00%	13.185%
23	5.468	1373	1377	1380	rBV2	438	352	0.02%	0.002%
24	5.519	1389	1393	1399	rVB2	497	491	0.02%	0.003%
25	5.551	1399	1403	1405	rBV3	368	266	0.01%	0.002%
26	5.612	1407	1422	1462	rBV	624440	1301872	61.04%	8.048%
27	5.870	1500	1502	1504	rBV2	656	381	0.02%	0.002%
28	5.908	1504	1514	1530	rVV4	9573	20440	0.96%	0.126%
29	6.066	1547	1563	1593	rBV	470320	983178	46.10%	6.078%
30	6.204	1604	1606	1609	rBV4	718	545	0.03%	0.003%
31	6.284	1629	1631	1634	rVB2	644	317	0.01%	0.002%
32	6.320	1640	1642	1645	rVB2	556	291	0.01%	0.002%
33	6.352	1646	1652	1655	rBV2	483	414	0.02%	0.003%
34	6.374	1655	1659	1663	rVB3	648	473	0.02%	0.003%
35	6.490	1689	1695	1699	rBV3	366	382	0.02%	0.002%
36	6.522	1701	1705	1707	rVB	441	272	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027167.D
 Acq On : 02 Aug 2022 13:00
 Operator : SY/MD
 Sample : N3897-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.619	1733	1735	1742	rVV2	468	302	0.01%	0.002%
38	6.712	1761	1764	1768	rVB2	324	258	0.01%	0.002%
39	6.850	1801	1807	1810	rBV3	259	338	0.02%	0.002%
40	6.927	1826	1831	1835	rBV	416	253	0.01%	0.002%
41	6.982	1835	1848	1883	rBV	227853	433946	20.35%	2.683%
42	7.313	1939	1951	1984	rBV	901878	1605036	75.26%	9.922%
43	7.619	2036	2046	2074	rBV	164441	296833	13.92%	1.835%
44	7.812	2104	2106	2113	rVB4	632	542	0.03%	0.003%
45	7.841	2113	2115	2117	rVB2	561	256	0.01%	0.002%
46	7.944	2142	2147	2151	rBV2	583	489	0.02%	0.003%
47	7.985	2154	2160	2164	rBV6	1206	1371	0.06%	0.008%
48	8.027	2164	2173	2175	rBV6	1898	2203	0.10%	0.014%
49	8.088	2182	2192	2234	rBV	569198	1092264	51.21%	6.752%
50	8.358	2273	2276	2277	rBV3	542	268	0.01%	0.002%
51	8.464	2307	2309	2313	rBV	459	450	0.02%	0.003%
52	8.661	2365	2370	2372	rBV3	405	345	0.02%	0.002%
53	8.850	2417	2429	2456	rBV	976177	1587728	74.44%	9.815%
54	9.046	2489	2490	2493	rVB2	668	291	0.01%	0.002%
55	9.075	2493	2499	2502	rBV4	552	549	0.03%	0.003%
56	9.140	2516	2519	2521	rBV3	414	278	0.01%	0.002%
57	9.223	2543	2545	2550	rVB3	335	253	0.01%	0.002%
58	9.288	2561	2565	2569	rBV3	437	334	0.02%	0.002%
59	9.326	2575	2577	2579	rVV2	416	274	0.01%	0.002%
60	9.397	2597	2599	2603	rVB3	504	302	0.01%	0.002%
61	9.429	2603	2609	2612	rBV3	422	428	0.02%	0.003%
62	9.638	2670	2674	2678	rVB3	449	444	0.02%	0.003%
63	9.706	2689	2695	2697	rBV3	368	374	0.02%	0.002%
64	9.760	2707	2712	2718	rVB2	364	502	0.02%	0.003%
65	9.982	2777	2781	2785	rBV2	295	258	0.01%	0.002%
66	10.008	2785	2789	2793	rVB3	387	286	0.01%	0.002%
67	10.133	2820	2828	2829	rBV2	384	373	0.02%	0.002%
68	10.214	2840	2853	2877	rBV	752010	1173202	55.01%	7.253%
69	10.583	2964	2968	2971	rBV2	448	474	0.02%	0.003%
70	10.689	2998	3001	3007	rVB2	374	299	0.01%	0.002%
71	10.718	3007	3010	3013	rBV2	341	271	0.01%	0.002%
72	10.857	3047	3053	3061	rBV4	637	716	0.03%	0.004%
73	11.120	3133	3135	3141	rBV2	268	290	0.01%	0.002%
74	11.197	3154	3159	3163	rBV3	551	591	0.03%	0.004%
75	11.246	3163	3174	3198	rBV	857868	1339722	62.82%	8.282%
76	11.548	3260	3268	3276	rBV8	2067	3648	0.17%	0.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027167.D
 Acq On : 02 Aug 2022 13:00
 Operator : SY/MD
 Sample : N3897-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	11.622	3279	3291	3315	rBV	911212	1431338	67.11%	8.849%
78	11.863	3364	3366	3370	rBV2	443	343	0.02%	0.002%
79	12.033	3416	3419	3421	rBV	351	274	0.01%	0.002%
80	12.088	3433	3436	3441	rVB3	390	369	0.02%	0.002%
81	12.786	3649	3653	3656	rBV2	258	253	0.01%	0.002%
82	13.111	3751	3754	3757	rBV	362	285	0.01%	0.002%
83	13.162	3768	3770	3774	rVB3	494	348	0.02%	0.002%
84	13.278	3804	3806	3815	rVB3	398	390	0.02%	0.002%
85	13.320	3815	3819	3820	rBV2	509	345	0.02%	0.002%
86	13.368	3831	3834	3838	rVB3	502	338	0.02%	0.002%
87	13.397	3838	3843	3846	rBV2	606	393	0.02%	0.002%
88	13.422	3846	3851	3855	rBV3	706	730	0.03%	0.005%
89	13.464	3859	3864	3865	rBV2	404	326	0.02%	0.002%
90	13.580	3897	3900	3906	rBV3	555	426	0.02%	0.003%
91	13.670	3926	3928	3932	rVB	455	265	0.01%	0.002%
92	13.856	3984	3986	3988	rBV	462	294	0.01%	0.002%
93	14.053	4044	4047	4050	rBV3	437	317	0.01%	0.002%
94	14.072	4051	4053	4058	rVB3	407	266	0.01%	0.002%
95	14.114	4064	4066	4070	rBV3	386	295	0.01%	0.002%
96	14.181	4084	4087	4089	rBV2	443	291	0.01%	0.002%
97	14.323	4127	4131	4133	rBV	510	409	0.02%	0.003%
98	14.889	4304	4307	4313	rVB4	739	644	0.03%	0.004%
99	15.027	4346	4350	4353	rBV2	797	617	0.03%	0.004%
100	15.487	4489	4493	4495	rVB4	913	595	0.03%	0.004%




Sum of corrected areas: 16175786

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027167.D
Acq On : 02 Aug 2022 13:00
Operator : SY/MD
Sample : N3897-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

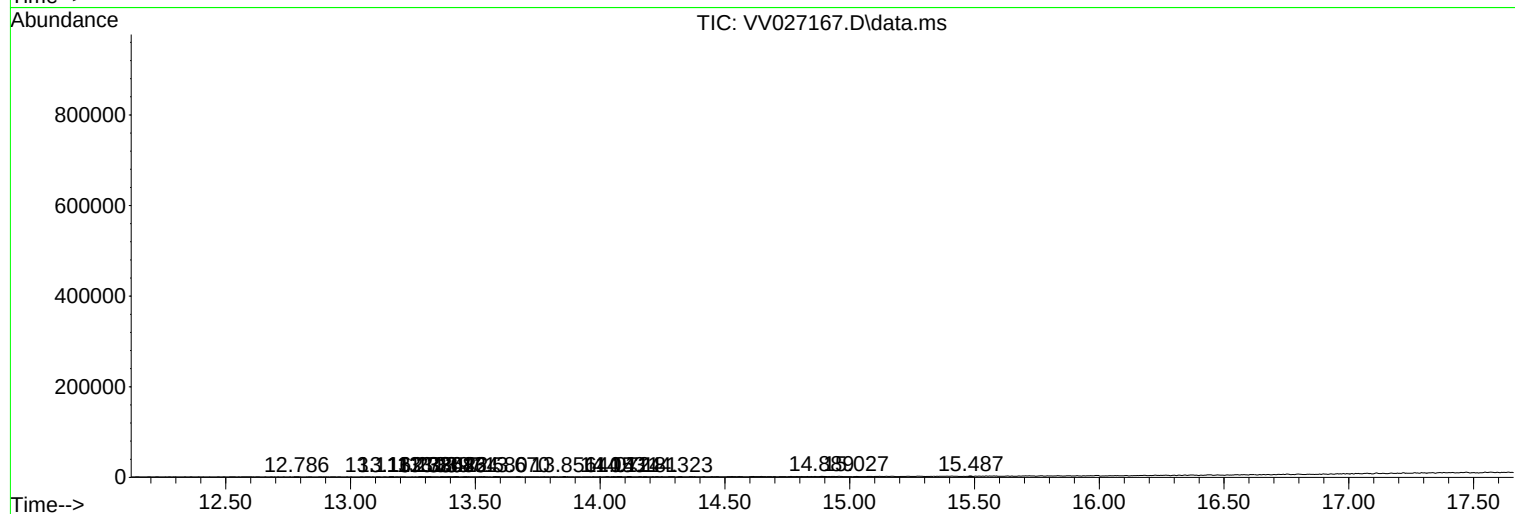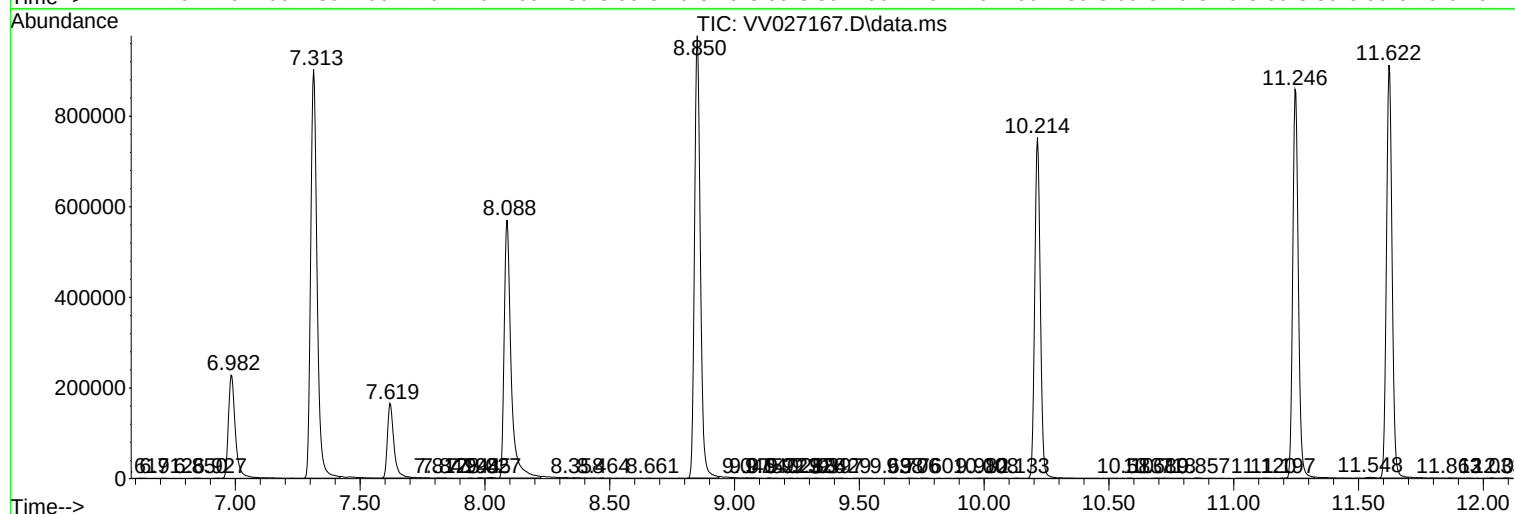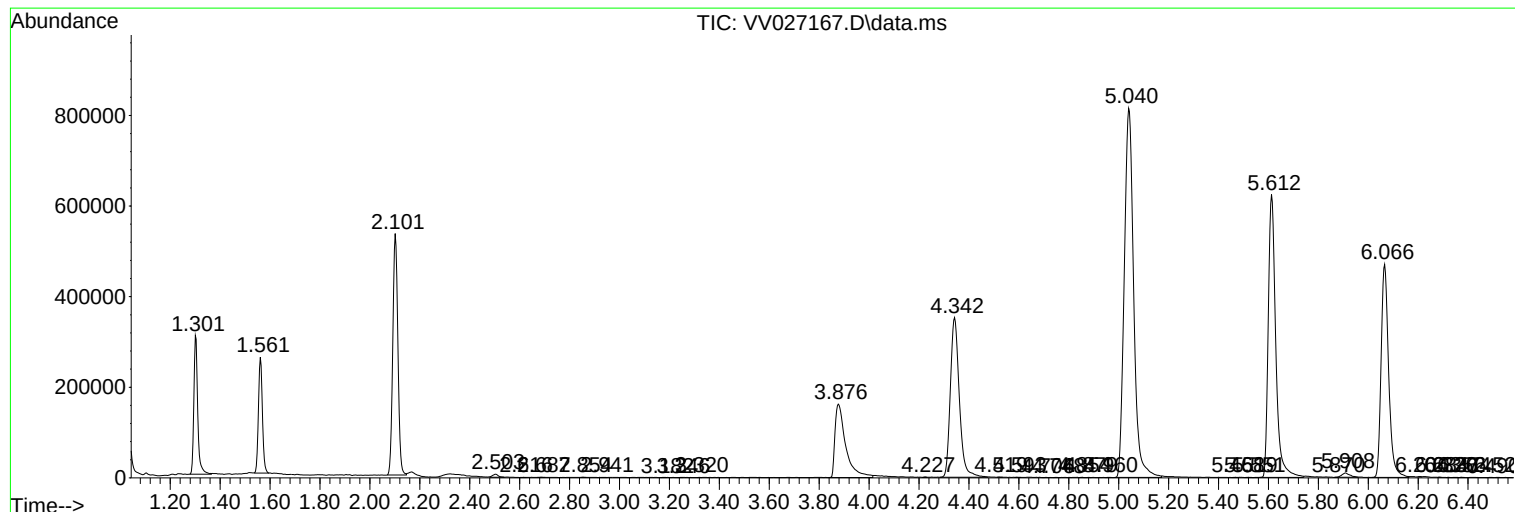

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027167.D
Acq On : 02 Aug 2022 13:00
Operator : SY/MD
Sample : N3897-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027167.D
Acq On : 02 Aug 2022 13:00
Operator : SY/MD
Sample : N3897-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc