

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027168.D
 Acq On : 02 Aug 2022 13:25
 Operator : SY/MD
 Sample : N3899-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027168.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	104	rVB	308288	325238	14.86%	1.957%
2	1.564	156	163	175	rVB	252224	286719	13.10%	1.726%
3	2.105	321	331	345	rBV	538004	763011	34.85%	4.592%
4	2.796	544	546	550	rBV3	233	189	0.01%	0.001%
5	2.857	561	565	567	rVV	315	231	0.01%	0.001%
6	2.963	595	598	600	rBV	273	199	0.01%	0.001%
7	3.066	627	630	632	rBV	328	222	0.01%	0.001%
8	3.105	637	642	643	rBV	357	216	0.01%	0.001%
9	3.175	660	664	667	rBV3	294	221	0.01%	0.001%
10	3.240	682	684	687	rBV2	175	105	0.00%	0.001%
11	3.268	691	693	696	rBV2	202	148	0.01%	0.001%
12	3.297	700	702	707	rBV2	180	175	0.01%	0.001%
13	3.394	729	732	735	rBV	284	213	0.01%	0.001%
14	3.416	735	739	742	rVB2	337	257	0.01%	0.002%
15	3.436	742	745	747	rBV	278	158	0.01%	0.001%
16	3.452	747	750	752	rBV	245	174	0.01%	0.001%
17	3.558	781	783	786	rBV	196	127	0.01%	0.001%
18	3.584	786	791	793	rBV2	241	193	0.01%	0.001%
19	3.625	801	804	806	rBV2	284	217	0.01%	0.001%
20	3.677	817	820	822	rBV2	259	197	0.01%	0.001%
21	3.738	833	839	841	rBV2	311	272	0.01%	0.002%
22	3.751	841	843	845	rBV	349	209	0.01%	0.001%
23	3.818	861	864	866	rBV	279	165	0.01%	0.001%
24	3.879	872	883	918	rBV	172378	495477	22.63%	2.982%
25	4.342	1011	1027	1075	rBV	356090	904203	41.30%	5.442%
26	4.706	1135	1140	1143	rBV2	278	247	0.01%	0.001%
27	4.796	1164	1168	1172	rBV2	466	306	0.01%	0.002%
28	4.838	1178	1181	1182	rBV2	181	98	0.00%	0.001%
29	4.854	1182	1186	1189	rVV2	302	320	0.01%	0.002%
30	4.886	1192	1196	1203	rVB3	318	339	0.02%	0.002%
31	4.915	1203	1205	1207	rBV2	149	100	0.00%	0.001%
32	5.043	1228	1245	1290	rBV2	824655	2189277	100.00%	13.176%
33	5.516	1390	1392	1395	rBV2	266	135	0.01%	0.001%
34	5.551	1400	1403	1405	rBV2	490	311	0.01%	0.002%
35	5.612	1411	1422	1457	rBV	646585	1352332	61.77%	8.139%
36	5.908	1504	1514	1528	rBV3	10159	21638	0.99%	0.130%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027168.D
 Acq On : 02 Aug 2022 13:25
 Operator : SY/MD
 Sample : N3899-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.066	1550	1563	1595	rBV	488705	1008902	46.08%	6.072%
38	6.329	1643	1645	1647	rBV3	349	116	0.01%	0.001%
39	6.371	1655	1658	1660	rBV	216	135	0.01%	0.001%
40	6.387	1660	1663	1664	rVB2	382	186	0.01%	0.001%
41	6.397	1665	1666	1669	rBV2	222	109	0.00%	0.001%
42	6.416	1669	1672	1674	rBV2	278	179	0.01%	0.001%
43	6.452	1680	1683	1684	rBV2	516	251	0.01%	0.002%
44	6.487	1690	1694	1699	rBV2	386	406	0.02%	0.002%
45	6.574	1717	1721	1722	rBV2	269	183	0.01%	0.001%
46	6.702	1757	1761	1762	rBV	246	107	0.00%	0.001%
47	6.744	1767	1774	1775	rBV3	185	152	0.01%	0.001%
48	6.757	1775	1778	1784	rBV2	281	272	0.01%	0.002%
49	6.889	1816	1819	1821	rBV	254	137	0.01%	0.001%
50	6.915	1825	1827	1829	rVB	734	217	0.01%	0.001%
51	6.985	1834	1849	1874	rBV	233618	441737	20.18%	2.659%
52	7.262	1933	1935	1938	rBV2	420	295	0.01%	0.002%
53	7.313	1939	1951	1990	rBV	902413	1642068	75.01%	9.883%
54	7.619	2036	2046	2067	rBV	168159	301474	13.77%	1.814%
55	7.860	2117	2121	2127	rVB3	1022	1123	0.05%	0.007%
56	7.921	2137	2140	2142	rBV	438	310	0.01%	0.002%
57	7.979	2153	2158	2159	rBV2	788	498	0.02%	0.003%
58	8.030	2166	2174	2177	rBV5	1544	2075	0.09%	0.012%
59	8.088	2182	2192	2228	rBV	589858	1139730	52.06%	6.859%
60	8.522	2325	2327	2333	rVB	441	278	0.01%	0.002%
61	8.722	2384	2389	2394	rBV4	575	807	0.04%	0.005%
62	8.805	2413	2415	2417	rBV2	302	176	0.01%	0.001%
63	8.850	2417	2429	2459	rBV	1022326	1663820	76.00%	10.014%
64	9.207	2536	2540	2542	rBV4	551	425	0.02%	0.003%
65	9.236	2546	2549	2550	rBV	258	119	0.01%	0.001%
66	9.278	2560	2562	2567	rVB2	362	275	0.01%	0.002%
67	9.320	2572	2575	2577	rBV2	458	287	0.01%	0.002%
68	9.352	2582	2585	2588	rBV2	327	220	0.01%	0.001%
69	9.452	2613	2616	2621	rVB2	356	335	0.02%	0.002%
70	9.506	2630	2633	2634	rBV	277	167	0.01%	0.001%
71	9.686	2684	2689	2692	rBV2	263	239	0.01%	0.001%
72	9.702	2692	2694	2697	rBV2	231	150	0.01%	0.001%
73	9.744	2703	2707	2710	rVB2	260	186	0.01%	0.001%
74	9.763	2710	2713	2717	rBV2	260	230	0.01%	0.001%
75	9.792	2717	2722	2727	rVV3	317	353	0.02%	0.002%
76	9.876	2742	2748	2751	rBV3	332	337	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027168.D
 Acq On : 02 Aug 2022 13:25
 Operator : SY/MD
 Sample : N3899-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	9.905	2754	2757	2759	rBV2	256	157	0.01%	0.001%
78	9.992	2780	2784	2788	rVV2	451	363	0.02%	0.002%
79	10.124	2823	2825	2831	rBV2	324	239	0.01%	0.001%
80	10.214	2840	2853	2880	rBV	772925	1209173	55.23%	7.277%
81	10.448	2924	2926	2929	rBV3	318	214	0.01%	0.001%
82	10.599	2964	2973	2977	rBV3	578	990	0.05%	0.006%
83	10.651	2986	2989	2992	rBV	338	200	0.01%	0.001%
84	10.751	3016	3020	3023	rVB2	324	286	0.01%	0.002%
85	10.773	3023	3027	3028	rBV2	363	180	0.01%	0.001%
86	10.783	3028	3030	3035	rVB3	287	143	0.01%	0.001%
87	10.821	3039	3042	3044	rBV2	456	267	0.01%	0.002%
88	10.857	3049	3053	3056	rVV2	482	392	0.02%	0.002%
89	10.895	3062	3065	3067	rBV2	399	227	0.01%	0.001%
90	10.940	3077	3079	3083	rVB	236	141	0.01%	0.001%
91	11.066	3115	3118	3121	rBV	179	102	0.00%	0.001%
92	11.091	3121	3126	3128	rBV3	383	376	0.02%	0.002%
93	11.249	3163	3175	3204	rBV	878222	1387049	63.36%	8.348%
94	11.545	3261	3267	3272	rBV5	1278	1791	0.08%	0.011%
95	11.622	3279	3291	3319	rBV	923118	1459484	66.67%	8.784%
96	11.950	3390	3393	3395	rBV2	480	279	0.01%	0.002%
97	12.008	3408	3411	3414	rBV2	570	375	0.02%	0.002%
98	12.484	3557	3559	3560	rBV2	291	120	0.01%	0.001%
99	12.792	3653	3655	3657	rBV2	394	163	0.01%	0.001%
100	13.500	3873	3875	3877	rBV3	403	216	0.01%	0.001%




Sum of corrected areas: 16615632

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027168.D
Acq On : 02 Aug 2022 13:25
Operator : SY/MD
Sample : N3899-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

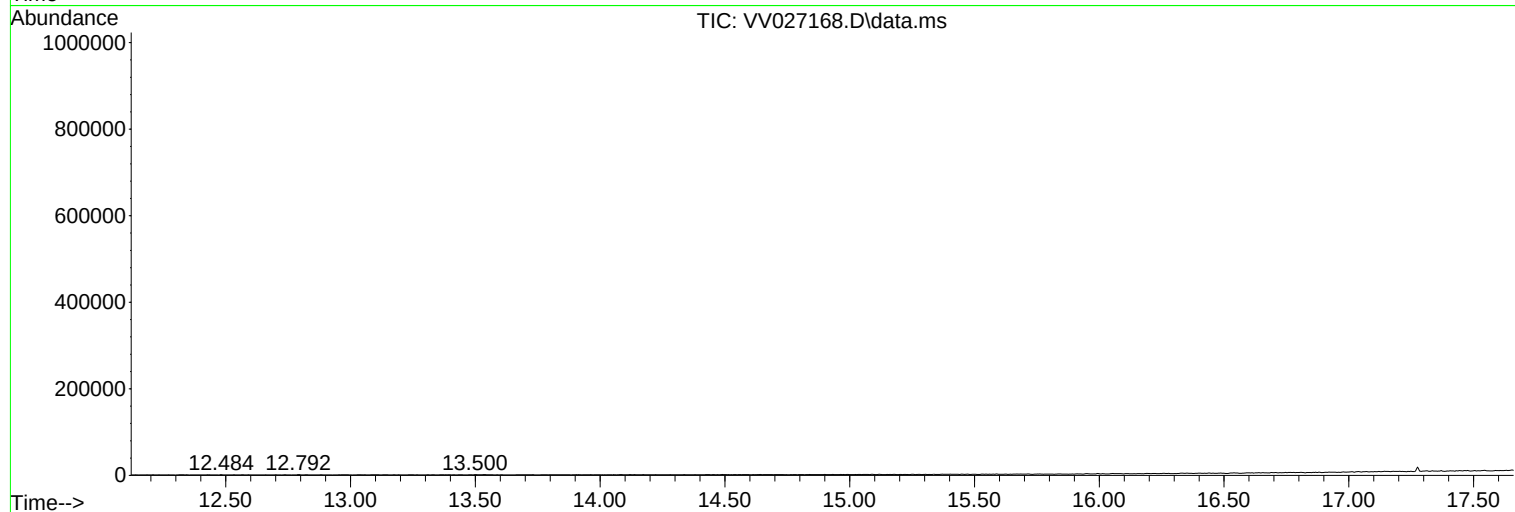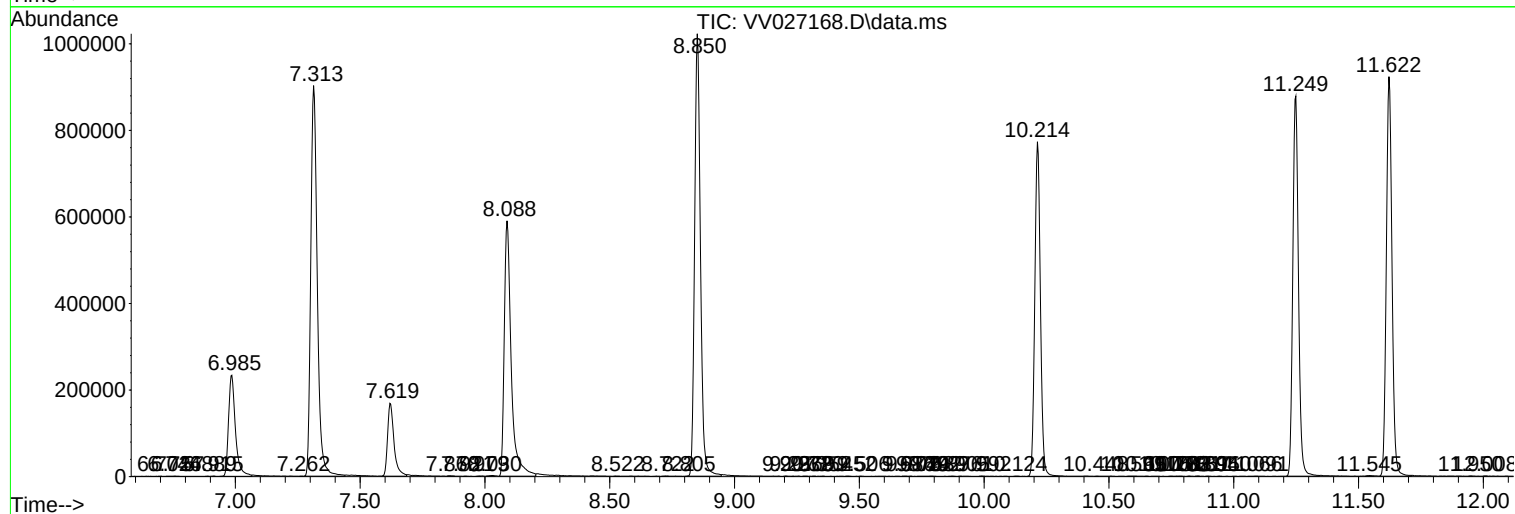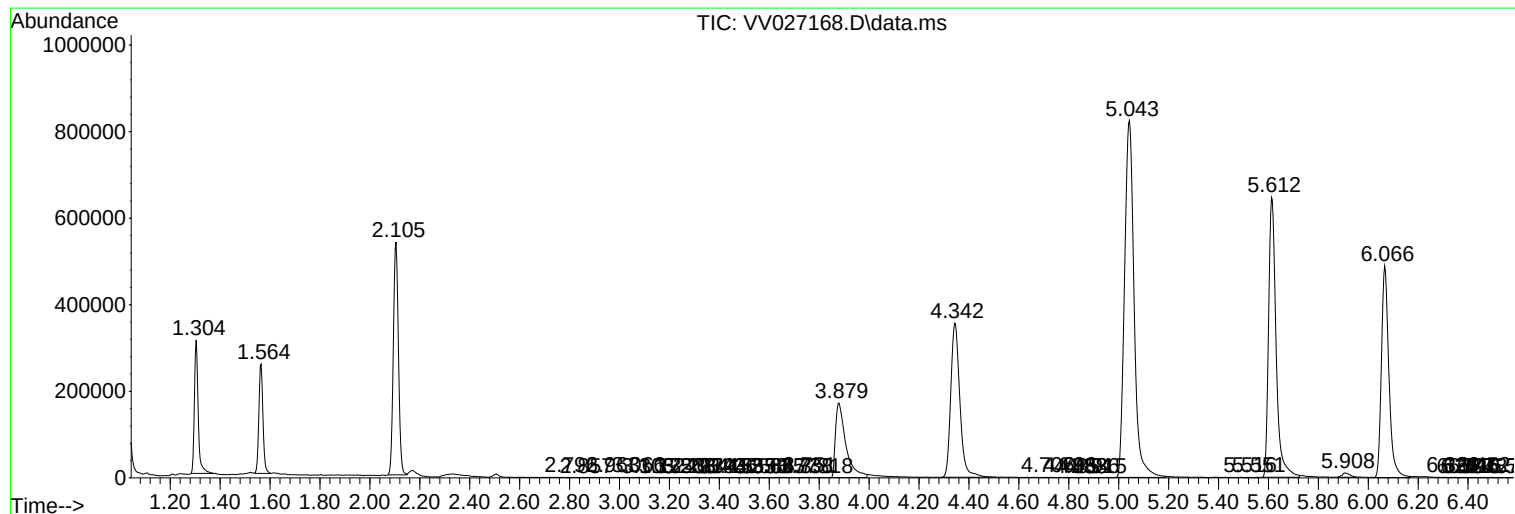

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027168.D
Acq On : 02 Aug 2022 13:25
Operator : SY/MD
Sample : N3899-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027168.D
Acq On : 02 Aug 2022 13:25
Operator : SY/MD
Sample : N3899-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------