

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027169.D
 Acq On : 02 Aug 2022 13:49
 Operator : SY/MD
 Sample : N3880-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027169.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rBV	312931	332875	15.32%	2.027%
2	1.565	156	163	177	rVB	257211	289025	13.30%	1.760%
3	2.105	321	331	345	rBV	533607	759978	34.97%	4.628%
4	2.893	574	576	579	rBV3	389	224	0.01%	0.001%
5	2.947	591	593	597	rVB2	411	276	0.01%	0.002%
6	3.015	611	614	616	rBV	308	185	0.01%	0.001%
7	3.156	656	658	660	rBV2	195	67	0.00%	0.000%
8	3.233	679	682	685	rVB	397	236	0.01%	0.001%
9	3.256	686	689	692	rVV2	221	137	0.01%	0.001%
10	3.307	702	705	708	rBV	250	161	0.01%	0.001%
11	3.323	708	710	712	rBV2	106	46	0.00%	0.000%
12	3.339	712	715	718	rBV2	304	218	0.01%	0.001%
13	3.410	735	737	739	rBV2	382	158	0.01%	0.001%
14	3.468	752	755	757	rBV2	317	181	0.01%	0.001%
15	3.513	763	769	770	rBV	283	229	0.01%	0.001%
16	3.523	770	772	776	rVB2	303	200	0.01%	0.001%
17	3.568	783	786	791	rVV3	298	177	0.01%	0.001%
18	3.600	793	796	802	rVB2	303	262	0.01%	0.002%
19	3.725	833	835	840	rVB3	414	339	0.02%	0.002%
20	3.751	840	843	847	rVB2	163	135	0.01%	0.001%
21	3.777	847	851	852	rBV	294	167	0.01%	0.001%
22	3.880	873	883	936	rBV	167758	502205	23.11%	3.058%
23	4.343	1012	1027	1075	rVB	354141	891857	41.04%	5.431%
24	4.680	1127	1132	1134	rBV2	476	423	0.02%	0.003%
25	4.725	1143	1146	1149	rBV3	201	164	0.01%	0.001%
26	4.777	1158	1162	1166	rBV3	480	413	0.02%	0.003%
27	4.899	1197	1200	1203	rBV	211	120	0.01%	0.001%
28	4.921	1206	1207	1208	rVB	254	49	0.00%	0.000%
29	4.931	1208	1210	1212	rBV2	56	31	0.00%	0.000%
30	4.947	1212	1215	1219	rBV	426	257	0.01%	0.002%
31	4.979	1224	1225	1226	rVB	205	39	0.00%	0.000%
32	5.044	1227	1245	1289	rBV2	825684	2173347	100.00%	13.235%
33	5.552	1399	1403	1410	rBV3	772	1121	0.05%	0.007%
34	5.613	1410	1422	1471	rVV	632439	1337603	61.55%	8.146%
35	5.908	1506	1514	1526	rBV3	8387	16165	0.74%	0.098%
36	6.066	1549	1563	1594	rBV	487025	1000386	46.03%	6.092%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027169.D
 Acq On : 02 Aug 2022 13:49
 Operator : SY/MD
 Sample : N3880-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.326	1643	1644	1646	rBV2	469	203	0.01%	0.001%
38	6.429	1671	1676	1681	rBV4	433	519	0.02%	0.003%
39	6.478	1689	1691	1693	rBV2	85	39	0.00%	0.000%
40	6.494	1693	1696	1697	rBV	145	93	0.00%	0.001%
41	6.580	1719	1723	1726	rBV2	276	201	0.01%	0.001%
42	6.597	1726	1728	1729	rBV	358	109	0.01%	0.001%
43	6.651	1743	1745	1750	rVB2	233	128	0.01%	0.001%
44	6.674	1750	1752	1754	rBV	198	92	0.00%	0.001%
45	6.693	1757	1758	1760	rBV	101	42	0.00%	0.000%
46	6.715	1762	1765	1767	rVB	268	140	0.01%	0.001%
47	6.793	1786	1789	1793	rVB2	211	150	0.01%	0.001%
48	6.828	1793	1800	1804	rBV2	403	329	0.02%	0.002%
49	6.851	1804	1807	1809	rVB2	245	121	0.01%	0.001%
50	6.863	1809	1811	1813	rBV	170	69	0.00%	0.000%
51	6.928	1828	1831	1834	rBV	276	162	0.01%	0.001%
52	6.986	1837	1849	1872	rBV	228300	434335	19.98%	2.645%
53	7.314	1939	1951	1998	rBV	907159	1631475	75.07%	9.935%
54	7.619	2036	2046	2075	rBV	166329	299210	13.77%	1.822%
55	7.879	2125	2127	2130	rVB2	436	241	0.01%	0.001%
56	7.924	2139	2141	2145	rBV3	330	268	0.01%	0.002%
57	7.941	2145	2146	2150	rBV2	332	265	0.01%	0.002%
58	8.031	2167	2174	2180	rBV4	1295	2055	0.09%	0.013%
59	8.088	2182	2192	2230	rBV	569549	1104540	50.82%	6.726%
60	8.494	2316	2318	2320	rBV3	371	163	0.01%	0.001%
61	8.622	2355	2358	2361	rVB3	671	373	0.02%	0.002%
62	8.699	2380	2382	2383	rBV3	380	152	0.01%	0.001%
63	8.793	2408	2411	2414	rBV2	303	229	0.01%	0.001%
64	8.850	2417	2429	2457	rBV	991562	1627815	74.90%	9.913%
65	9.259	2553	2556	2560	rBV2	418	267	0.01%	0.002%
66	9.285	2561	2564	2568	rBV2	438	372	0.02%	0.002%
67	9.333	2577	2579	2580	rVB	301	85	0.00%	0.001%
68	9.387	2594	2596	2598	rBV	247	95	0.00%	0.001%
69	9.465	2616	2620	2624	rBV3	264	223	0.01%	0.001%
70	9.484	2624	2626	2629	rBV2	313	246	0.01%	0.001%
71	9.600	2658	2662	2664	rBV2	342	258	0.01%	0.002%
72	9.638	2672	2674	2676	rBV	286	111	0.01%	0.001%
73	9.821	2729	2731	2734	rBV2	446	201	0.01%	0.001%
74	9.963	2772	2775	2779	rBV3	416	321	0.01%	0.002%
75	10.034	2794	2797	2802	rBV3	348	411	0.02%	0.003%
76	10.153	2831	2834	2837	rBV	344	243	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027169.D
Acq On : 02 Aug 2022 13:49
Operator : SY/MD
Sample : N3880-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M

Title : VOC Analysis

77	10.169	2837	2839	2840	rBV	153	48	0.00%	0.000%
78	10.214	2840	2853	2877	rBV	767602	1192741	54.88%	7.263%
79	10.455	2925	2928	2930	rBV2	308	200	0.01%	0.001%
80	10.838	3046	3047	3048	rBV	186	48	0.00%	0.000%
81	11.249	3163	3175	3204	rBV	864017	1360164	62.58%	8.283%
82	11.622	3279	3291	3317	rBV	921497	1452170	66.82%	8.843%




Sum of corrected areas: 16421178

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027169.D
Acq On : 02 Aug 2022 13:49
Operator : SY/MD
Sample : N3880-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

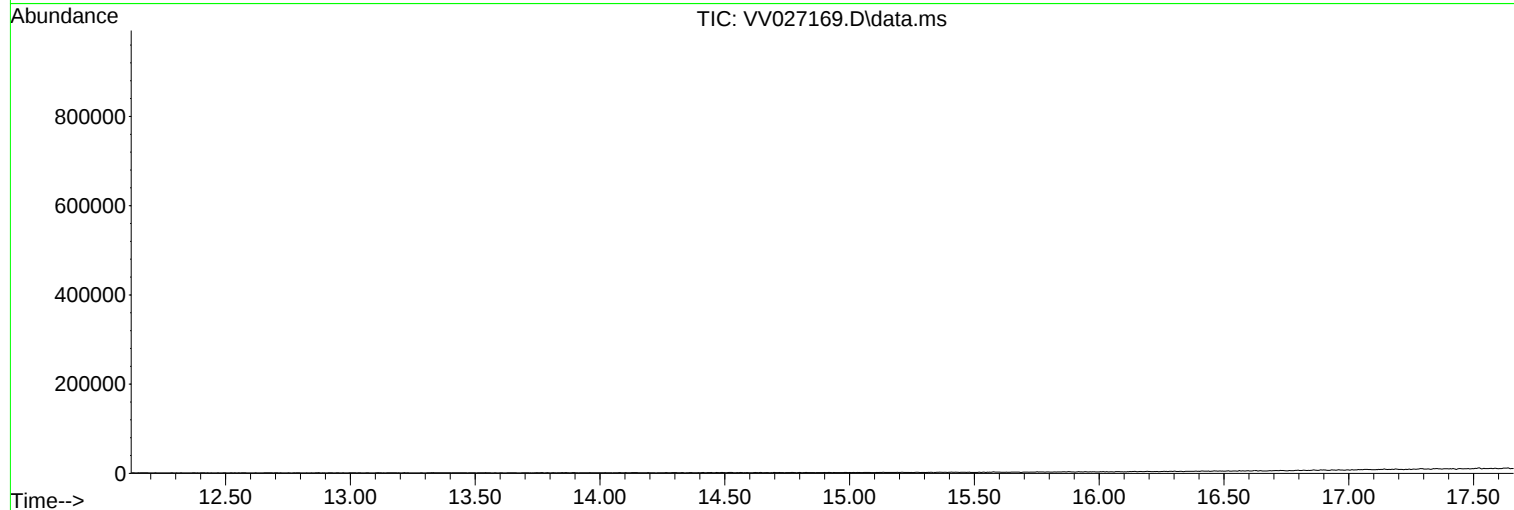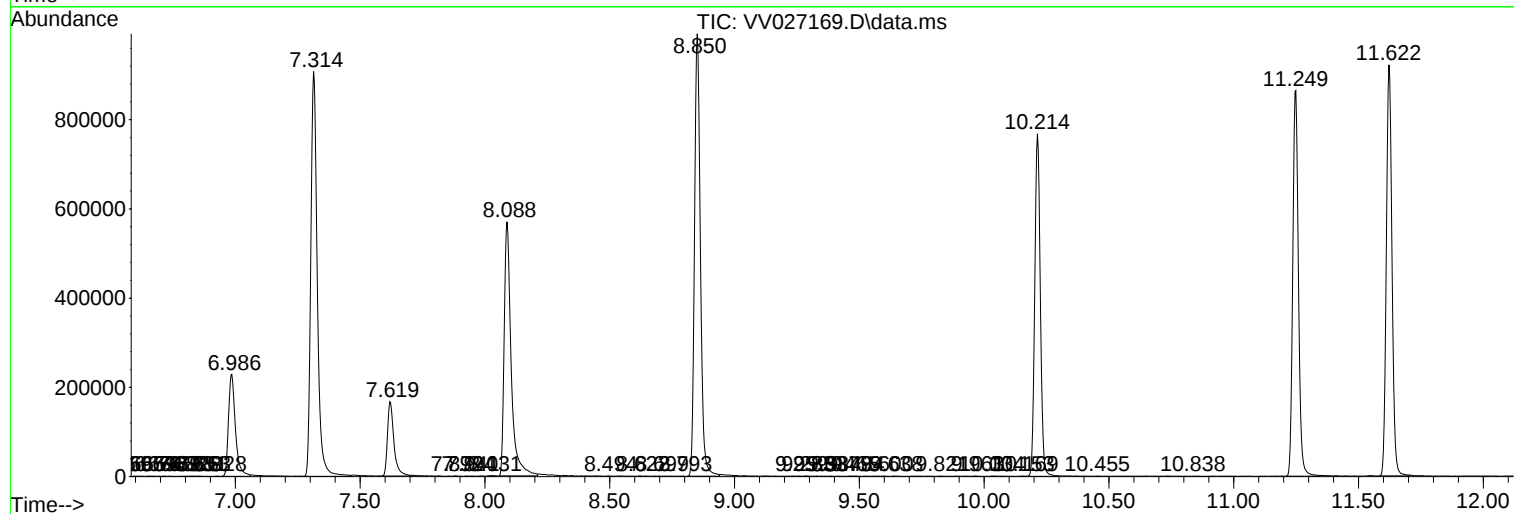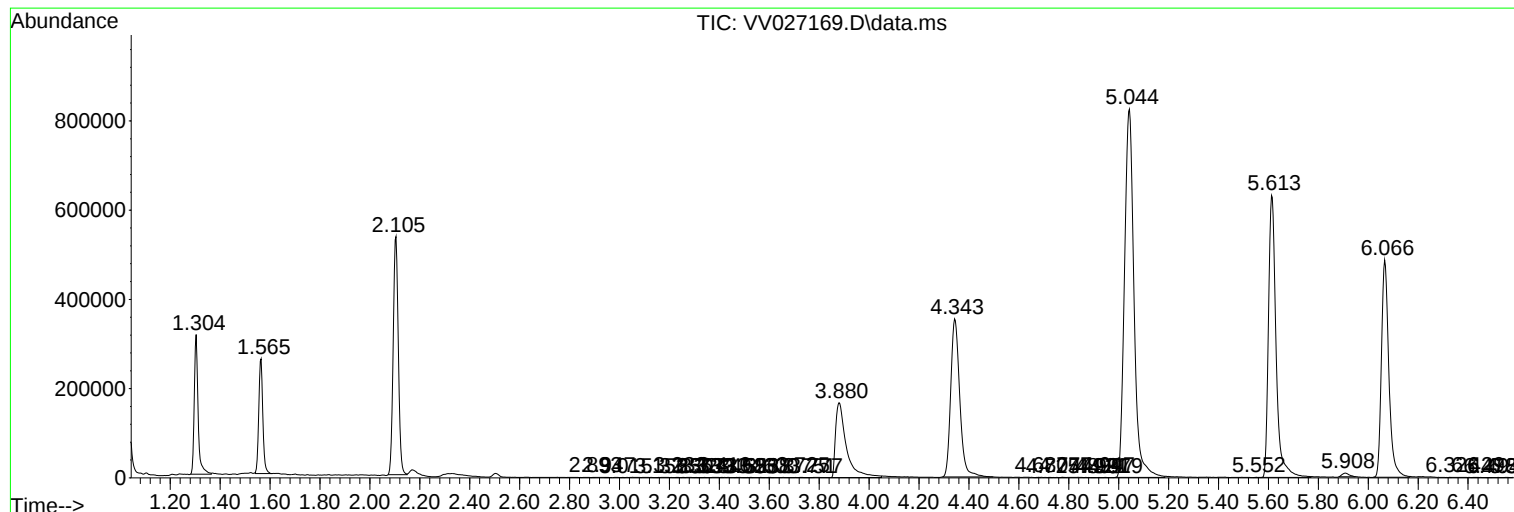

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027169.D
Acq On : 02 Aug 2022 13:49
Operator : SY/MD
Sample : N3880-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027169.D
Acq On : 02 Aug 2022 13:49
Operator : SY/MD
Sample : N3880-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc