

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027172.D
 Acq On : 02 Aug 2022 15:19
 Operator : SY/MD
 Sample : VV0801WBL04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK247

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M

Title : VOC Analysis

Signal : TIC: VV027172.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	102	rBV	297703	326595	15.18%	1.961%
2	1.561	155	162	179	rVB	257454	297488	13.82%	1.786%
3	2.101	320	330	345	rBV	535153	753483	35.02%	4.524%
4	2.172	347	352	353	rBV2	8832	7941	0.37%	0.048%
5	2.288	381	388	403	rVB	4141	7056	0.33%	0.042%
6	2.455	438	440	446	rVB4	665	617	0.03%	0.004%
7	2.500	446	454	466	rBV2	6415	10141	0.47%	0.061%
8	2.596	479	484	486	rBV	528	472	0.02%	0.003%
9	2.764	528	536	543	rVB4	1489	2109	0.10%	0.013%
10	2.895	574	577	582	rVB2	451	294	0.01%	0.002%
11	3.027	611	618	621	rBV3	538	499	0.02%	0.003%
12	3.137	649	652	655	rVB2	527	290	0.01%	0.002%
13	3.535	771	776	778	rBV	428	414	0.02%	0.002%
14	3.715	830	832	835	rVB3	513	284	0.01%	0.002%
15	3.764	845	847	854	rVB2	331	297	0.01%	0.002%
16	3.873	871	881	918	rBV	173324	510354	23.72%	3.064%
17	4.133	959	962	964	rVB4	796	408	0.02%	0.002%
18	4.339	1009	1026	1077	rBV	344239	893075	41.50%	5.362%
19	4.641	1118	1120	1124	rVB3	559	333	0.02%	0.002%
20	4.686	1132	1134	1137	rVB3	469	293	0.01%	0.002%
21	4.722	1139	1145	1148	rVB4	420	442	0.02%	0.003%
22	4.738	1148	1150	1154	rBV4	334	297	0.01%	0.002%
23	4.831	1175	1179	1183	rBV3	502	373	0.02%	0.002%
24	4.854	1183	1186	1193	rVB4	581	611	0.03%	0.004%
25	4.915	1197	1205	1212	rBV2	563	965	0.04%	0.006%
26	4.969	1219	1222	1226	rBV4	479	400	0.02%	0.002%
27	5.040	1226	1244	1291	rBV2	815050	2151836	100.00%	12.920%
28	5.352	1338	1341	1344	rBV4	583	296	0.01%	0.002%
29	5.387	1350	1352	1354	rBV2	487	279	0.01%	0.002%
30	5.410	1357	1359	1365	rVB5	660	581	0.03%	0.003%
31	5.481	1376	1381	1383	rBV	807	471	0.02%	0.003%
32	5.609	1408	1421	1458	rBV	645483	1365814	63.47%	8.201%
33	5.841	1491	1493	1499	rVB3	856	543	0.03%	0.003%
34	5.905	1503	1513	1527	rVV6	10107	22025	1.02%	0.132%
35	6.005	1540	1544	1546	rBV3	751	576	0.03%	0.003%
36	6.063	1547	1562	1595	rBV	467939	991530	46.08%	5.953%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027172.D
 Acq On : 02 Aug 2022 15:19
 Operator : SY/MD
 Sample : VV0801WBL04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK247

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.310	1637	1639	1641	rBV2	463	303	0.01%	0.002%
38	6.410	1668	1670	1674	rVB2	364	292	0.01%	0.002%
39	6.635	1734	1740	1742	rBV4	286	328	0.02%	0.002%
40	6.683	1752	1755	1760	rVB2	379	328	0.02%	0.002%
41	6.747	1771	1775	1777	rBV2	384	283	0.01%	0.002%
42	6.844	1800	1805	1809	rVB3	293	290	0.01%	0.002%
43	6.982	1837	1848	1884	rBV	229993	443902	20.63%	2.665%
44	7.313	1939	1951	1983	rBV	907907	1622884	75.42%	9.744%
45	7.619	2036	2046	2074	rBV	165710	302969	14.08%	1.819%
46	7.847	2112	2117	2119	rBV4	745	566	0.03%	0.003%
47	7.882	2126	2128	2132	rBV4	559	391	0.02%	0.002%
48	7.911	2134	2137	2142	rVB2	507	344	0.02%	0.002%
49	7.979	2152	2158	2164	rVB5	1015	1329	0.06%	0.008%
50	8.021	2169	2171	2175	rBV4	354	304	0.01%	0.002%
51	8.085	2181	2191	2223	rBV	562820	1059895	49.26%	6.364%
52	8.423	2290	2296	2302	rVB5	1591	2023	0.09%	0.012%
53	8.545	2330	2334	2338	rBV3	567	560	0.03%	0.003%
54	8.622	2355	2358	2364	rVB3	927	753	0.03%	0.005%
55	8.657	2364	2369	2375	rBV3	448	366	0.02%	0.002%
56	8.789	2406	2410	2412	rBV3	448	290	0.01%	0.002%
57	8.850	2416	2429	2467	rBV	1011453	1666029	77.42%	10.003%
58	9.146	2518	2521	2523	rBV3	494	336	0.02%	0.002%
59	9.191	2532	2535	2539	rVB2	448	294	0.01%	0.002%
60	9.349	2580	2584	2588	rBV2	362	344	0.02%	0.002%
61	9.461	2615	2619	2622	rBV2	539	413	0.02%	0.002%
62	9.538	2637	2643	2645	rBV3	421	418	0.02%	0.003%
63	9.551	2645	2647	2649	rVV2	573	361	0.02%	0.002%
64	9.583	2655	2657	2663	rVB2	640	573	0.03%	0.003%
65	9.696	2686	2692	2696	rBV2	485	509	0.02%	0.003%
66	9.789	2715	2721	2724	rVV3	247	280	0.01%	0.002%
67	9.931	2760	2765	2772	rVV3	1075	1261	0.06%	0.008%
68	9.960	2772	2774	2784	rVB3	432	484	0.02%	0.003%
69	10.005	2786	2788	2793	rBV3	304	288	0.01%	0.002%
70	10.214	2841	2853	2884	rBV	741605	1170526	54.40%	7.028%
71	10.371	2898	2902	2907	rBV3	502	502	0.02%	0.003%
72	10.545	2949	2956	2962	rVB4	889	1203	0.06%	0.007%
73	10.853	3048	3052	3058	rVB4	991	731	0.03%	0.004%
74	10.931	3073	3076	3079	rVB2	684	512	0.02%	0.003%
75	10.963	3079	3086	3089	rBV2	559	671	0.03%	0.004%
76	11.188	3149	3156	3163	rBV4	2688	3866	0.18%	0.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027172.D
 Acq On : 02 Aug 2022 15:19
 Operator : SY/MD
 Sample : VV0801WBL04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK247

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	11.246	3163	3174	3204	rBV	919998	1440482	66.94%	8.649%
78	11.384	3214	3217	3221	rBV4	622	424	0.02%	0.003%
79	11.622	3278	3291	3312	rBV	943780	1484765	69.00%	8.915%
80	11.857	3360	3364	3367	rVB2	573	471	0.02%	0.003%
81	11.879	3367	3371	3376	rBV5	619	646	0.03%	0.004%
82	11.924	3381	3385	3389	rBV2	369	308	0.01%	0.002%
83	12.255	3484	3488	3492	rVB2	452	392	0.02%	0.002%
84	12.313	3500	3506	3511	rBV4	642	668	0.03%	0.004%
85	12.435	3538	3544	3550	rVB4	1027	1361	0.06%	0.008%
86	12.590	3586	3592	3595	rBV3	454	564	0.03%	0.003%
87	12.651	3603	3611	3627	rVB5	4123	7605	0.35%	0.046%
88	12.847	3669	3672	3677	rVB2	493	378	0.02%	0.002%
89	12.972	3708	3711	3713	rBV	563	327	0.02%	0.002%
90	13.078	3742	3744	3749	rBV2	472	389	0.02%	0.002%
91	13.265	3792	3802	3818	rBV4	7286	11650	0.54%	0.070%
92	13.503	3867	3876	3892	rBV	30102	48853	2.27%	0.293%
93	13.596	3902	3905	3909	rVB2	599	406	0.02%	0.002%
94	13.744	3943	3951	3962	rVB4	10296	15052	0.70%	0.090%
95	13.918	4001	4005	4008	rBV3	566	410	0.02%	0.002%
96	14.123	4066	4069	4071	rBV3	435	332	0.02%	0.002%
97	14.512	4187	4190	4192	rBV	530	340	0.02%	0.002%
98	14.554	4200	4203	4208	rBV3	550	513	0.02%	0.003%
99	14.747	4259	4263	4266	rBV4	486	499	0.02%	0.003%
100	14.953	4323	4327	4331	rBV4	756	848	0.04%	0.005%




Sum of corrected areas: 16655166

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027172.D
Acq On : 02 Aug 2022 15:19
Operator : SY/MD
Sample : VV0801WBL04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK247

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

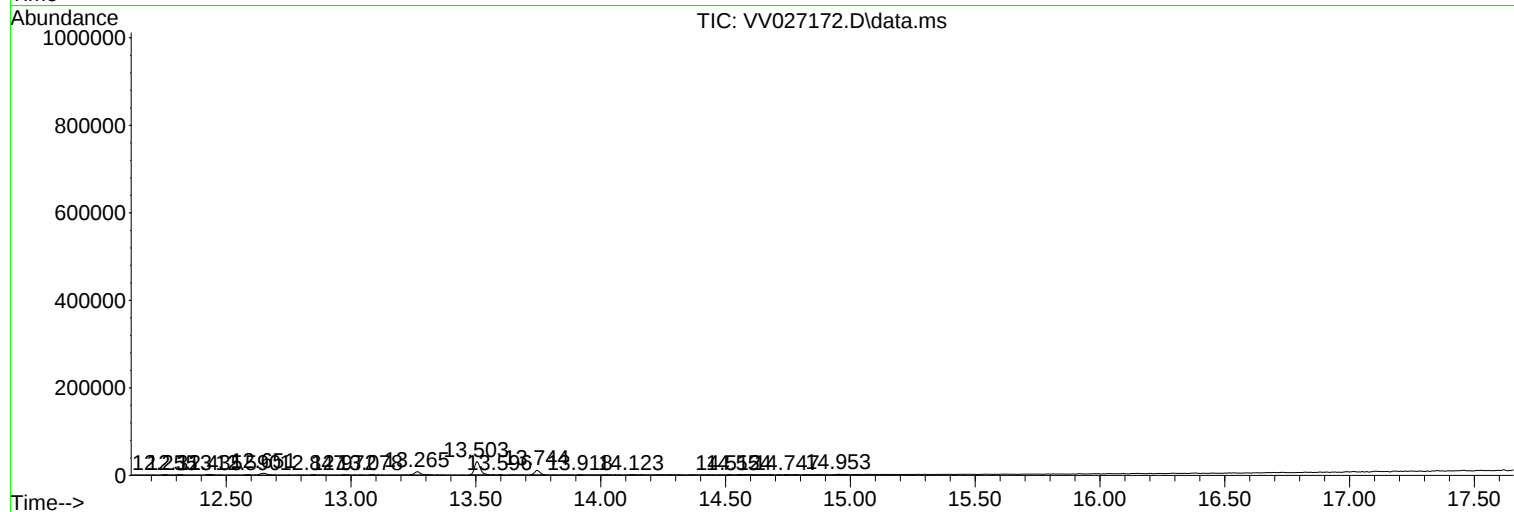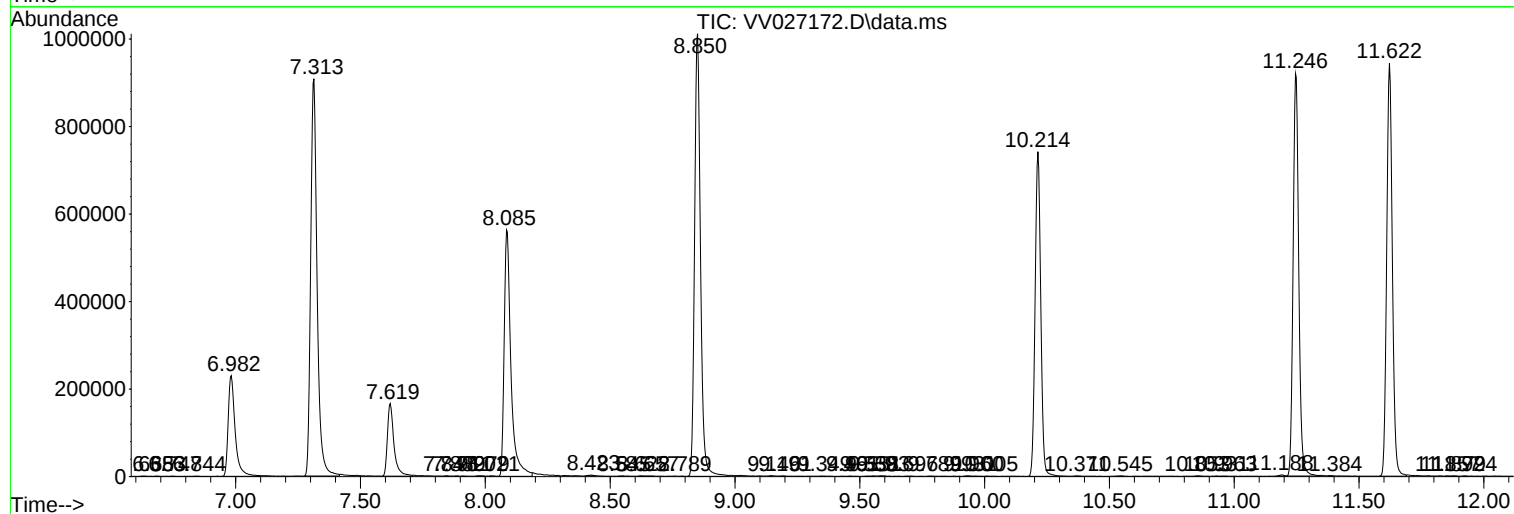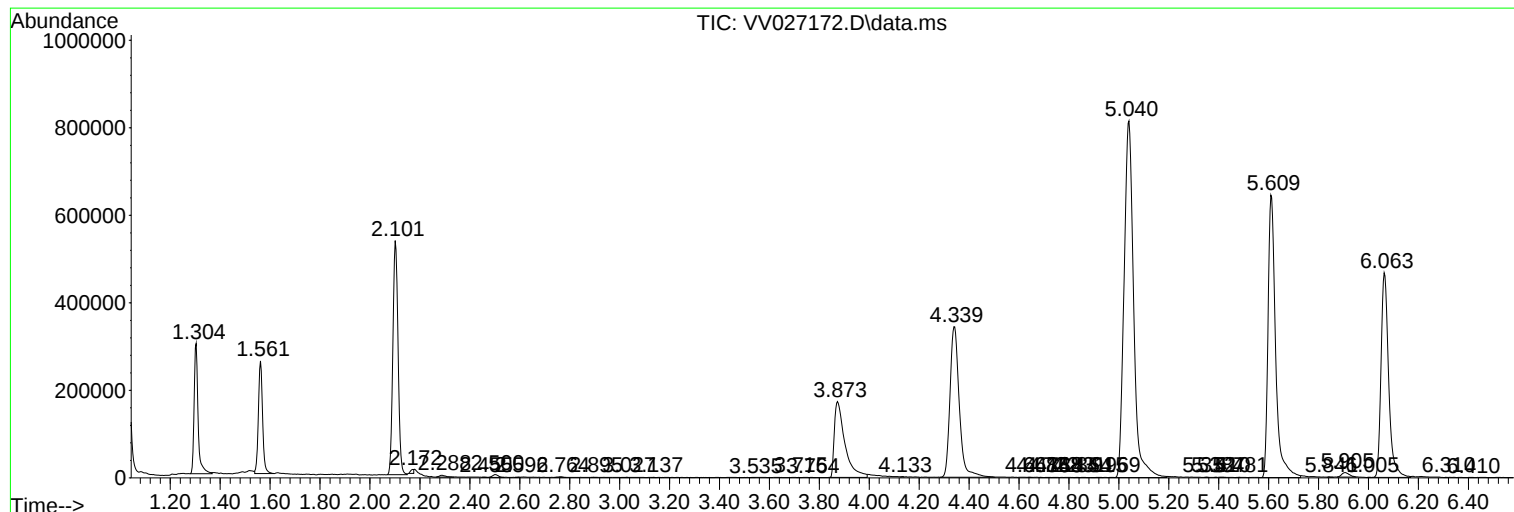

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027172.D
Acq On : 02 Aug 2022 15:19
Operator : SY/MD
Sample : VV0801WBL04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK247

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027172.D
Acq On : 02 Aug 2022 15:19
Operator : SY/MD
Sample : VV0801WBL04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK247

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------