

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027174.D
 Acq On : 02 Aug 2022 16:32
 Operator : SY/MD
 Sample : N4005-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY149

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027174.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	103	rBV	261815	284888	14.90%	1.946%
2	1.561	155	162	178	rVB	228456	262727	13.74%	1.795%
3	2.101	321	330	345	rBV	462130	654541	34.24%	4.471%
4	2.539	463	466	469	rBV2	486	245	0.01%	0.002%
5	2.606	483	487	489	rBV2	532	419	0.02%	0.003%
6	2.732	524	526	528	rBV2	428	287	0.02%	0.002%
7	2.966	596	599	602	rBV2	382	323	0.02%	0.002%
8	3.085	631	636	642	rBV2	287	381	0.02%	0.003%
9	3.156	656	658	662	rBV	194	150	0.01%	0.001%
10	3.179	663	665	668	rVV3	340	168	0.01%	0.001%
11	3.224	674	679	683	rBV3	288	372	0.02%	0.003%
12	3.275	692	695	696	rBV2	260	132	0.01%	0.001%
13	3.317	702	708	712	rBV2	290	293	0.02%	0.002%
14	3.346	713	717	721	rVV3	268	224	0.01%	0.002%
15	3.397	730	733	735	rBV2	254	164	0.01%	0.001%
16	3.449	745	749	750	rBV2	175	114	0.01%	0.001%
17	3.468	753	755	758	rVB	254	118	0.01%	0.001%
18	3.494	759	763	767	rVB3	326	253	0.01%	0.002%
19	3.513	767	769	770	rBV3	195	80	0.00%	0.001%
20	3.629	802	805	808	rVB2	369	201	0.01%	0.001%
21	3.671	816	818	820	rVB	103	45	0.00%	0.000%
22	3.680	820	821	824	rBV2	198	79	0.00%	0.001%
23	3.703	825	828	831	rVV	197	112	0.01%	0.001%
24	3.719	831	833	834	rBV	156	61	0.00%	0.000%
25	3.738	837	839	841	rVB	285	119	0.01%	0.001%
26	3.757	841	845	848	rBV	299	223	0.01%	0.002%
27	3.812	861	862	863	rBV	184	61	0.00%	0.000%
28	3.876	872	882	920	rBV	149391	429280	22.45%	2.932%
29	4.343	1012	1027	1076	rVB	311564	795787	41.62%	5.436%
30	4.738	1146	1150	1154	rVB3	492	442	0.02%	0.003%
31	4.770	1157	1160	1161	rBV3	262	168	0.01%	0.001%
32	4.802	1168	1170	1171	rBV3	343	120	0.01%	0.001%
33	4.828	1176	1178	1180	rVB	309	105	0.01%	0.001%
34	4.844	1181	1183	1188	rVB2	284	172	0.01%	0.001%
35	4.867	1188	1190	1193	rBV2	205	139	0.01%	0.001%
36	4.944	1207	1214	1219	rBV3	434	674	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027174.D
 Acq On : 02 Aug 2022 16:32
 Operator : SY/MD
 Sample : N4005-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY149

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	4.970	1220	1222	1226	rBV3	243	154	0.01%	0.001%
38	5.043	1228	1245	1289	rBV2	720733	1911899	100.00%	13.060%
39	5.362	1341	1344	1346	rBV	557	266	0.01%	0.002%
40	5.516	1389	1392	1395	rVB2	447	298	0.02%	0.002%
41	5.542	1395	1400	1403	rBV4	434	514	0.03%	0.004%
42	5.613	1410	1422	1462	rBV	584798	1239216	64.82%	8.465%
43	5.905	1503	1513	1535	rBV2	14343	33291	1.74%	0.227%
44	6.066	1549	1563	1595	rBV	422432	883699	46.22%	6.036%
45	6.359	1650	1654	1659	rVB4	637	534	0.03%	0.004%
46	6.387	1659	1663	1664	rBV	268	181	0.01%	0.001%
47	6.439	1676	1679	1681	rBV	222	135	0.01%	0.001%
48	6.539	1707	1710	1716	rVB2	418	306	0.02%	0.002%
49	6.564	1716	1718	1720	rBV3	228	141	0.01%	0.001%
50	6.616	1732	1734	1737	rBV2	257	136	0.01%	0.001%
51	6.661	1743	1748	1754	rVB2	301	301	0.02%	0.002%
52	6.696	1754	1759	1764	rVB2	495	459	0.02%	0.003%
53	6.725	1764	1768	1772	rBV2	410	360	0.02%	0.002%
54	6.770	1779	1782	1788	rVB3	368	328	0.02%	0.002%
55	6.809	1788	1794	1795	rBV	256	155	0.01%	0.001%
56	6.831	1795	1801	1805	rVV3	328	380	0.02%	0.003%
57	6.870	1810	1813	1816	rVB3	314	187	0.01%	0.001%
58	6.892	1816	1820	1823	rBV2	432	270	0.01%	0.002%
59	6.915	1823	1827	1830	rBV2	340	250	0.01%	0.002%
60	6.986	1837	1849	1878	rBV	199391	379972	19.87%	2.596%
61	7.314	1939	1951	1986	rBV	773963	1408207	73.65%	9.619%
62	7.619	2036	2046	2071	rBV	143436	261638	13.68%	1.787%
63	7.908	2133	2136	2137	rBV3	357	184	0.01%	0.001%
64	7.940	2145	2146	2147	rBV	563	135	0.01%	0.001%
65	8.088	2182	2192	2227	rBV	505075	978931	51.20%	6.687%
66	8.535	2328	2331	2334	rBV3	549	471	0.02%	0.003%
67	8.555	2334	2337	2339	rVB2	510	300	0.02%	0.002%
68	8.587	2344	2347	2348	rBV	346	183	0.01%	0.001%
69	8.648	2364	2366	2367	rBV	236	86	0.00%	0.001%
70	8.793	2407	2411	2412	rBV2	1156	777	0.04%	0.005%
71	8.850	2418	2429	2458	rBV	911530	1509020	78.93%	10.308%
72	9.329	2577	2578	2582	rBV2	220	131	0.01%	0.001%
73	9.355	2582	2586	2590	rBV2	362	303	0.02%	0.002%
74	9.429	2607	2609	2611	rVB2	298	120	0.01%	0.001%
75	9.481	2620	2625	2628	rBV3	340	382	0.02%	0.003%
76	9.571	2649	2653	2654	rBV	286	212	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027174.D
 Acq On : 02 Aug 2022 16:32
 Operator : SY/MD
 Sample : N4005-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY149

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	9.641	2672	2675	2677	rBV	189	123	0.01%	0.001%
78	9.683	2685	2688	2690	rBV2	295	177	0.01%	0.001%
79	9.741	2703	2706	2708	rBV2	309	232	0.01%	0.002%
80	9.847	2733	2739	2742	rBV2	300	347	0.02%	0.002%
81	9.918	2757	2761	2763	rBV2	217	184	0.01%	0.001%
82	10.214	2837	2853	2878	rBV	658746	1046631	54.74%	7.149%
83	10.384	2902	2906	2909	rBV3	438	390	0.02%	0.003%
84	10.423	2915	2918	2921	rBV	453	304	0.02%	0.002%
85	10.548	2955	2957	2960	rBV	224	149	0.01%	0.001%
86	10.802	3033	3036	3039	rBV3	172	128	0.01%	0.001%
87	10.928	3072	3075	3078	rBV2	362	255	0.01%	0.002%
88	11.056	3112	3115	3117	rVB2	440	264	0.01%	0.002%
89	11.069	3117	3119	3120	rBV2	202	65	0.00%	0.000%
90	11.124	3132	3136	3139	rBV2	364	290	0.02%	0.002%
91	11.249	3163	3175	3199	rBV	801168	1260174	65.91%	8.608%
92	11.542	3258	3266	3275	rBV5	5029	9230	0.48%	0.063%
93	11.622	3280	3291	3328	rVB	803636	1264369	66.13%	8.637%
94	12.310	3500	3505	3510	rVB3	1294	1399	0.07%	0.010%
95	12.352	3516	3518	3519	rBV	570	267	0.01%	0.002%
96	12.464	3550	3553	3557	rBV3	555	501	0.03%	0.003%
97	13.130	3758	3760	3762	rBV2	390	245	0.01%	0.002%
98	15.149	4385	4388	4392	rVB	10097	5570	0.29%	0.038%




Sum of corrected areas: 14639473

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027174.D
Acq On : 02 Aug 2022 16:32
Operator : SY/MD
Sample : N4005-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY149

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

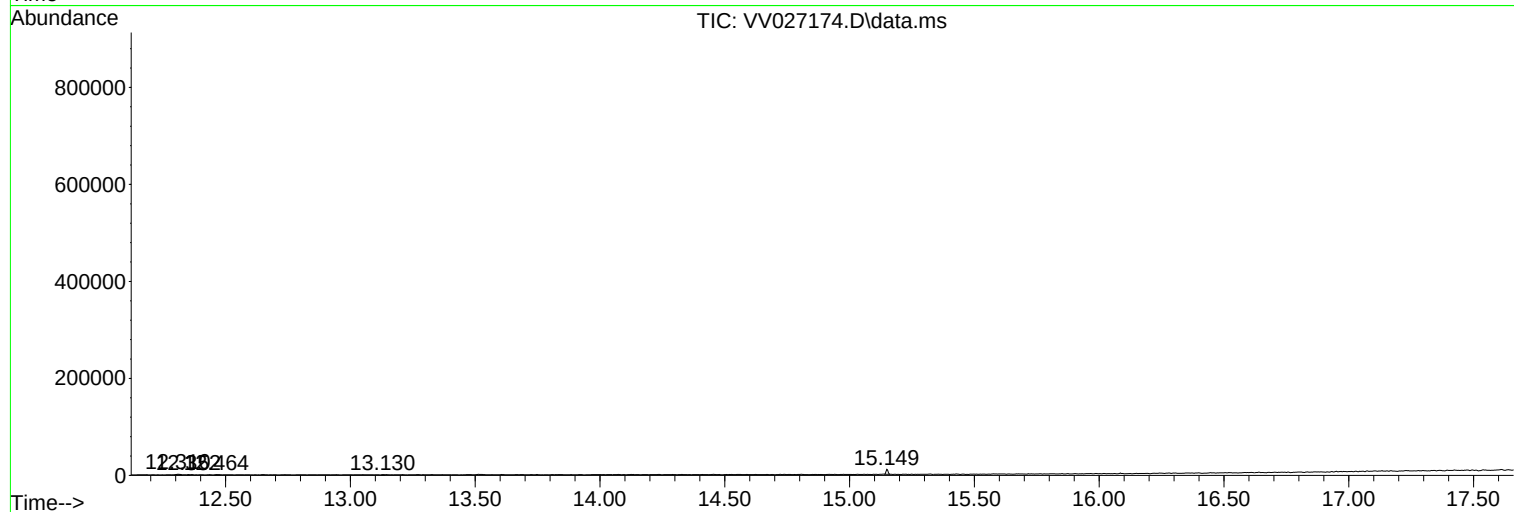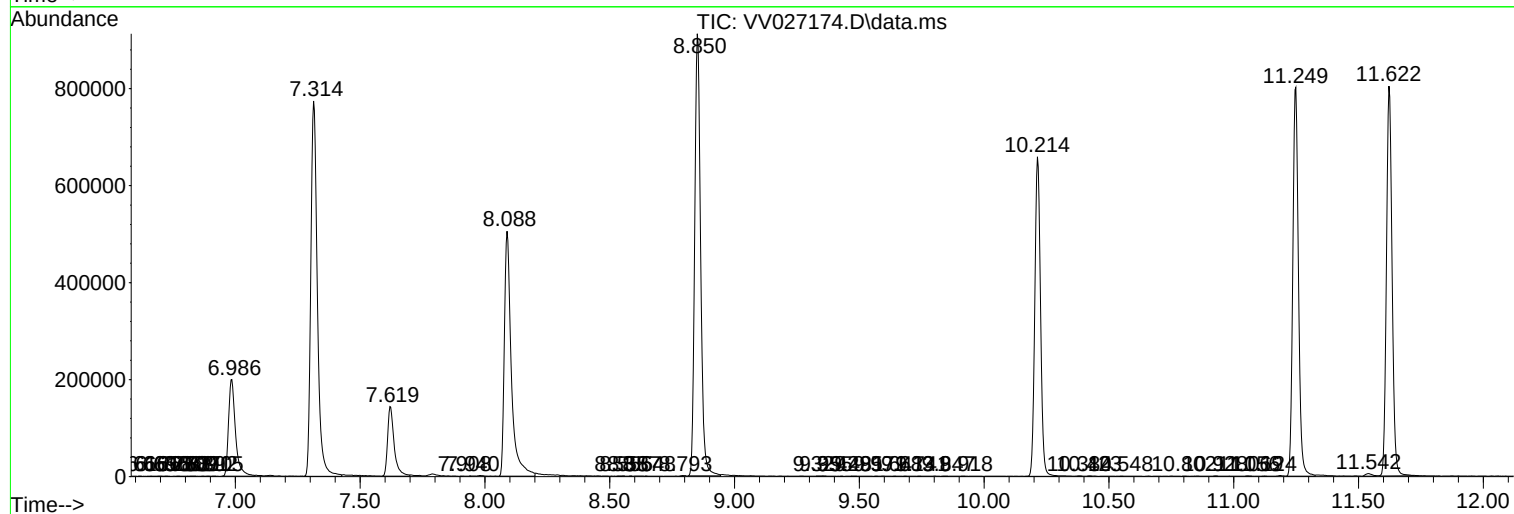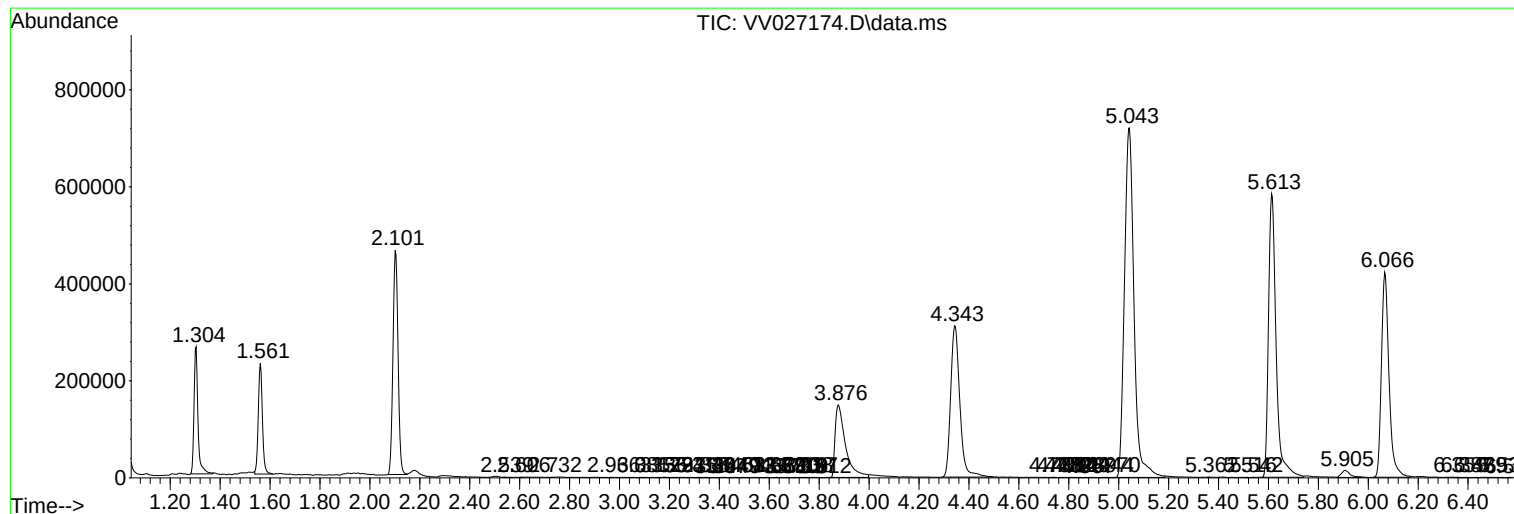

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027174.D
Acq On : 02 Aug 2022 16:32
Operator : SY/MD
Sample : N4005-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY149

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027174.D
Acq On : 02 Aug 2022 16:32
Operator : SY/MD
Sample : N4005-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY149

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------