

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027175.D
 Acq On : 02 Aug 2022 16:57
 Operator : SY/MD
 Sample : N4003-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027175.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	126	rVB	2766600	3192909	100.00%	17.342%
2	1.561	155	162	179	rVB	236429	276225	8.65%	1.500%
3	2.101	320	330	346	rBV	485934	684860	21.45%	3.720%
4	2.510	448	457	463	rVV5	1899	3164	0.10%	0.017%
5	2.542	463	467	469	rVB2	518	326	0.01%	0.002%
6	2.584	476	480	484	rBV4	335	304	0.01%	0.002%
7	2.641	489	498	510	rBV5	1721	3732	0.12%	0.020%
8	2.757	519	534	552	rBV	151189	267260	8.37%	1.452%
9	3.101	639	641	647	rVB2	421	332	0.01%	0.002%
10	3.140	647	653	657	rBV2	309	355	0.01%	0.002%
11	3.182	662	666	671	rVB2	411	390	0.01%	0.002%
12	3.301	698	703	706	rBV2	336	300	0.01%	0.002%
13	3.365	720	723	727	rBV2	339	256	0.01%	0.001%
14	3.400	727	734	739	rVB2	598	687	0.02%	0.004%
15	3.436	739	745	750	rBV2	401	497	0.02%	0.003%
16	3.465	750	754	764	rBV2	358	469	0.01%	0.003%
17	3.606	794	798	802	rBV2	380	356	0.01%	0.002%
18	3.760	841	846	848	rBV3	403	343	0.01%	0.002%
19	3.876	872	882	926	rBV	160125	526505	16.49%	2.860%
20	4.182	973	977	979	rBV4	772	608	0.02%	0.003%
21	4.342	1011	1027	1051	rBV	322126	819071	25.65%	4.449%
22	4.857	1185	1187	1191	rVB3	396	288	0.01%	0.002%
23	4.921	1203	1207	1210	rBV3	328	335	0.01%	0.002%
24	5.043	1227	1245	1289	rBV2	756696	2023442	63.37%	10.990%
25	5.368	1338	1346	1351	rBV6	4491	7214	0.23%	0.039%
26	5.455	1369	1373	1377	rBV3	431	395	0.01%	0.002%
27	5.490	1379	1384	1385	rBV3	375	258	0.01%	0.001%
28	5.497	1385	1386	1390	rVB2	704	415	0.01%	0.002%
29	5.519	1390	1393	1396	rBV2	426	352	0.01%	0.002%
30	5.612	1409	1422	1466	rBV	563881	1217965	38.15%	6.615%
31	5.911	1503	1515	1521	rBV	9450	20863	0.65%	0.113%
32	6.066	1548	1563	1596	rBV	441545	934839	29.28%	5.077%
33	6.320	1640	1642	1646	rVB2	587	478	0.01%	0.003%
34	6.342	1646	1649	1652	rBV2	535	408	0.01%	0.002%
35	6.435	1672	1678	1679	rBV2	391	293	0.01%	0.002%
36	6.445	1679	1681	1687	rVB4	691	544	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027175.D
 Acq On : 02 Aug 2022 16:57
 Operator : SY/MD
 Sample : N4003-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.673	1750	1752	1756	rVB3	422	272	0.01%	0.001%
38	6.725	1765	1768	1772	rVB2	555	435	0.01%	0.002%
39	6.985	1834	1849	1873	rBV	207471	396103	12.41%	2.151%
40	7.313	1938	1951	1988	rBV	806677	1494320	46.80%	8.116%
41	7.535	2013	2020	2027	rBV2	4160	5776	0.18%	0.031%
42	7.622	2036	2047	2072	rBV	146797	271412	8.50%	1.474%
43	7.847	2113	2117	2122	rBV3	393	374	0.01%	0.002%
44	7.873	2122	2125	2127	rVB	603	334	0.01%	0.002%
45	7.934	2141	2144	2145	rBV2	497	285	0.01%	0.002%
46	7.976	2153	2157	2158	rBV3	948	602	0.02%	0.003%
47	8.027	2167	2173	2176	rBV3	708	700	0.02%	0.004%
48	8.088	2181	2192	2228	rBV	545447	1035538	32.43%	5.624%
49	8.387	2282	2285	2286	rBV3	428	277	0.01%	0.002%
50	8.480	2312	2314	2319	rVB2	565	327	0.01%	0.002%
51	8.545	2331	2334	2341	rBV5	606	655	0.02%	0.004%
52	8.673	2372	2374	2379	rVB3	539	353	0.01%	0.002%
53	8.763	2398	2402	2405	rBV2	524	475	0.01%	0.003%
54	8.850	2417	2429	2459	rBV	908410	1493107	46.76%	8.110%
55	9.095	2501	2505	2506	rBV3	468	315	0.01%	0.002%
56	9.149	2517	2522	2524	rBV3	821	580	0.02%	0.003%
57	9.236	2547	2549	2553	rVB2	629	466	0.01%	0.003%
58	9.342	2580	2582	2588	rVB3	356	304	0.01%	0.002%
59	9.406	2599	2602	2605	rBV	753	447	0.01%	0.002%
60	9.439	2609	2612	2614	rVB	502	281	0.01%	0.002%
61	9.471	2620	2622	2628	rVB3	299	294	0.01%	0.002%
62	9.532	2636	2641	2644	rBV2	436	411	0.01%	0.002%
63	9.551	2644	2647	2652	rVV3	473	392	0.01%	0.002%
64	9.677	2683	2686	2692	rBV3	273	330	0.01%	0.002%
65	9.705	2692	2695	2700	rVB2	349	284	0.01%	0.002%
66	9.731	2701	2703	2707	rVB3	408	252	0.01%	0.001%
67	9.934	2764	2766	2771	rVB2	557	360	0.01%	0.002%
68	9.982	2779	2781	2786	rVB	346	257	0.01%	0.001%
69	10.130	2823	2827	2831	rBV3	337	328	0.01%	0.002%
70	10.213	2840	2853	2875	rBV	712422	1125467	35.25%	6.113%
71	10.451	2921	2927	2929	rVV2	390	404	0.01%	0.002%
72	10.487	2933	2938	2940	rVV3	501	430	0.01%	0.002%
73	10.541	2947	2955	2960	rVB4	565	808	0.03%	0.004%
74	10.857	3048	3053	3059	rVB5	992	1162	0.04%	0.006%
75	10.924	3071	3074	3078	rBV2	360	301	0.01%	0.002%
76	10.953	3079	3083	3088	rVB3	346	340	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027175.D
 Acq On : 02 Aug 2022 16:57
 Operator : SY/MD
 Sample : N4003-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	11.082	3120	3123	3129	rVB2	401	354	0.01%	0.002%
78	11.181	3151	3154	3157	rBV	505	359	0.01%	0.002%
79	11.249	3163	3175	3200	rBV	789639	1232689	38.61%	6.695%
80	11.532	3260	3263	3266	rBV3	886	688	0.02%	0.004%
81	11.622	3277	3291	3314	rBV	838149	1346390	42.17%	7.313%
82	11.950	3390	3393	3397	rBV2	524	361	0.01%	0.002%
83	12.156	3453	3457	3459	rBV	423	335	0.01%	0.002%
84	12.387	3525	3529	3532	rBV2	406	398	0.01%	0.002%
85	12.599	3592	3595	3600	rBV3	487	473	0.01%	0.003%
86	13.139	3760	3763	3766	rBV2	443	330	0.01%	0.002%
87	13.355	3827	3830	3832	rBV2	388	257	0.01%	0.001%
88	13.577	3896	3899	3903	rBV2	404	273	0.01%	0.001%
89	13.602	3903	3907	3913	rBV2	471	397	0.01%	0.002%
90	13.635	3913	3917	3922	rVB2	555	519	0.02%	0.003%
91	13.696	3932	3936	3938	rBV	582	500	0.02%	0.003%
92	13.741	3947	3950	3956	rBV4	638	772	0.02%	0.004%
93	13.811	3969	3972	3976	rBV3	460	346	0.01%	0.002%
94	14.014	4029	4035	4041	rBV2	857	1161	0.04%	0.006%
95	14.200	4092	4093	4099	rBV3	352	285	0.01%	0.002%
96	14.242	4104	4106	4109	rBV	458	271	0.01%	0.001%
97	15.081	4364	4367	4370	rBV2	742	478	0.01%	0.003%
98	15.178	4393	4397	4398	rBV2	827	571	0.02%	0.003%
99	15.525	4503	4505	4506	rBV	688	362	0.01%	0.002%
100	15.731	4567	4569	4571	rBV	741	399	0.01%	0.002%




Sum of corrected areas: 18411564

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027175.D
Acq On : 02 Aug 2022 16:57
Operator : SY/MD
Sample : N4003-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

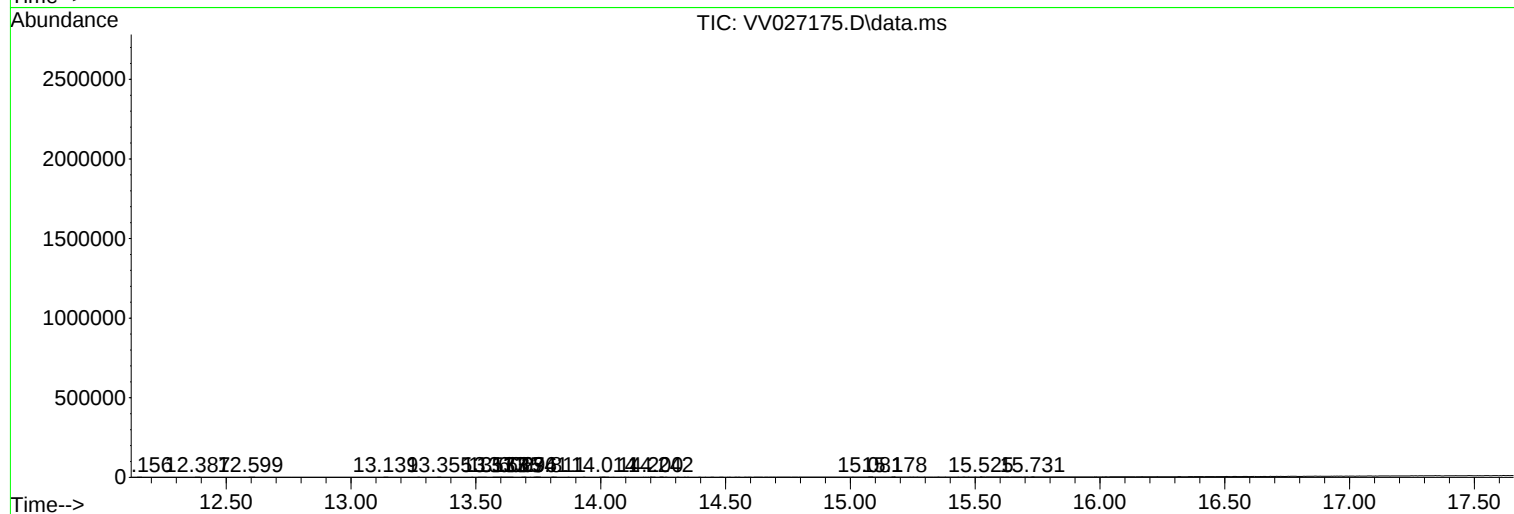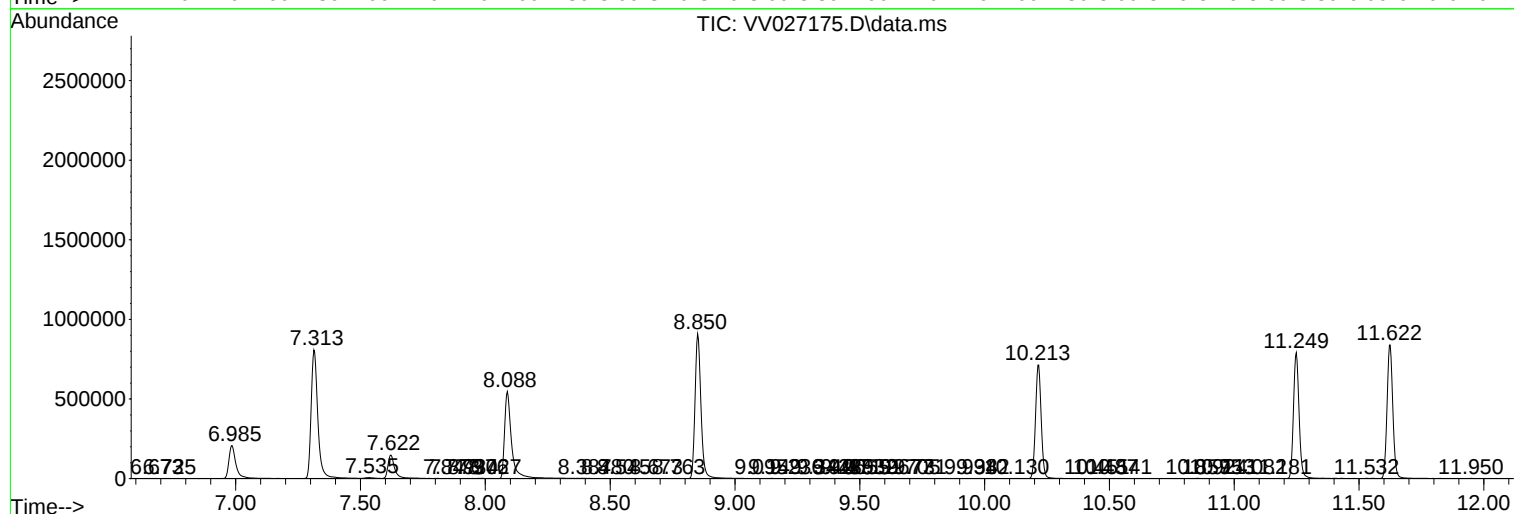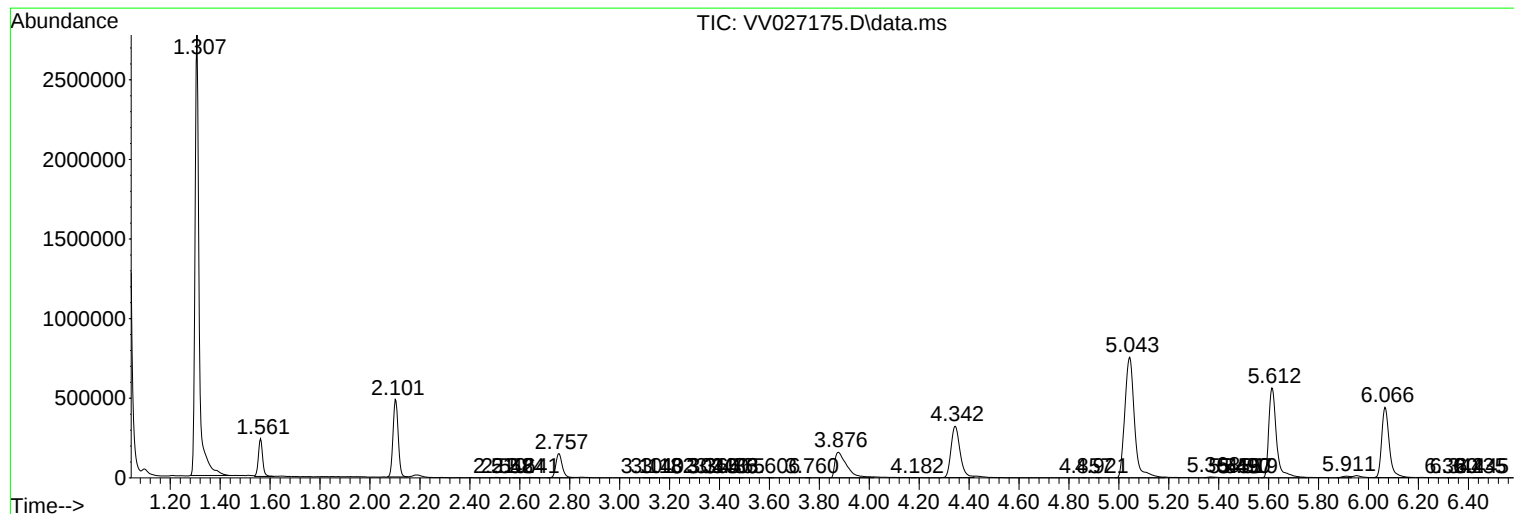

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027175.D
Acq On : 02 Aug 2022 16:57
Operator : SY/MD
Sample : N4003-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027175.D
Acq On : 02 Aug 2022 16:57
Operator : SY/MD
Sample : N4003-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------