

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027176.D
 Acq On : 02 Aug 2022 17:21
 Operator : SY/MD
 Sample : N4003-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027176.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	152	rBV	19402154	25818156	100.00%	49.490%
2	1.558	155	161	181	rVB	223031	272101	1.05%	0.522%
3	2.101	320	330	345	rBV	473497	669822	2.59%	1.284%
4	2.497	448	453	461	rVB4	1881	2793	0.01%	0.005%
5	2.645	485	499	500	rBV4	2722	4343	0.02%	0.008%
6	2.754	520	533	551	rBV	960456	1640187	6.35%	3.144%
7	3.143	650	654	657	rVB3	452	315	0.00%	0.001%
8	3.294	697	701	705	rBV3	416	426	0.00%	0.001%
9	3.490	758	762	767	rBV2	356	457	0.00%	0.001%
10	3.529	771	774	778	rVV3	379	348	0.00%	0.001%
11	3.603	792	797	800	rVB	340	269	0.00%	0.001%
12	3.902	871	890	909	rBV	4437193	10638359	41.20%	20.393%
13	4.342	1011	1027	1048	rBV2	312547	785820	3.04%	1.506%
14	4.648	1117	1122	1128	rBV6	734	933	0.00%	0.002%
15	4.674	1128	1130	1134	rVB2	797	547	0.00%	0.001%
16	4.696	1134	1137	1141	rBV4	556	553	0.00%	0.001%
17	4.757	1152	1156	1160	rBV3	570	423	0.00%	0.001%
18	4.850	1183	1185	1191	rVB2	604	527	0.00%	0.001%
19	5.040	1222	1244	1284	rBV2	735112	1968277	7.62%	3.773%
20	5.371	1334	1347	1359	rBV3	9113	21148	0.08%	0.041%
21	5.477	1376	1380	1381	rBV3	537	449	0.00%	0.001%
22	5.503	1385	1388	1393	rVB4	408	406	0.00%	0.001%
23	5.612	1410	1422	1466	rBV	569577	1213233	4.70%	2.326%
24	5.860	1495	1499	1501	rBV4	569	324	0.00%	0.001%
25	5.911	1503	1515	1520	rBV5	8790	17746	0.07%	0.034%
26	6.066	1548	1563	1600	rBV	433764	904333	3.50%	1.734%
27	6.291	1631	1633	1637	rVB3	798	504	0.00%	0.001%
28	6.313	1637	1640	1643	rBV3	742	652	0.00%	0.001%
29	6.336	1645	1647	1649	rVV2	720	371	0.00%	0.001%
30	6.484	1689	1693	1697	rBV2	630	477	0.00%	0.001%
31	6.529	1703	1707	1709	rBV3	336	301	0.00%	0.001%
32	6.616	1731	1734	1739	rVB2	316	279	0.00%	0.001%
33	6.641	1739	1742	1747	rBV2	310	306	0.00%	0.001%
34	6.850	1804	1807	1812	rVB3	327	273	0.00%	0.001%
35	6.985	1836	1849	1878	rBV	200108	382707	1.48%	0.734%
36	7.252	1928	1932	1936	rVB4	465	440	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027176.D
 Acq On : 02 Aug 2022 17:21
 Operator : SY/MD
 Sample : N4003-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	7.313	1938	1951	1974	rBV	807125	1432158	5.55%	2.745%
38	7.532	2014	2019	2030	rVB3	5700	8847	0.03%	0.017%
39	7.619	2036	2046	2067	rBV2	143601	260141	1.01%	0.499%
40	7.915	2134	2138	2139	rBV3	582	387	0.00%	0.001%
41	7.934	2139	2144	2146	rBV5	1000	936	0.00%	0.002%
42	8.021	2165	2171	2175	rVB4	691	669	0.00%	0.001%
43	8.088	2181	2192	2228	rBV	523080	1003042	3.89%	1.923%
44	8.448	2301	2304	2305	rBV	536	312	0.00%	0.001%
45	8.612	2353	2355	2358	rVB2	500	279	0.00%	0.001%
46	8.706	2381	2384	2388	rBV	509	378	0.00%	0.001%
47	8.786	2405	2409	2411	rBV2	454	331	0.00%	0.001%
48	8.850	2417	2429	2464	rBV	896472	1478790	5.73%	2.835%
49	9.101	2506	2507	2511	rVB3	612	347	0.00%	0.001%
50	9.130	2511	2516	2518	rBV4	722	650	0.00%	0.001%
51	9.149	2518	2522	2525	rVV3	791	745	0.00%	0.001%
52	9.165	2525	2527	2532	rVB3	481	369	0.00%	0.001%
53	9.214	2538	2542	2545	rBV4	426	366	0.00%	0.001%
54	9.384	2592	2595	2598	rBV	436	281	0.00%	0.001%
55	9.426	2605	2608	2614	rVB3	438	457	0.00%	0.001%
56	9.866	2743	2745	2749	rBV	518	286	0.00%	0.001%
57	9.892	2749	2753	2758	rBV2	402	381	0.00%	0.001%
58	9.931	2760	2765	2768	rBV4	434	422	0.00%	0.001%
59	10.037	2796	2798	2802	rVB2	338	267	0.00%	0.001%
60	10.101	2811	2818	2820	rBV3	297	362	0.00%	0.001%
61	10.214	2840	2853	2879	rBV	694921	1088964	4.22%	2.087%
62	10.377	2897	2904	2911	rBV5	731	948	0.00%	0.002%
63	10.448	2923	2926	2930	rBV3	470	290	0.00%	0.001%
64	10.538	2949	2954	2955	rVV2	394	309	0.00%	0.001%
65	10.586	2966	2969	2972	rVB2	436	287	0.00%	0.001%
66	10.683	2994	2999	3001	rBV3	447	422	0.00%	0.001%
67	10.792	3030	3033	3038	rVB3	387	288	0.00%	0.001%
68	10.815	3038	3040	3044	rBV2	362	272	0.00%	0.001%
69	10.853	3045	3052	3056	rVV4	605	731	0.00%	0.001%
70	11.072	3117	3120	3123	rBV	435	264	0.00%	0.001%
71	11.101	3123	3129	3130	rBV	270	279	0.00%	0.001%
72	11.111	3130	3132	3138	rVB2	506	391	0.00%	0.001%
73	11.194	3152	3158	3161	rBV4	621	619	0.00%	0.001%
74	11.249	3163	3175	3197	rBV	792515	1222583	4.74%	2.344%
75	11.458	3237	3240	3243	rVB3	714	559	0.00%	0.001%
76	11.622	3279	3291	3316	rBV	826512	1300830	5.04%	2.494%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027176.D
 Acq On : 02 Aug 2022 17:21
 Operator : SY/MD
 Sample : N4003-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	12.008	3405	3411	3414	rBV3	400	455	0.00%	0.001%
78	12.172	3458	3462	3466	rVB5	418	370	0.00%	0.001%
79	12.194	3466	3469	3475	rVB2	418	405	0.00%	0.001%
80	12.580	3586	3589	3594	rVB3	349	301	0.00%	0.001%
81	12.705	3626	3628	3634	rVB3	458	362	0.00%	0.001%
82	12.940	3697	3701	3705	rBV3	532	594	0.00%	0.001%
83	13.065	3734	3740	3744	rBV3	370	469	0.00%	0.001%
84	13.152	3763	3767	3771	rBV2	367	369	0.00%	0.001%
85	13.348	3824	3828	3834	rBV4	463	573	0.00%	0.001%
86	13.519	3876	3881	3883	rBV3	686	639	0.00%	0.001%
87	13.535	3883	3886	3890	rVB3	670	506	0.00%	0.001%
88	13.641	3916	3919	3924	rBV2	276	294	0.00%	0.001%
89	13.686	3930	3933	3936	rBV	511	392	0.00%	0.001%
90	13.741	3945	3950	3953	rBV	436	513	0.00%	0.001%
91	13.895	3994	3998	4004	rVB3	553	559	0.00%	0.001%
92	14.075	4049	4054	4056	rBV2	395	429	0.00%	0.001%
93	14.168	4079	4083	4084	rBV2	578	427	0.00%	0.001%
94	14.197	4090	4092	4095	rBV2	485	317	0.00%	0.001%
95	14.291	4118	4121	4126	rVB4	496	455	0.00%	0.001%
96	14.348	4136	4139	4141	rVB2	551	267	0.00%	0.001%
97	14.409	4154	4158	4160	rBV3	539	424	0.00%	0.001%
98	14.525	4191	4194	4197	rBV	371	301	0.00%	0.001%
99	14.754	4262	4265	4267	rBV2	757	380	0.00%	0.001%
100	15.014	4344	4346	4351	rBV2	449	314	0.00%	0.001%




Sum of corrected areas: 52167959

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027176.D
Acq On : 02 Aug 2022 17:21
Operator : SY/MD
Sample : N4003-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

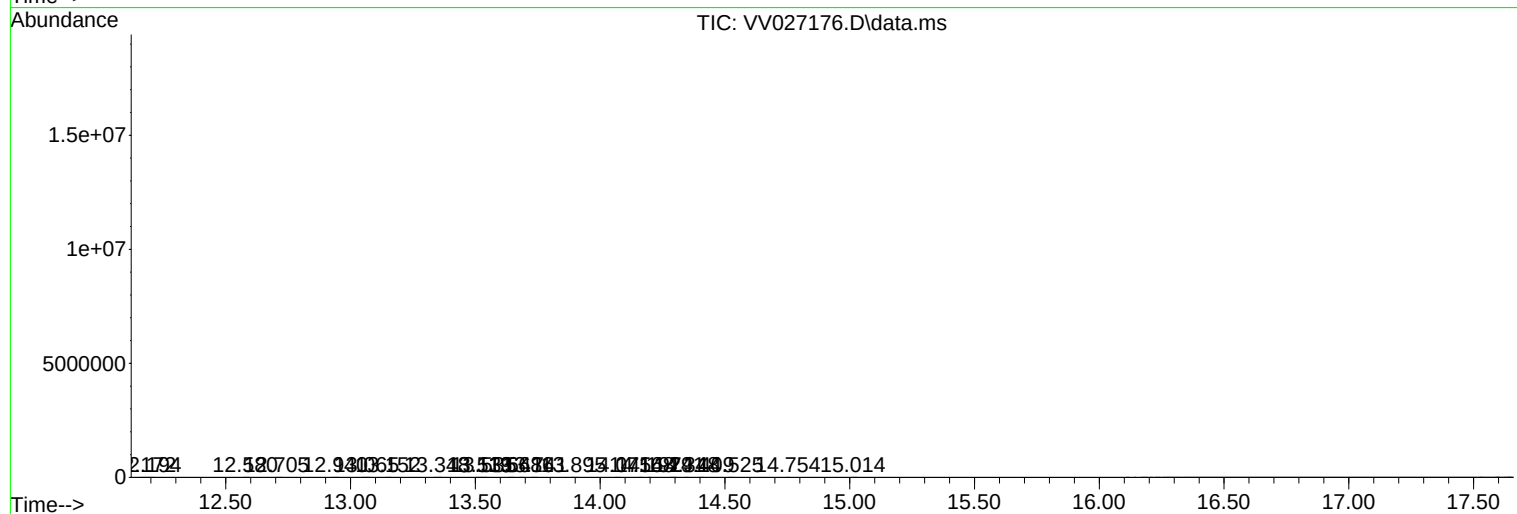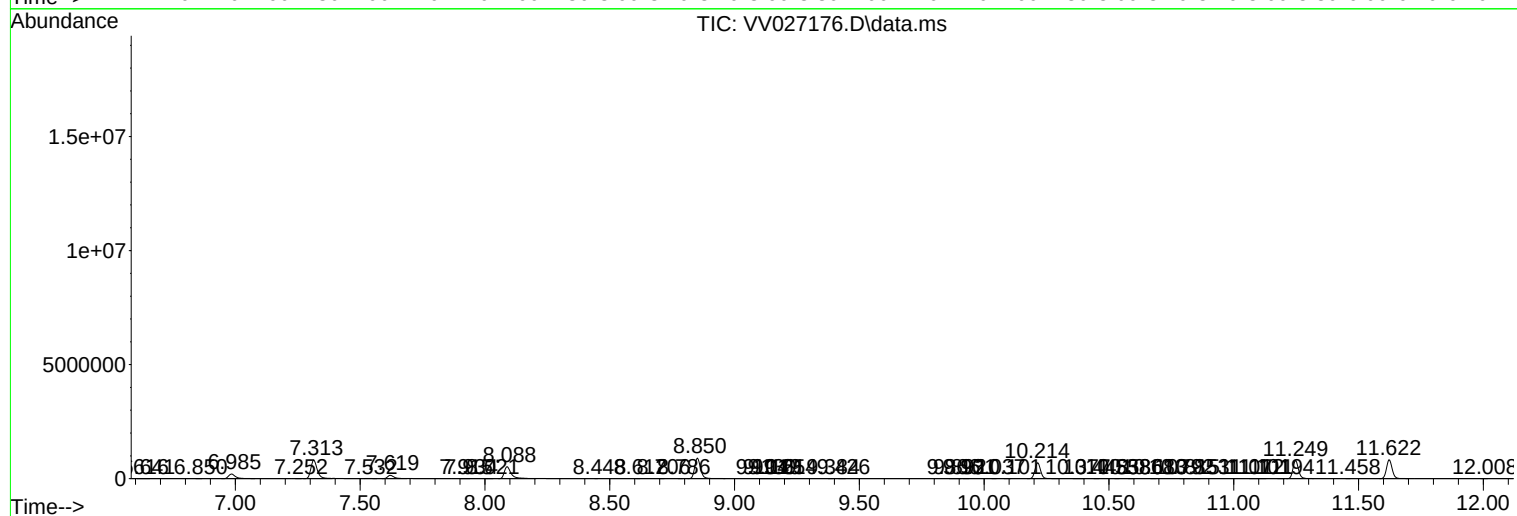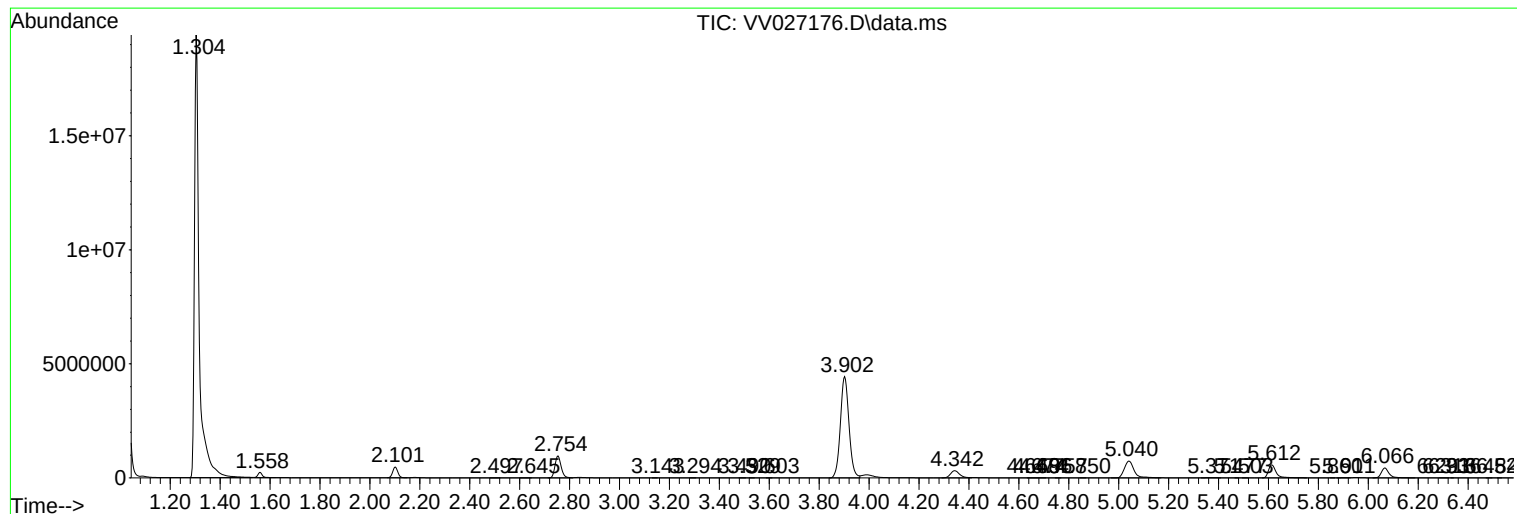

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027176.D
Acq On : 02 Aug 2022 17:21
Operator : SY/MD
Sample : N4003-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027176.D
Acq On : 02 Aug 2022 17:21
Operator : SY/MD
Sample : N4003-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------