

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027179.D
 Acq On : 02 Aug 2022 18:35
 Operator : SY/MD
 Sample : N4005-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY145

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027179.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	102	rBV2	322904	358468	5.63%	1.584%
2	1.561	154	162	176	rVB	238613	271245	4.26%	1.198%
3	2.101	320	330	345	rBV	475910	684481	10.75%	3.024%
4	2.288	383	388	400	rVB6	2857	4741	0.07%	0.021%
5	2.407	423	425	431	rVB2	436	370	0.01%	0.002%
6	2.465	438	443	445	rBV4	442	333	0.01%	0.001%
7	2.506	447	456	463	rBV6	1896	3324	0.05%	0.015%
8	2.568	468	475	487	rVB5	4597	7195	0.11%	0.032%
9	2.674	504	508	516	rBV3	427	496	0.01%	0.002%
10	2.754	521	533	553	rBV	676755	1160861	18.24%	5.129%
11	2.976	600	602	607	rBV2	645	566	0.01%	0.003%
12	3.124	645	648	654	rBV2	347	294	0.00%	0.001%
13	3.182	664	666	671	rVB2	468	337	0.01%	0.001%
14	3.256	684	689	691	rBV2	319	282	0.00%	0.001%
15	3.291	695	700	707	rVV5	954	1299	0.02%	0.006%
16	3.657	809	814	819	rBV2	421	459	0.01%	0.002%
17	3.805	858	860	866	rVB3	428	376	0.01%	0.002%
18	3.905	871	891	911	rBV2	2564885	6364342	100.00%	28.118%
19	4.342	1012	1027	1052	rBV	323896	803757	12.63%	3.551%
20	4.545	1088	1090	1096	rBV3	458	456	0.01%	0.002%
21	4.583	1099	1102	1104	rBV3	721	339	0.01%	0.001%
22	4.638	1115	1119	1120	rBV4	539	300	0.00%	0.001%
23	4.667	1121	1128	1130	rBV7	1412	1549	0.02%	0.007%
24	4.792	1164	1167	1171	rVB3	528	294	0.00%	0.001%
25	5.043	1227	1245	1291	rBV2	754377	2131018	33.48%	9.415%
26	5.323	1330	1332	1334	rBV	576	371	0.01%	0.002%
27	5.371	1342	1347	1348	rBV4	1299	1023	0.02%	0.005%
28	5.416	1359	1361	1365	rVB3	554	321	0.01%	0.001%
29	5.612	1410	1422	1463	rBV	581108	1237738	19.45%	5.468%
30	5.915	1502	1516	1542	rBV3	52332	123291	1.94%	0.545%
31	6.066	1549	1563	1598	rBV	438257	921270	14.48%	4.070%
32	6.419	1668	1673	1675	rBV3	328	312	0.00%	0.001%
33	6.481	1689	1692	1696	rBV3	365	363	0.01%	0.002%
34	6.545	1707	1712	1715	rVB2	612	402	0.01%	0.002%
35	6.699	1755	1760	1763	rVB3	487	371	0.01%	0.002%
36	6.747	1771	1775	1781	rVB3	443	452	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027179.D
 Acq On : 02 Aug 2022 18:35
 Operator : SY/MD
 Sample : N4005-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY145

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.985	1837	1849	1876	rBV	201150	383589	6.03%	1.695%
38	7.265	1932	1936	1939	rBV3	483	351	0.01%	0.002%
39	7.313	1939	1951	1974	rBV	802692	1438835	22.61%	6.357%
40	7.619	2036	2046	2067	rBV	146464	261894	4.12%	1.157%
41	7.979	2153	2158	2160	rBV3	964	676	0.01%	0.003%
42	8.030	2170	2174	2176	rBV3	624	398	0.01%	0.002%
43	8.088	2182	2192	2234	rBV	545580	1043373	16.39%	4.610%
44	8.384	2281	2284	2287	rBV2	530	457	0.01%	0.002%
45	8.458	2303	2307	2310	rBV3	407	299	0.00%	0.001%
46	8.551	2332	2336	2342	rBV5	366	312	0.00%	0.001%
47	8.606	2348	2353	2355	rBV2	394	310	0.00%	0.001%
48	8.635	2355	2362	2364	rVV5	598	743	0.01%	0.003%
49	8.651	2365	2367	2371	rVV3	833	707	0.01%	0.003%
50	8.670	2371	2373	2377	rVB2	737	467	0.01%	0.002%
51	8.760	2399	2401	2404	rVB2	591	338	0.01%	0.001%
52	8.792	2404	2411	2412	rBV2	455	513	0.01%	0.002%
53	8.850	2417	2429	2457	rBV	916501	1508468	23.70%	6.664%
54	9.021	2473	2482	2495	rVB	12323	21086	0.33%	0.093%
55	9.152	2513	2523	2531	rBV6	3717	6520	0.10%	0.029%
56	9.214	2538	2542	2545	rBV3	420	306	0.00%	0.001%
57	9.400	2598	2600	2605	rBV2	391	314	0.00%	0.001%
58	9.548	2637	2646	2654	rBV3	10037	16263	0.26%	0.072%
59	9.644	2672	2676	2679	rBV2	494	380	0.01%	0.002%
60	9.689	2686	2690	2693	rBV2	358	354	0.01%	0.002%
61	9.808	2723	2727	2729	rBV	429	318	0.00%	0.001%
62	9.937	2761	2767	2772	rBV3	1007	1305	0.02%	0.006%
63	10.114	2819	2822	2826	rVB3	378	275	0.00%	0.001%
64	10.213	2841	2853	2880	rBV	716250	1124006	17.66%	4.966%
65	10.545	2952	2956	2958	rBV3	482	392	0.01%	0.002%
66	10.738	3012	3016	3018	rBV3	404	333	0.01%	0.001%
67	10.853	3048	3052	3056	rBV4	996	741	0.01%	0.003%
68	10.921	3060	3073	3088	rVB3	4888	8557	0.13%	0.038%
69	10.982	3088	3092	3095	rBV2	439	377	0.01%	0.002%
70	11.069	3113	3119	3123	rVB3	1417	1339	0.02%	0.006%
71	11.175	3148	3152	3154	rBV3	406	322	0.01%	0.001%
72	11.249	3163	3175	3198	rBV	803183	1248113	19.61%	5.514%
73	11.532	3253	3263	3278	rBV2	16328	28982	0.46%	0.128%
74	11.622	3278	3291	3313	rBV	844879	1329272	20.89%	5.873%
75	11.747	3322	3330	3343	rVB	18153	28589	0.45%	0.126%
76	12.101	3436	3440	3443	rBV	556	506	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027179.D
 Acq On : 02 Aug 2022 18:35
 Operator : SY/MD
 Sample : N4005-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY145

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	12.236	3479	3482	3485	rBV2	413	319	0.01%	0.001%
78	12.297	3496	3501	3503	rBV3	475	383	0.01%	0.002%
79	12.371	3516	3524	3530	rBV2	3034	3228	0.05%	0.014%
80	12.471	3547	3555	3567	rBV7	4761	9445	0.15%	0.042%
81	12.715	3628	3631	3633	rBV2	603	362	0.01%	0.002%
82	12.889	3679	3685	3691	rBV4	1315	1617	0.03%	0.007%
83	12.950	3699	3704	3706	rBV4	1698	1344	0.02%	0.006%
84	13.056	3730	3737	3748	rVB5	2238	3962	0.06%	0.018%
85	13.104	3748	3752	3754	rBV3	387	315	0.00%	0.001%
86	13.188	3772	3778	3780	rBV3	619	593	0.01%	0.003%
87	13.506	3867	3877	3888	rBV2	30634	49859	0.78%	0.220%
88	13.628	3907	3915	3923	rBV	5199	7486	0.12%	0.033%
89	13.696	3933	3936	3940	rBV2	343	291	0.00%	0.001%
90	13.776	3956	3961	3964	rBV3	455	424	0.01%	0.002%
91	13.827	3975	3977	3982	rVB2	533	334	0.01%	0.001%
92	14.049	4043	4046	4048	rBV2	493	348	0.01%	0.002%
93	14.381	4146	4149	4151	rBV2	437	378	0.01%	0.002%
94	14.409	4155	4158	4164	rVB3	587	505	0.01%	0.002%
95	14.583	4206	4212	4213	rBV3	722	768	0.01%	0.003%
96	14.818	4278	4285	4297	rVB3	4079	6238	0.10%	0.028%
97	15.226	4410	4412	4416	rBV3	581	475	0.01%	0.002%
98	15.307	4433	4437	4443	rBV4	1084	1204	0.02%	0.005%
99	15.519	4501	4503	4506	rVB4	614	284	0.00%	0.001%
100	15.696	4554	4558	4561	rBV4	1081	1031	0.02%	0.005%




Sum of corrected areas: 22634669

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027179.D
Acq On : 02 Aug 2022 18:35
Operator : SY/MD
Sample : N4005-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY145

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

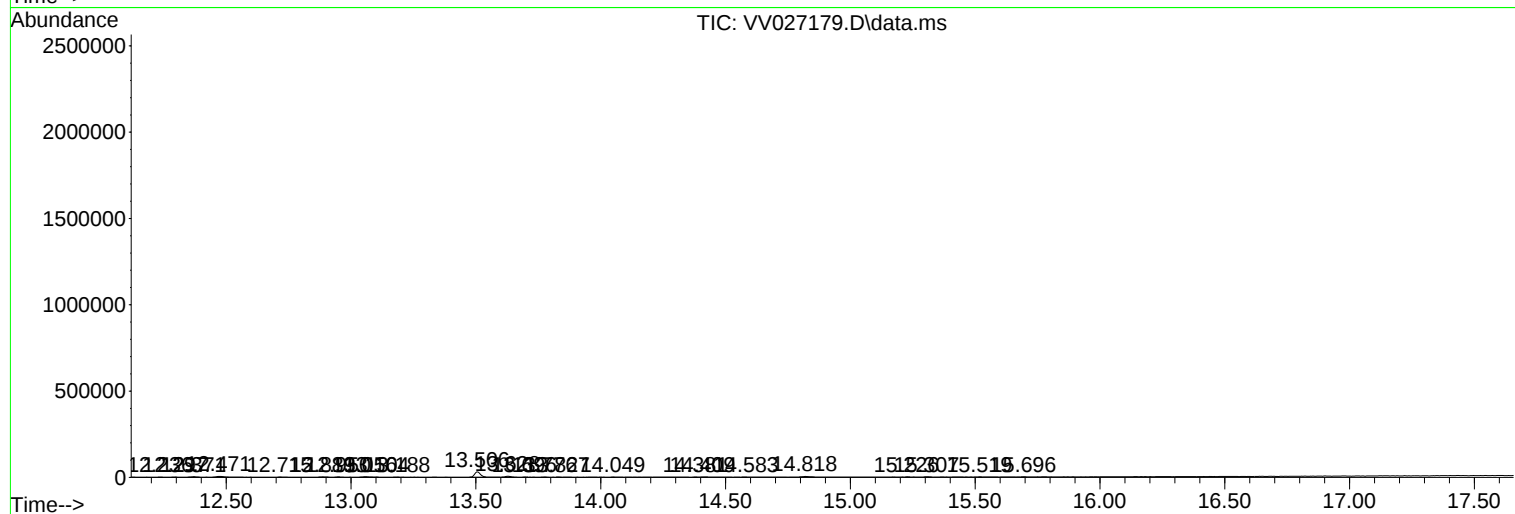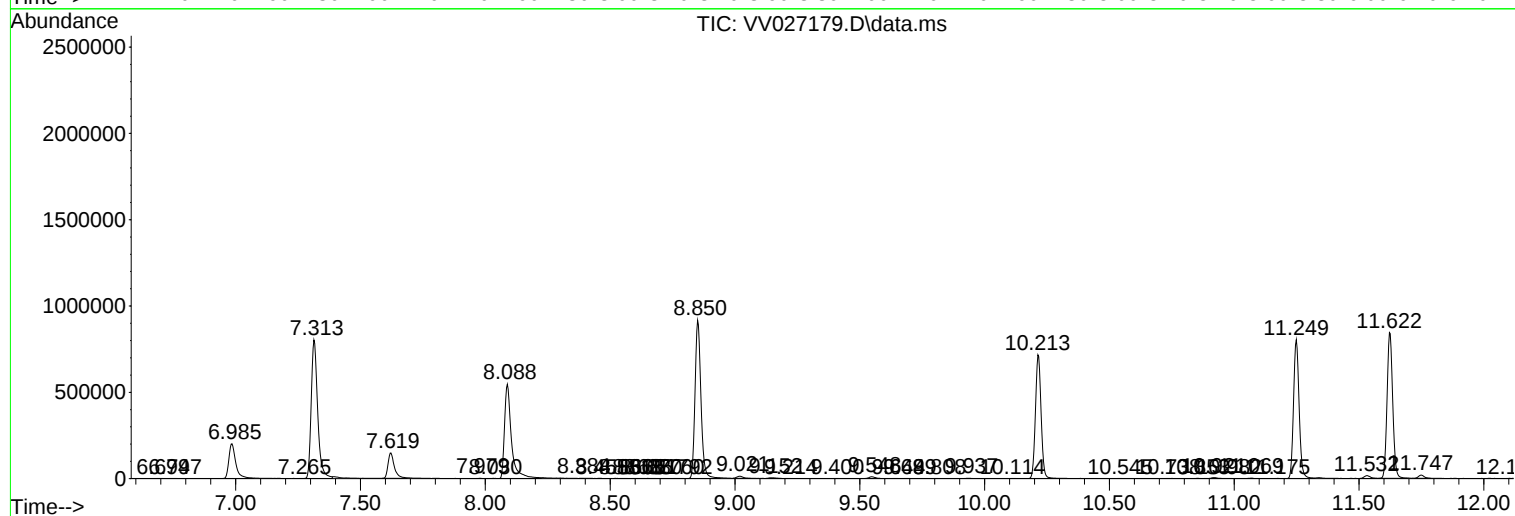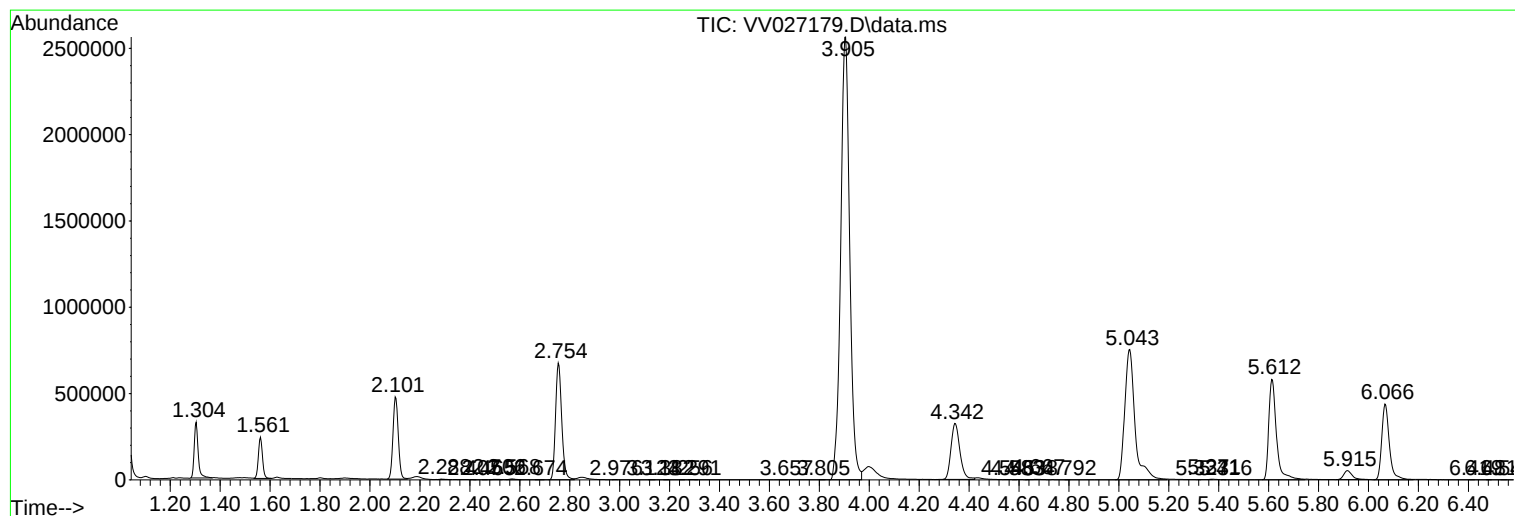

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027179.D
Acq On : 02 Aug 2022 18:35
Operator : SY/MD
Sample : N4005-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY145

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027179.D
Acq On : 02 Aug 2022 18:35
Operator : SY/MD
Sample : N4005-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY145

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------