

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027180.D
 Acq On : 02 Aug 2022 19:00
 Operator : SY/MD
 Sample : N4005-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY146

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027180.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	100	rBV	282669	303312	3.30%	1.056%
2	1.561	155	162	176	rVB	236840	268750	2.92%	0.936%
3	2.101	321	330	346	rBV	471925	674227	7.33%	2.347%
4	2.503	448	455	462	rVB6	1956	3191	0.03%	0.011%
5	2.635	494	496	503	rVB3	767	698	0.01%	0.002%
6	2.754	519	533	550	rBV	5494380	9196841	100.00%	32.015%
7	3.339	713	715	716	rBV	235	82	0.00%	0.000%
8	3.352	717	719	720	rVV2	514	156	0.00%	0.001%
9	3.362	720	722	723	rVB	390	115	0.00%	0.000%
10	3.462	750	753	755	rBV	392	231	0.00%	0.001%
11	3.564	783	785	787	rBV	190	118	0.00%	0.000%
12	3.600	794	796	798	rVB	165	69	0.00%	0.000%
13	3.616	798	801	805	rBV3	269	223	0.00%	0.001%
14	3.683	820	822	825	rBV2	250	135	0.00%	0.000%
15	3.777	849	851	854	rBV2	251	108	0.00%	0.000%
16	3.905	871	891	910	rBV2	1860414	4723384	51.36%	16.442%
17	4.343	1013	1027	1048	rBV	316134	777273	8.45%	2.706%
18	4.603	1106	1108	1110	rBV	710	295	0.00%	0.001%
19	4.773	1158	1161	1164	rVB3	543	310	0.00%	0.001%
20	4.886	1193	1196	1199	rVB3	438	272	0.00%	0.001%
21	4.912	1199	1204	1207	rBV3	420	279	0.00%	0.001%
22	4.928	1207	1209	1211	rBV2	283	150	0.00%	0.001%
23	4.944	1211	1214	1215	rBV3	265	148	0.00%	0.001%
24	5.043	1226	1245	1297	rBV2	740822	1976529	21.49%	6.880%
25	5.471	1374	1378	1382	rBV5	660	617	0.01%	0.002%
26	5.494	1382	1385	1388	rBV2	470	338	0.00%	0.001%
27	5.555	1401	1404	1406	rBV3	266	162	0.00%	0.001%
28	5.613	1410	1422	1464	rBV	560797	1203808	13.09%	4.191%
29	5.912	1502	1515	1543	rBV	264575	559363	6.08%	1.947%
30	6.066	1552	1563	1604	rVB	430724	909460	9.89%	3.166%
31	6.326	1641	1644	1647	rBV2	435	336	0.00%	0.001%
32	6.359	1652	1654	1658	rVB2	790	443	0.00%	0.002%
33	6.410	1667	1670	1671	rBV2	247	153	0.00%	0.001%
34	6.429	1675	1676	1677	rBV2	228	72	0.00%	0.000%
35	6.471	1685	1689	1693	rVB3	423	306	0.00%	0.001%
36	6.494	1693	1696	1699	rBV3	224	172	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027180.D
 Acq On : 02 Aug 2022 19:00
 Operator : SY/MD
 Sample : N4005-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY146

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	6.561	1715	1717	1720	rBV2	321	159	0.00%	0.001%
38	6.616	1731	1734	1735	rBV2	196	107	0.00%	0.000%
39	6.658	1745	1747	1748	rVB	399	94	0.00%	0.000%
40	6.670	1750	1751	1754	rBV	208	129	0.00%	0.000%
41	6.715	1764	1765	1771	rVB2	595	319	0.00%	0.001%
42	6.741	1771	1773	1775	rBV2	306	157	0.00%	0.001%
43	6.770	1778	1782	1784	rVV2	415	304	0.00%	0.001%
44	6.789	1787	1788	1791	rVB	317	128	0.00%	0.000%
45	6.876	1811	1815	1817	rBV3	170	101	0.00%	0.000%
46	6.889	1817	1819	1821	rBV	163	94	0.00%	0.000%
47	6.982	1837	1848	1873	rBV	195725	378355	4.11%	1.317%
48	7.204	1915	1917	1922	rBV3	527	470	0.01%	0.002%
49	7.313	1939	1951	1991	rBV	789667	1436540	15.62%	5.001%
50	7.619	2036	2046	2076	rBV	144065	260729	2.83%	0.908%
51	7.867	2121	2123	2125	rBV2	341	130	0.00%	0.000%
52	7.934	2140	2144	2145	rBV2	350	258	0.00%	0.001%
53	8.008	2165	2167	2169	rBV	234	113	0.00%	0.000%
54	8.088	2181	2192	2231	rBV	525395	1007455	10.95%	3.507%
55	8.632	2356	2361	2362	rBV2	434	392	0.00%	0.001%
56	8.812	2414	2417	2418	rBV2	541	279	0.00%	0.001%
57	8.850	2418	2429	2457	rBV	885132	1457347	15.85%	5.073%
58	9.178	2529	2531	2533	rBV2	470	241	0.00%	0.001%
59	9.233	2545	2548	2550	rBV	374	191	0.00%	0.001%
60	9.246	2550	2552	2557	rVB3	541	407	0.00%	0.001%
61	9.272	2557	2560	2565	rVB3	306	241	0.00%	0.001%
62	9.297	2565	2568	2569	rBV3	221	132	0.00%	0.000%
63	9.374	2589	2592	2596	rBV3	659	551	0.01%	0.002%
64	9.410	2599	2603	2604	rBV	298	202	0.00%	0.001%
65	9.522	2636	2638	2641	rVV	340	167	0.00%	0.001%
66	9.548	2644	2646	2648	rBV	263	144	0.00%	0.001%
67	9.616	2662	2667	2670	rBV3	169	172	0.00%	0.001%
68	9.654	2676	2679	2683	rBV2	235	161	0.00%	0.001%
69	9.677	2683	2686	2689	rVB3	293	159	0.00%	0.001%
70	9.696	2689	2692	2694	rBV	282	198	0.00%	0.001%
71	9.863	2741	2744	2745	rBV	211	141	0.00%	0.000%
72	9.992	2781	2784	2787	rBV2	250	167	0.00%	0.001%
73	10.008	2787	2789	2792	rVV2	331	228	0.00%	0.001%
74	10.043	2796	2800	2804	rVV2	278	240	0.00%	0.001%
75	10.075	2809	2810	2811	rBV	467	109	0.00%	0.000%
76	10.156	2833	2835	2837	rBV	202	117	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027180.D
 Acq On : 02 Aug 2022 19:00
 Operator : SY/MD
 Sample : N4005-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY146

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	10.214	2841	2853	2880	rVV	702005	1101383	11.98%	3.834%
78	10.362	2897	2899	2903	rBV3	437	310	0.00%	0.001%
79	10.471	2930	2933	2937	rBV3	385	320	0.00%	0.001%
80	10.583	2963	2968	2971	rBV4	535	502	0.01%	0.002%
81	10.670	2992	2995	2998	rBV2	333	324	0.00%	0.001%
82	10.702	3004	3005	3008	rBV3	304	109	0.00%	0.000%
83	10.747	3017	3019	3022	rVB	319	125	0.00%	0.000%
84	10.886	3061	3062	3063	rBV	481	113	0.00%	0.000%
85	10.911	3068	3070	3072	rBV2	306	163	0.00%	0.001%
86	10.947	3079	3081	3084	rBV	387	239	0.00%	0.001%
87	11.008	3097	3100	3106	rVB2	240	180	0.00%	0.001%
88	11.034	3106	3108	3109	rBV	165	74	0.00%	0.000%
89	11.069	3117	3119	3120	rBV	206	78	0.00%	0.000%
90	11.156	3141	3146	3148	rBV3	482	427	0.00%	0.001%
91	11.188	3154	3156	3157	rBV2	313	79	0.00%	0.000%
92	11.249	3163	3175	3204	rBV	750226	1186902	12.91%	4.132%
93	11.622	3280	3291	3314	rBV	814266	1283894	13.96%	4.469%
94	12.111	3440	3443	3444	rBV2	293	184	0.00%	0.001%
95	12.407	3531	3535	3536	rBV	441	289	0.00%	0.001%
96	12.886	3682	3684	3685	rBV	375	114	0.00%	0.000%
97	13.275	3802	3805	3807	rBV	606	330	0.00%	0.001%
98	13.394	3841	3842	3846	rBV2	334	199	0.00%	0.001%
99	13.426	3849	3852	3853	rBV2	491	251	0.00%	0.001%
100	14.892	4305	4308	4309	rBV2	871	559	0.01%	0.002%




Sum of corrected areas: 28726902

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027180.D
Acq On : 02 Aug 2022 19:00
Operator : SY/MD
Sample : N4005-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY146

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

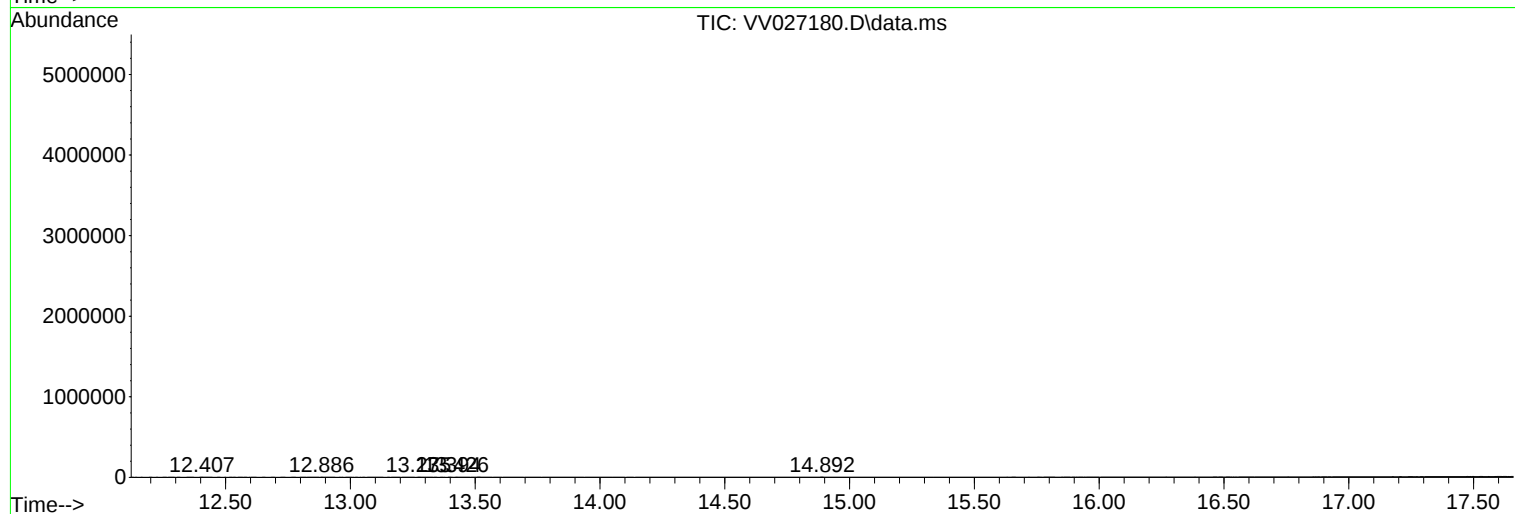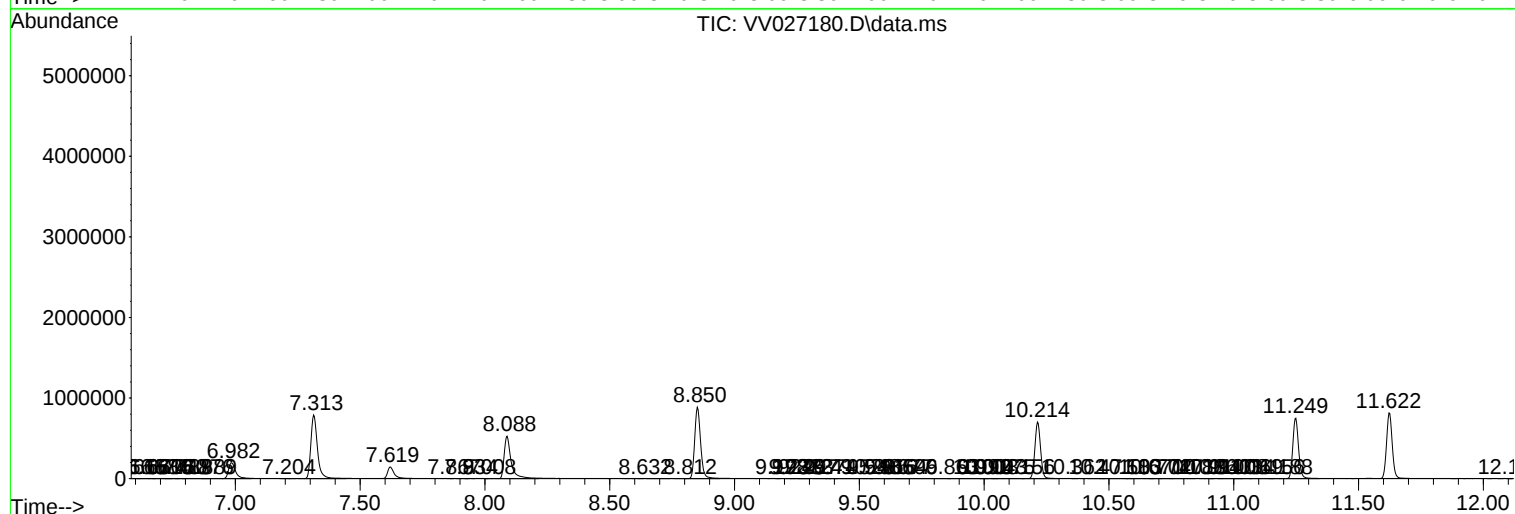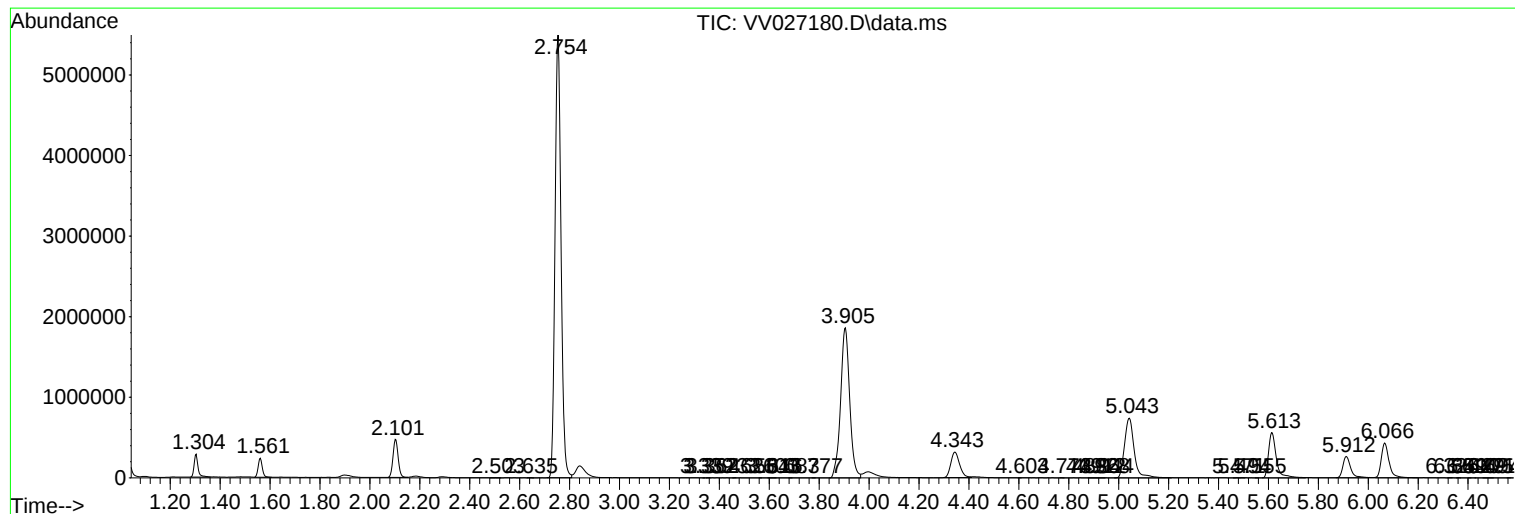

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027180.D
Acq On : 02 Aug 2022 19:00
Operator : SY/MD
Sample : N4005-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY146

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027180.D
Acq On : 02 Aug 2022 19:00
Operator : SY/MD
Sample : N4005-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY146

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------