

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027184.D
 Acq On : 02 Aug 2022 20:38
 Operator : SY/MD
 Sample : VIBLK269
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK269

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

Signal : TIC: VV027184.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	100	rBV	289856	303114	14.51%	1.846%
2	1.561	155	162	180	rVB	243840	283279	13.56%	1.725%
3	2.101	320	330	346	rBV	493037	700540	33.52%	4.267%
4	2.291	382	389	398	rBV2	5828	8223	0.39%	0.050%
5	2.503	446	455	468	rVB2	6113	9932	0.48%	0.060%
6	2.609	480	488	492	rBV3	2512	3792	0.18%	0.023%
7	2.757	524	534	548	rBV	20668	37402	1.79%	0.228%
8	2.847	560	562	567	rVB2	398	279	0.01%	0.002%
9	2.899	573	578	581	rBV3	293	304	0.01%	0.002%
10	3.214	670	676	679	rBV3	260	290	0.01%	0.002%
11	3.365	720	723	729	rVB3	284	274	0.01%	0.002%
12	3.394	729	732	736	rBV2	351	262	0.01%	0.002%
13	3.651	806	812	820	rBV	512	773	0.04%	0.005%
14	3.876	871	882	922	rBV2	185227	595396	28.49%	3.627%
15	4.342	1011	1027	1069	rBV	333619	851785	40.76%	5.188%
16	4.600	1105	1107	1113	rVB4	342	312	0.01%	0.002%
17	4.661	1120	1126	1135	rBV7	1690	2217	0.11%	0.014%
18	4.699	1136	1138	1143	rVV3	648	532	0.03%	0.003%
19	4.744	1150	1152	1156	rVB3	355	292	0.01%	0.002%
20	4.834	1172	1180	1182	rBV4	801	936	0.04%	0.006%
21	4.940	1209	1213	1216	rVB2	335	275	0.01%	0.002%
22	5.043	1227	1245	1294	rBV2	787519	2089702	100.00%	12.728%
23	5.612	1410	1422	1459	rBV	656703	1393261	66.67%	8.486%
24	5.866	1499	1501	1503	rVB2	573	250	0.01%	0.002%
25	5.908	1503	1514	1533	rBV6	12835	29066	1.39%	0.177%
26	6.066	1548	1563	1591	rBV	447168	952626	45.59%	5.802%
27	6.291	1629	1633	1637	rVB4	682	564	0.03%	0.003%
28	6.313	1638	1640	1645	rVB3	534	389	0.02%	0.002%
29	6.812	1789	1795	1797	rBV	300	328	0.02%	0.002%
30	6.847	1802	1806	1809	rBV2	370	292	0.01%	0.002%
31	6.928	1828	1831	1833	rBV	563	315	0.02%	0.002%
32	6.982	1836	1848	1881	rBV	212339	408554	19.55%	2.488%
33	7.198	1911	1915	1920	rVB3	467	323	0.02%	0.002%
34	7.313	1939	1951	1985	rBV	861191	1560894	74.69%	9.507%
35	7.619	2036	2046	2076	rBV	148867	277820	13.29%	1.692%
36	7.767	2089	2092	2096	rBV5	494	425	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027184.D
 Acq On : 02 Aug 2022 20:38
 Operator : SY/MD
 Sample : VIBLK269
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK269

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

37	7.805	2101	2104	2106	rBV3	575	342	0.02%	0.002%
38	7.834	2112	2113	2118	rBV3	355	257	0.01%	0.002%
39	7.905	2131	2135	2138	rBV3	448	426	0.02%	0.003%
40	7.979	2152	2158	2170	rBV5	3216	5422	0.26%	0.033%
41	8.027	2170	2173	2176	rBV2	482	255	0.01%	0.002%
42	8.088	2181	2192	2236	rBV	562121	1085403	51.94%	6.611%
43	8.355	2272	2275	2286	rVB6	1264	1823	0.09%	0.011%
44	8.477	2310	2313	2319	rVB3	726	595	0.03%	0.004%
45	8.702	2380	2383	2390	rVB2	285	267	0.01%	0.002%
46	8.735	2390	2393	2397	rBV4	490	338	0.02%	0.002%
47	8.850	2417	2429	2462	rBV	1006550	1674117	80.11%	10.197%
48	9.117	2506	2512	2515	rVV5	582	581	0.03%	0.004%
49	9.152	2515	2523	2535	rVB7	2156	4394	0.21%	0.027%
50	9.313	2571	2573	2576	rVB2	546	287	0.01%	0.002%
51	9.397	2594	2599	2602	rBV2	398	330	0.02%	0.002%
52	9.551	2644	2647	2649	rBV2	781	633	0.03%	0.004%
53	9.757	2706	2711	2713	rBV2	580	488	0.02%	0.003%
54	9.937	2759	2767	2778	rBV3	2450	3468	0.17%	0.021%
55	10.120	2822	2824	2829	rVB2	372	272	0.01%	0.002%
56	10.214	2841	2853	2877	rBV	718835	1137809	54.45%	6.930%
57	10.345	2890	2894	2897	rBV3	334	265	0.01%	0.002%
58	10.387	2905	2907	2910	rBV2	413	261	0.01%	0.002%
59	10.542	2949	2955	2956	rBV	1268	820	0.04%	0.005%
60	10.850	3046	3051	3056	rBV4	978	956	0.05%	0.006%
61	10.918	3066	3072	3080	rBV4	918	1430	0.07%	0.009%
62	10.985	3091	3093	3100	rVB	466	399	0.02%	0.002%
63	11.075	3118	3121	3126	rVB2	445	366	0.02%	0.002%
64	11.188	3145	3156	3163	rBV6	5018	7892	0.38%	0.048%
65	11.249	3163	3175	3202	rVV	894701	1429601	68.41%	8.708%
66	11.622	3279	3291	3316	rBV	901069	1417571	67.84%	8.634%
67	11.773	3335	3338	3341	rVB5	761	474	0.02%	0.003%
68	11.831	3353	3356	3359	rBV3	589	335	0.02%	0.002%
69	11.982	3399	3403	3407	rVB3	467	299	0.01%	0.002%
70	12.040	3416	3421	3424	rBV2	407	332	0.02%	0.002%
71	12.059	3424	3427	3434	rBV2	683	454	0.02%	0.003%
72	12.281	3491	3496	3498	rBV2	446	435	0.02%	0.003%
73	12.429	3534	3542	3545	rBV6	1445	1877	0.09%	0.011%
74	12.480	3556	3558	3564	rVB3	313	249	0.01%	0.002%
75	12.567	3582	3585	3589	rVB2	390	296	0.01%	0.002%
76	12.651	3602	3611	3624	rBV5	6692	10933	0.52%	0.067%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027184.D
 Acq On : 02 Aug 2022 20:38
 Operator : SY/MD
 Sample : VIBLK269
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK269

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis

77	12.705	3626	3628	3632	rVB2	752	392	0.02%	0.002%
78	12.812	3657	3661	3665	rBV2	385	460	0.02%	0.003%
79	12.882	3680	3683	3687	rVB3	650	494	0.02%	0.003%
80	13.037	3726	3731	3735	rBV2	368	374	0.02%	0.002%
81	13.136	3758	3762	3765	rBV	288	272	0.01%	0.002%
82	13.175	3772	3774	3777	rBV	398	255	0.01%	0.002%
83	13.265	3794	3802	3817	rVB3	10278	16659	0.80%	0.101%
84	13.326	3817	3821	3824	rBV3	364	376	0.02%	0.002%
85	13.413	3845	3848	3850	rBV2	401	273	0.01%	0.002%
86	13.458	3857	3862	3867	rBV3	422	586	0.03%	0.004%
87	13.503	3867	3876	3893	rBV	36881	62369	2.98%	0.380%
88	13.644	3917	3920	3926	rBV3	595	523	0.03%	0.003%
89	13.709	3936	3940	3942	rBV2	638	473	0.02%	0.003%
90	13.744	3942	3951	3962	rVB3	13481	21396	1.02%	0.130%
91	13.824	3973	3976	3979	rBV2	338	277	0.01%	0.002%
92	13.863	3985	3988	3993	rVB2	426	431	0.02%	0.003%
93	13.956	4013	4017	4020	rBV3	512	447	0.02%	0.003%
94	14.062	4046	4050	4054	rBV3	474	468	0.02%	0.003%
95	14.146	4074	4076	4079	rVB2	602	289	0.01%	0.002%
96	14.217	4096	4098	4101	rBV2	356	252	0.01%	0.002%
97	14.760	4263	4267	4269	rBV3	468	385	0.02%	0.002%
98	14.824	4283	4287	4288	rBV2	1167	707	0.03%	0.004%
99	15.416	4466	4471	4474	rBV4	950	1010	0.05%	0.006%
100	15.834	4597	4601	4602	rBV4	1141	805	0.04%	0.005%


Sum of corrected areas: 16417743

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027184.D
Acq On : 02 Aug 2022 20:38
Operator : SY/MD
Sample : VIBLK269
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK269

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

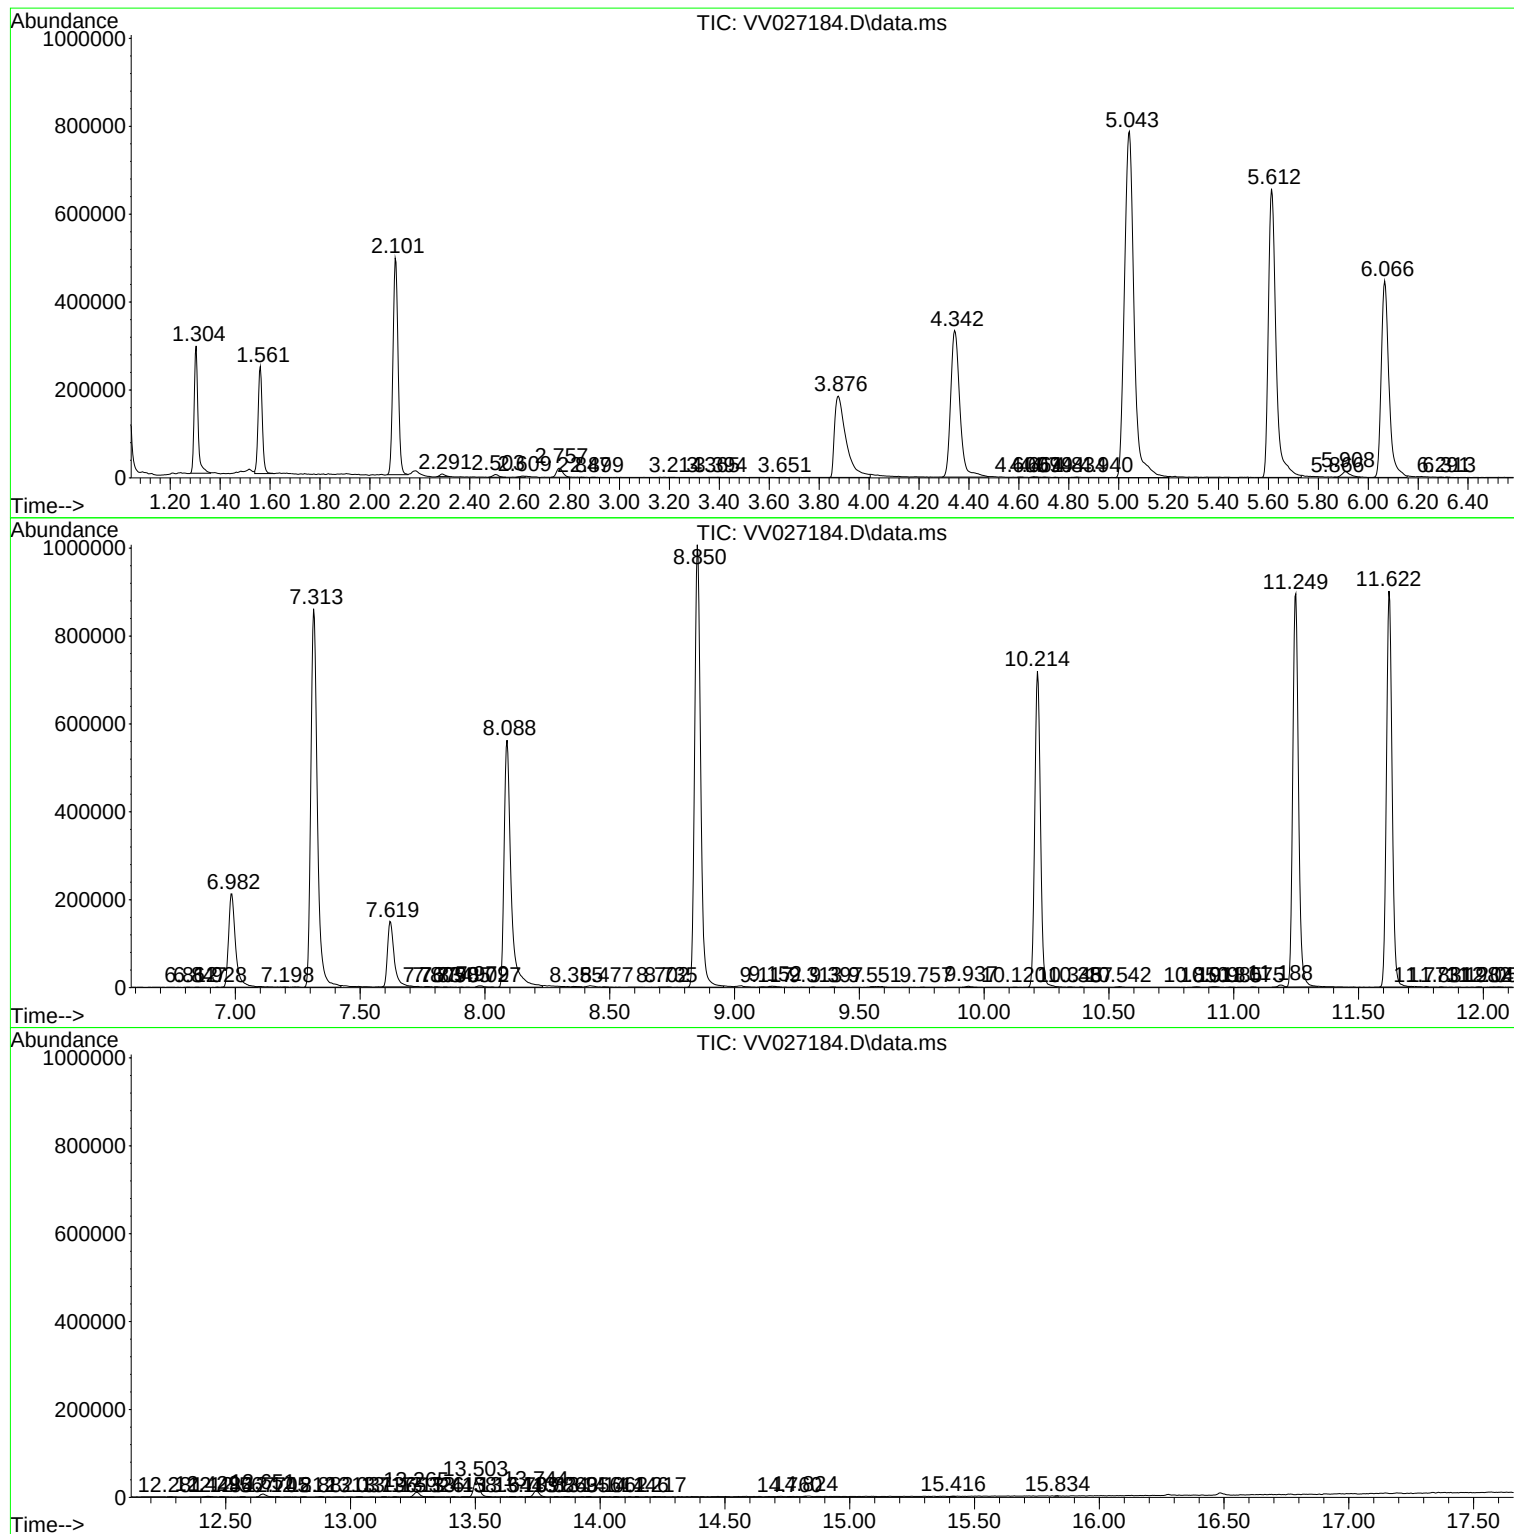

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027184.D
Acq On : 02 Aug 2022 20:38
Operator : SY/MD
Sample : VIBLK269
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK269

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
Data File : VV027184.D
Acq On : 02 Aug 2022 20:38
Operator : SY/MD
Sample : VIBLK269
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK269

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
