
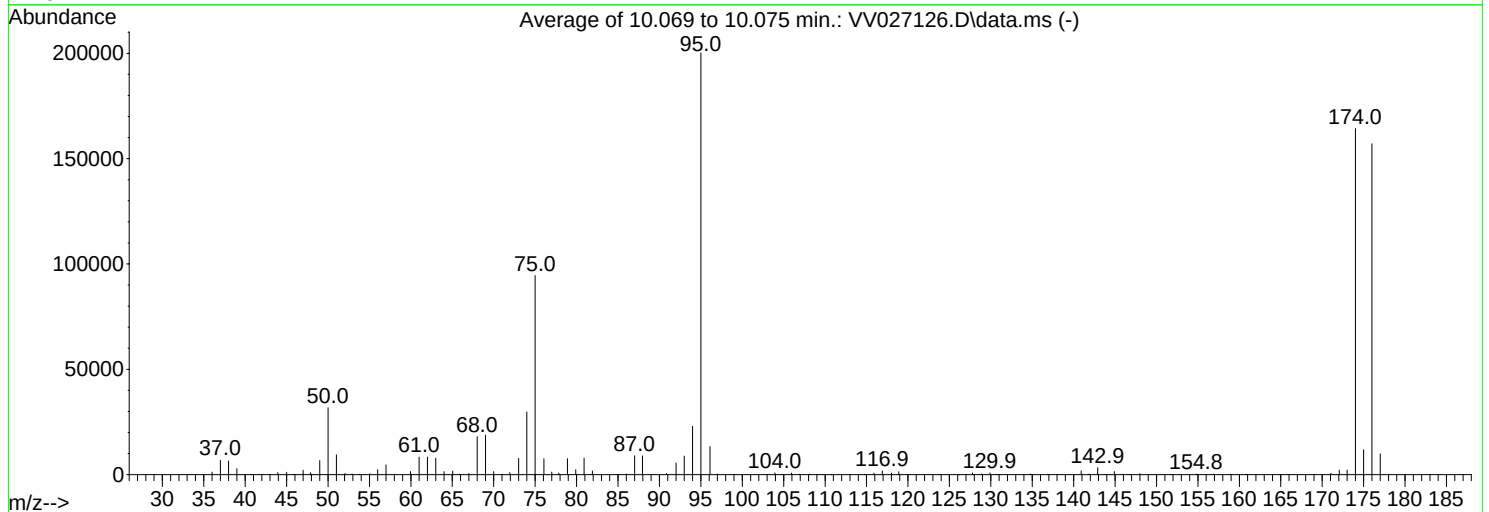


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080122\
 Data File : VV027126.D
 Acq On : 01 Aug 2022 10:55
 Operator : SY/MD
 Sample : BFB303
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB303

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080122WMA.M
 Title : VOC Analysis
 Last Update : Wed Aug 03 02:00:39 2022

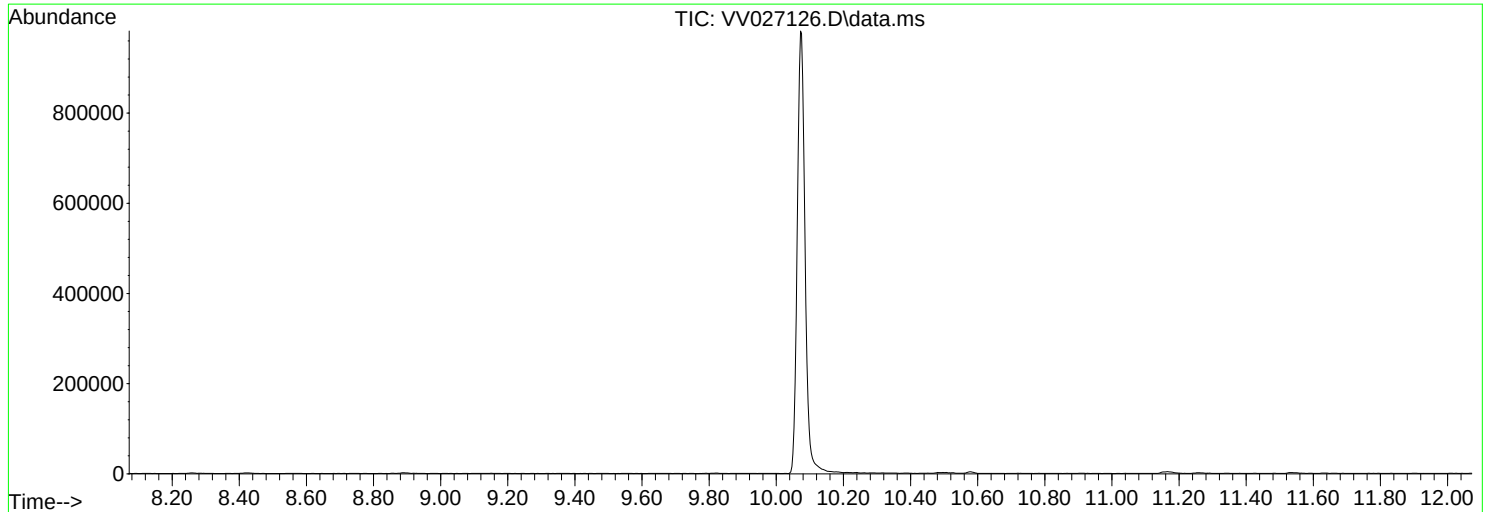

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	31717	PASS
75	95	30	80	47.2	94496	PASS
95	95	100	100	100.0	200213	PASS
96	95	5	9	6.7	13374	PASS
173	174	0.00	2	1.4	2223	PASS
174	95	50	120	82.1	164309	PASS
175	174	5	9	7.2	11785	PASS
176	174	95	105	95.6	157056	PASS
177	176	5	10	6.3	9906	PASS

m/z	Abundance
39.90	318.0
44.00	512.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303

m/z	Abundance
36.00	1147.0
37.00	6476.0
38.00	6331.0
39.00	2822.0
43.00	158.0
43.90	1418.0
45.00	1071.0
45.90	251.0
47.00	2188.0
47.90	825.0
49.00	6666.0
50.00	30352.0
51.00	9109.0
52.00	637.0
52.90	259.0
53.80	126.0
55.00	449.0
56.00	2466.0
57.00	4314.0
58.00	213.0
59.90	1500.0
61.00	8010.0
62.00	7865.0
63.00	7647.0
64.00	1460.0
65.10	1687.0
65.90	328.0
67.00	538.0
68.00	17376.0
69.00	17928.0
70.00	1400.0
71.00	125.0
71.90	896.0
73.00	7347.0
74.00	27992.0
75.00	89000.0
76.00	7376.0
77.00	1217.0
77.80	790.0
78.90	7355.0
79.90	2198.0
80.90	7692.0
81.90	1589.0
83.10	151.0
86.00	422.0
87.00	8606.0
87.90	8371.0
90.90	529.0
92.00	5148.0
93.00	8472.0
94.00	21728.0
95.00	190464.0
96.10	13072.0
97.00	394.0
104.00	895.0
104.90	265.0
106.00	720.0
106.90	262.0
108.10	254.0
109.70	166.0
110.70	142.0
111.90	106.0
112.90	174.0
114.80	132.0
115.90	788.0
116.90	1574.0
118.00	802.0
118.90	1350.0
124.00	104.0
127.80	738.0
128.90	355.0
129.90	875.0
130.80	279.0
134.80	414.0
136.90	246.0
140.90	1693.0
141.80	333.0
142.90	3149.0
143.90	304.0
144.90	1230.0
146.00	261.0
146.70	133.0
148.00	476.0
149.90	223.0
151.70	140.0
153.00	110.0
154.80	469.0
156.90	355.0
159.00	212.0
160.80	212.0
171.10	613.0
172.10	1899.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303

173.00	2098.0
174.00	150080.0
175.00	11185.0
176.00	143488.0
177.00	9184.0
178.10	296.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303

m/z	Abundance
36.00	1297.0
37.00	7113.0
38.00	6685.0
39.00	2982.0
40.00	553.0
43.00	142.0
44.00	1568.0
45.00	1170.0
45.90	262.0
47.00	2106.0
47.90	941.0
49.00	6933.0
50.00	33016.0
51.00	9771.0
52.00	604.0
52.90	297.0
53.80	200.0
55.00	446.0
56.00	2432.0
57.00	4841.0
58.00	294.0
59.90	1502.0
61.00	8578.0
62.00	8521.0
63.00	8088.0
64.00	1450.0
65.00	1824.0
65.90	339.0
67.00	567.0
68.00	18664.0
69.00	19400.0
70.00	1454.0
71.00	146.0
72.00	1015.0
73.00	8046.0
74.00	30616.0
75.00	97768.0
76.00	7783.0
77.00	1291.0
77.90	802.0
78.90	7872.0
79.90	2418.0
80.90	8110.0
81.90	1830.0
82.90	139.0
86.00	409.0
87.00	9358.0
88.00	9195.0
90.90	535.0
92.00	5717.0
93.00	9079.0
94.00	23624.0
95.00	206656.0
96.10	13944.0
97.00	377.0
103.90	881.0
104.90	251.0
106.00	778.0
106.90	292.0
108.10	279.0
109.70	198.0
111.00	128.0
111.90	145.0
112.90	183.0
114.80	167.0
115.90	803.0
116.90	1798.0
118.00	815.0
118.90	1447.0
123.80	133.0
127.80	884.0
128.90	398.0
129.90	913.0
131.00	237.0
134.80	329.0
136.90	262.0
140.90	1857.0
141.90	326.0
142.90	3415.0
143.90	266.0
144.90	1449.0
145.90	327.0
148.00	471.0
150.00	265.0
151.80	149.0
153.00	134.0
154.80	570.0
156.90	332.0
159.00	207.0
160.90	272.0
171.00	637.0
172.00	2137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303

173.00	2283.0
174.00	169792.0
175.00	12206.0
176.00	162304.0
177.00	10185.0
178.10	289.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303

m/z	Abundance
36.00	1266.0
37.00	6856.0
38.00	6316.0
39.00	2848.0
40.00	524.0
40.70	121.0
43.00	117.0
44.00	1549.0
45.00	1203.0
45.90	241.0
47.00	2090.0
47.90	954.0
49.00	6384.0
50.00	31784.0
51.00	9496.0
52.10	477.0
52.90	287.0
53.80	241.0
55.10	430.0
56.00	2169.0
57.00	4869.0
58.00	286.0
60.00	1439.0
61.00	8477.0
62.00	8679.0
63.00	7833.0
64.00	1352.0
65.00	1827.0
65.90	307.0
67.00	523.0
68.00	18120.0
69.00	18896.0
70.00	1404.0
71.00	152.0
72.00	1075.0
73.00	7880.0
74.00	30624.0
75.00	96720.0
76.10	7615.0
77.00	1199.0
77.90	753.0
78.90	7543.0
79.90	2448.0
80.90	7803.0
81.90	1923.0
82.90	165.0
86.00	364.0
87.00	8985.0
88.00	9199.0
90.80	529.0
92.00	5815.0
93.00	8861.0
94.00	23528.0
95.00	203520.0
96.10	13107.0
97.00	300.0
103.90	846.0
104.90	262.0
105.90	796.0
106.90	233.0
108.10	240.0
109.80	181.0
111.00	153.0
112.00	147.0
113.00	166.0
114.80	198.0
115.90	741.0
116.90	1778.0
118.00	718.0
118.90	1408.0
123.70	141.0
126.10	110.0
127.80	975.0
128.90	446.0
129.90	820.0
131.00	269.0
134.80	282.0
136.90	253.0
140.90	1859.0
141.90	258.0
142.90	3241.0
143.90	187.0
144.90	1557.0
145.90	337.0
148.00	460.0
150.00	248.0
151.80	127.0
152.90	151.0
155.00	635.0
156.90	308.0
158.90	210.0
160.90	292.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303

171.00	578.0
172.00	2392.0
173.00	2287.0
174.00	173056.0
175.00	11964.0
176.00	165376.0
177.00	10350.0
178.00	238.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303