
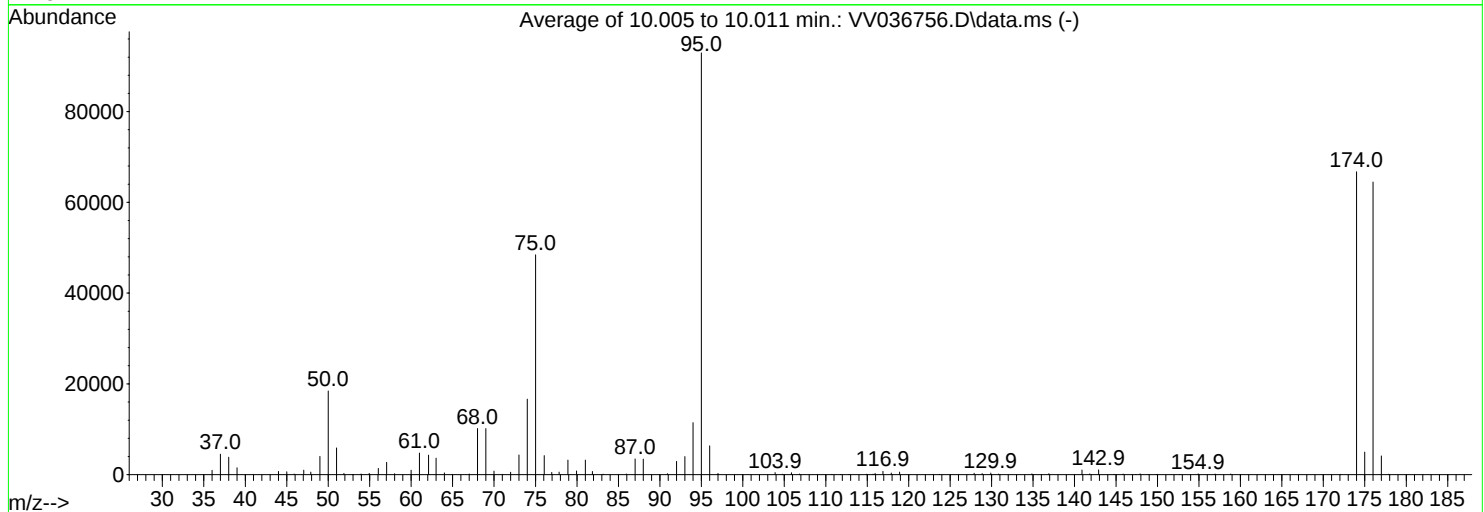


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080224\
Data File : VV036756.D
Acq On : 02 Aug 2024 08:22
Operator : SY/MD
Sample : BFB353
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB353

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Jan 11 01:51:56 2022

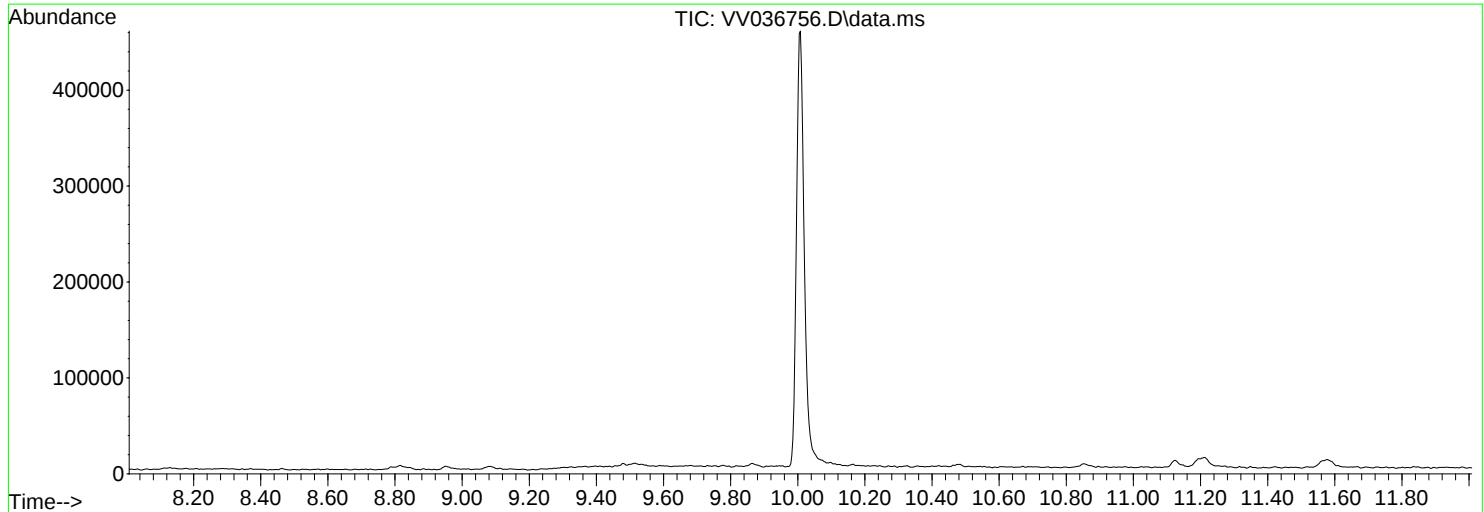

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	18451	PASS
75	95	30	80	52.1	48429	PASS
95	95	100	100	100.0	92944	PASS
96	95	5	9	6.8	6347	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.8	66741	PASS
175	174	5	9	7.5	4978	PASS
176	174	95	105	96.6	64493	PASS
177	176	5	10	6.4	4117	PASS

m/z	Abundance
36.00	1787.0
37.00	209.0
38.00	645.0
39.20	199.0
39.90	339.0
41.00	316.0
41.90	277.0
43.00	365.0
44.00	1011.0
44.80	121.0
45.20	148.0
52.90	107.0
55.00	257.0
56.10	146.0
57.10	209.0
60.20	104.0
67.00	147.0
69.00	175.0
71.00	127.0
77.00	229.0
79.10	119.0
83.00	120.0
91.00	107.0
104.90	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB353

m/z	Abundance
36.00	2729.0
37.00	4905.0
38.00	4691.0
39.00	1727.0
40.00	302.0
40.90	266.0
41.90	176.0
43.10	361.0
44.00	1774.0
45.00	961.0
45.90	140.0
47.00	1005.0
47.90	575.0
49.00	4227.0
50.00	19128.0
51.00	6366.0
51.90	311.0
52.90	140.0
53.90	158.0
55.00	565.0
56.10	1592.0
57.00	2967.0
58.00	222.0
60.00	1158.0
61.00	5055.0
62.10	4658.0
63.00	3999.0
64.00	409.0
67.10	340.0
68.00	10344.0
69.00	10767.0
70.00	832.0
71.10	163.0
72.00	547.0
73.00	4365.0
74.00	17296.0
75.00	50536.0
76.10	4302.0
76.90	760.0
77.80	528.0
78.90	3449.0
80.00	891.0
81.00	3221.0
81.80	701.0
83.20	186.0
86.00	123.0
87.00	3597.0
88.00	3587.0
90.90	336.0
92.00	3006.0
93.00	4214.0
94.00	11665.0
95.00	95392.0
96.00	6732.0
97.00	344.0
103.90	439.0
104.80	216.0
105.80	428.0
106.90	149.0
110.80	134.0
111.80	113.0
112.80	107.0
115.00	113.0
116.00	457.0
116.90	763.0
118.00	337.0
118.90	600.0
127.90	305.0
128.80	262.0
129.90	336.0
130.80	126.0
135.00	177.0
136.90	206.0
140.90	1090.0
141.90	190.0
142.90	1101.0
145.90	126.0
147.90	190.0
149.90	111.0
152.70	123.0
154.90	184.0
156.90	194.0
158.80	152.0
172.10	196.0
174.00	66384.0
175.00	5108.0
176.00	65112.0
177.00	4221.0
177.90	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB353

m/z	Abundance
36.00	2780.0
37.00	4904.0
38.00	4632.0
39.00	1752.0
39.90	298.0
40.90	208.0
41.90	220.0
43.10	350.0
44.00	1705.0
45.00	901.0
45.90	152.0
47.00	1011.0
47.90	569.0
49.00	4151.0
50.00	19000.0
51.00	6114.0
51.90	279.0
52.90	119.0
54.00	134.0
55.00	527.0
56.00	1593.0
57.10	3014.0
58.00	215.0
60.00	1111.0
61.00	4875.0
62.10	4396.0
63.00	3766.0
64.00	412.0
67.10	305.0
68.00	10578.0
69.00	10714.0
70.00	794.0
71.10	216.0
72.00	544.0
73.00	4540.0
74.00	17296.0
75.00	49824.0
76.10	4289.0
76.90	755.0
77.90	613.0
78.90	3467.0
80.00	818.0
81.00	3334.0
81.90	728.0
83.10	194.0
85.90	145.0
87.00	3503.0
88.00	3479.0
90.90	322.0
92.00	3030.0
93.00	4057.0
94.00	11897.0
95.00	96056.0
96.00	6547.0
97.00	302.0
103.90	497.0
104.80	244.0
105.90	454.0
106.80	140.0
110.70	111.0
114.90	106.0
115.90	359.0
116.90	760.0
117.90	352.0
118.90	609.0
123.70	121.0
127.90	329.0
128.90	259.0
129.90	349.0
130.80	152.0
134.80	164.0
136.90	230.0
140.90	1081.0
141.90	180.0
142.90	1117.0
144.70	114.0
145.80	145.0
147.40	104.0
147.90	169.0
154.90	201.0
156.90	149.0
158.90	142.0
174.00	68992.0
175.00	5217.0
176.00	66832.0
177.00	4280.0
177.90	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB353

m/z	Abundance
36.00	2761.0
37.00	4397.0
38.00	4170.0
39.00	1656.0
39.90	300.0
41.00	220.0
41.90	226.0
43.10	352.0
44.00	1673.0
45.00	845.0
45.90	151.0
47.10	1005.0
47.90	564.0
49.00	3659.0
50.00	17224.0
51.00	5201.0
51.90	237.0
52.90	106.0
54.00	110.0
54.90	487.0
56.00	1421.0
57.00	2818.0
58.00	177.0
60.00	960.0
61.00	4405.0
62.10	3822.0
63.00	3181.0
64.00	378.0
67.00	270.0
68.00	9513.0
69.00	9471.0
70.00	739.0
71.10	237.0
72.00	541.0
73.00	4127.0
74.00	15378.0
75.00	44928.0
76.00	3978.0
77.00	698.0
77.90	574.0
78.90	3104.0
79.90	713.0
81.00	3058.0
81.90	684.0
82.90	169.0
86.00	153.0
87.00	3263.0
88.00	3213.0
90.90	289.0
92.00	2714.0
93.00	3709.0
94.00	10819.0
95.00	87384.0
96.00	5761.0
97.00	257.0
103.90	498.0
104.80	226.0
105.90	443.0
106.80	141.0
115.00	100.0
115.70	317.0
116.90	655.0
117.80	339.0
118.90	530.0
123.70	116.0
127.90	314.0
128.90	226.0
129.90	353.0
130.90	179.0
134.80	159.0
136.90	200.0
140.90	918.0
141.80	154.0
142.90	1009.0
144.80	105.0
145.80	144.0
147.90	138.0
148.90	117.0
154.90	196.0
157.00	121.0
158.90	131.0
174.00	64848.0
175.00	4608.0
176.00	61536.0
177.00	3849.0

Instrument :
MSVOA_V
ClientSampleId :
BFB353