

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
 Data File : VV036779.D
 Acq On : 05 Aug 2024 12:25
 Operator : SY/MD
 Sample : P3437-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05T8

Quant Time: Aug 06 03:08:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 06 02:51:35 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.529	114	337044	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.780	117	318118	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.182	152	151645	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.278	65	207187	76.964	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	153.920%#	
7) Chloroethane-d5		1.532	69	164334	77.409	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	154.820%#	
11) 1,1-Dichloroethene-d2		2.056	65	90462	78.559	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	157.120%#	
21) 2-Butanone-d5		3.793	46	186101	130.477	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	130.480%#	
24) Chloroform-d		4.240	84	357829	74.071	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	148.140%#	
26) 1,2-Dichloroethane-d4		4.934	65	235432	75.798	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	151.600%#	
32) Benzene-d6		4.950	84	747856	77.834	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	155.660%#	
36) 1,2-Dichloropropane-d6		5.982	67	235114	75.848	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	151.700%#	
41) Toluene-d8		7.236	98	670251	76.045	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	152.100%#	
43) trans-1,3-Dichloroprop...		7.548	79	116742	72.366	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	144.740%#	
47) 2-Hexanone-d5		8.024	63	103702	116.352	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	116.350%	
56) 1,1,2,2-Tetrachloroeth...		10.146	84	238861	67.111	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	134.220%#	
66) 1,2-Dichlorobenzene-d4		11.554	152	236537	76.546	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	153.100%#	
Target Compounds							
13) Acetone		2.114	43	8319	6.971	ug/L	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
Data File : VV036779.D
Acq On : 05 Aug 2024 12:25
Operator : SY/MD
Sample : P3437-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05T8


Quant Time: Aug 06 03:08:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 06 02:51:35 2024
Response via : Initial Calibration

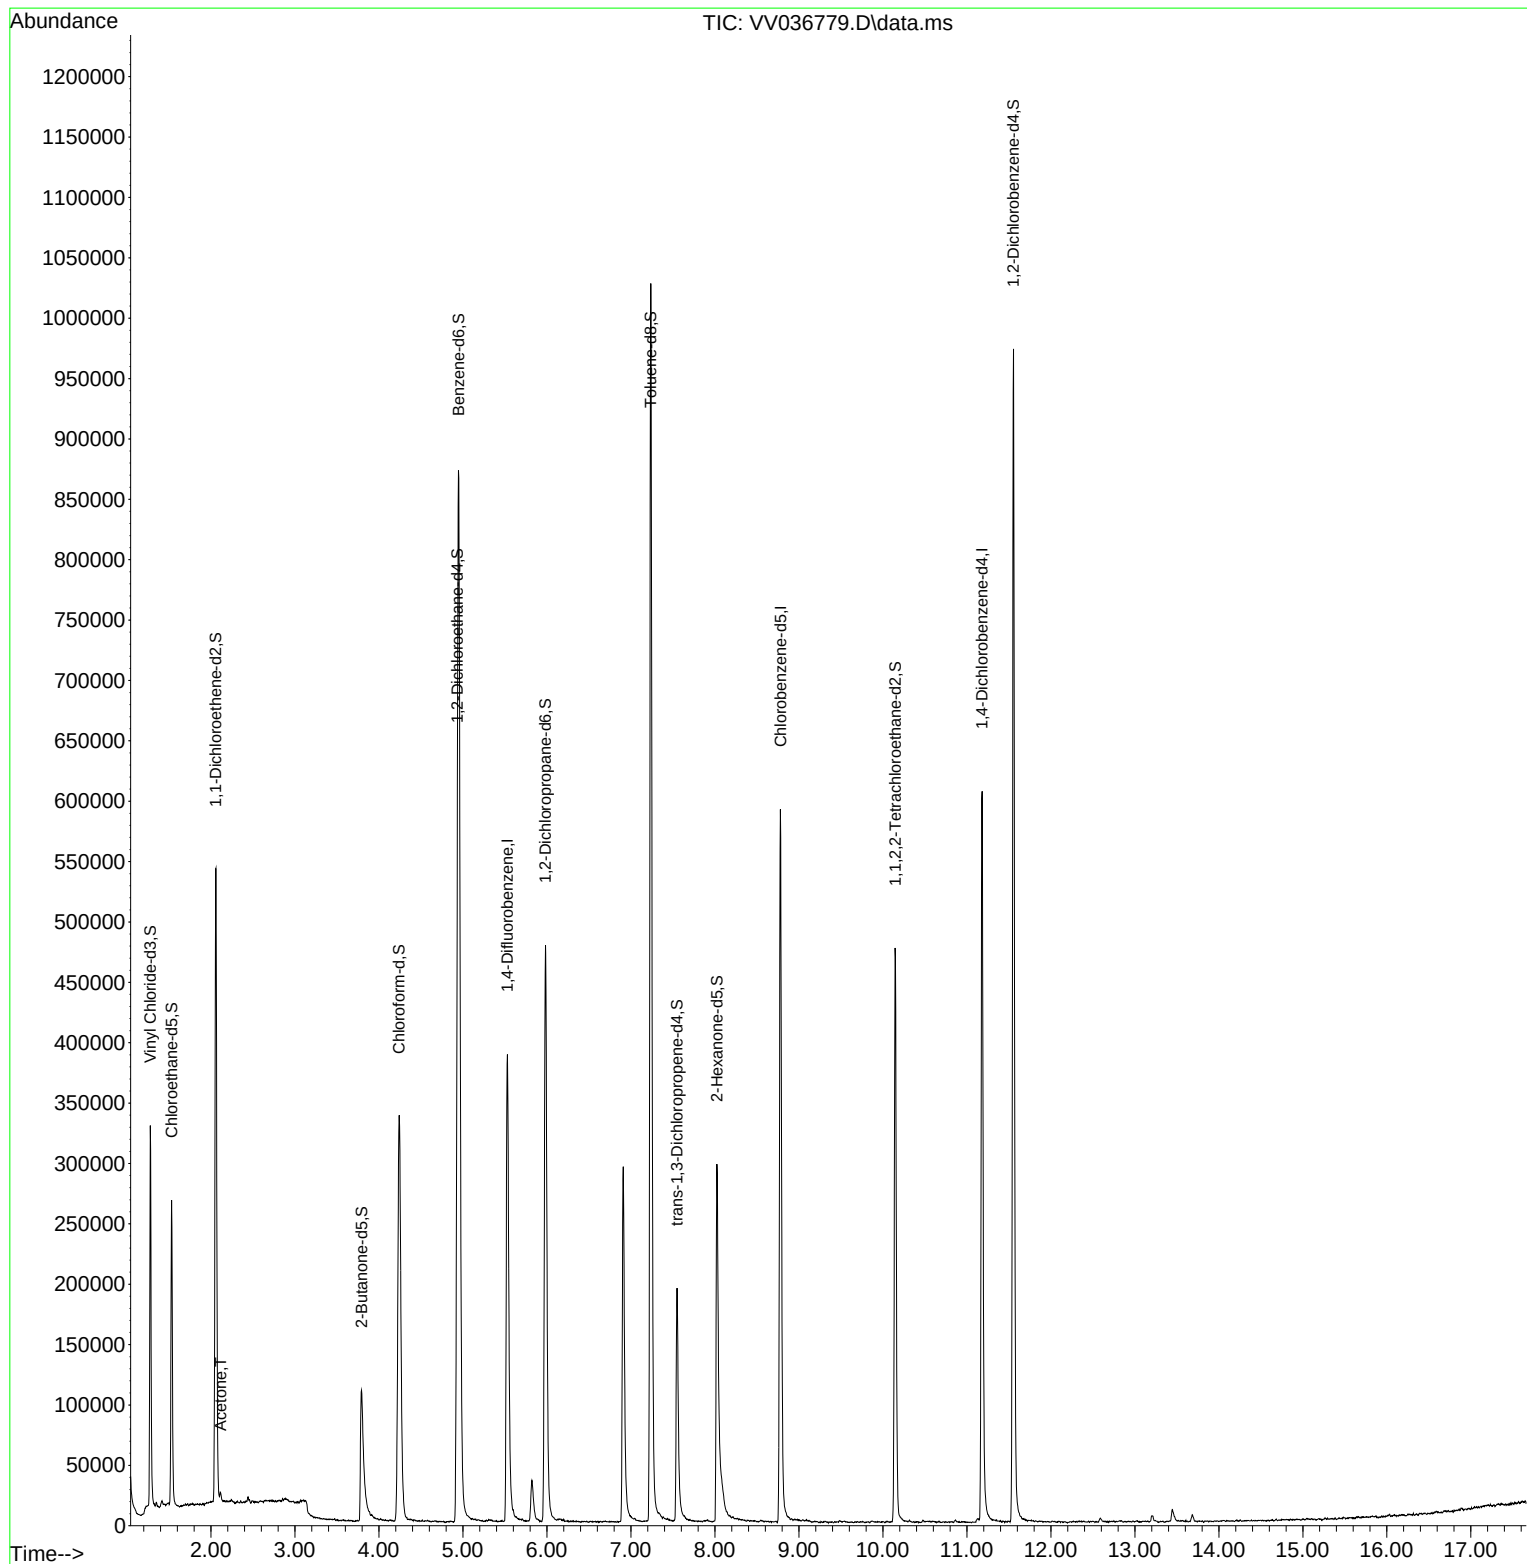

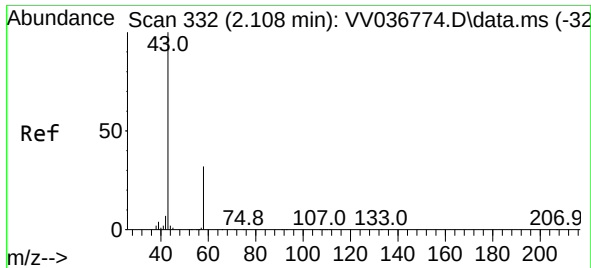

#13
 Acetone
 Concen: 6.971 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. 0.007 min
 Lab File: VV036779.D
 Acq: 05 Aug 2024 12:25

Instrument :
 MSVOA_V
 ClientSampleId :
 E05T8

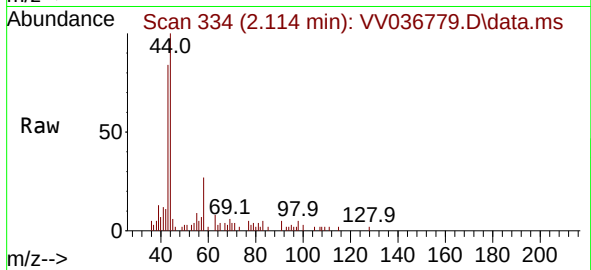

Tgt Ion: 43 Resp: 8319
 Ion Ratio Lower Upper
 43 100
 58 37.8 0.0 63.4

