

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
 Data File : VV036780.D
 Acq On : 05 Aug 2024 12:47
 Operator : SY/MD
 Sample : P3437-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05T9

Quant Time: Aug 06 03:09:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 06 02:51:35 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	357575	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	340818	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	164958	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	225321	78.894	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 157.780%#		
7) Chloroethane-d5	1.532	69	180222	80.019	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 160.040%#		
11) 1,1-Dichloroethene-d2	2.060	65	97152	79.525	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 159.040%#		
21) 2-Butanone-d5	3.796	46	211854	140.004	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 140.000%#		
24) Chloroform-d	4.243	84	390272	76.148	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 152.300%#		
26) 1,2-Dichloroethane-d4	4.937	65	258779	78.531	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 157.060%#		
32) Benzene-d6	4.953	84	817543	79.420	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 158.840%#		
36) 1,2-Dichloropropane-d6	5.985	67	262281	78.977	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 157.960%#		
41) Toluene-d8	7.239	98	737686	78.122	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 156.240%#		
43) trans-1,3-Dichloroprop...	7.551	79	129010	74.644	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 149.280%#		
47) 2-Hexanone-d5	8.024	63	117427	122.976	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 122.980%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	268680	70.461	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 140.920%#		
66) 1,2-Dichlorobenzene-d4	11.554	152	265989	79.130	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 158.260%#		
Target Compounds						Qvalue
13) Acetone	2.114	43	8476	6.695	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
Data File : VV036780.D
Acq On : 05 Aug 2024 12:47
Operator : SY/MD
Sample : P3437-02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05T9

Quant Time: Aug 06 03:09:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 06 02:51:35 2024
Response via : Initial Calibration

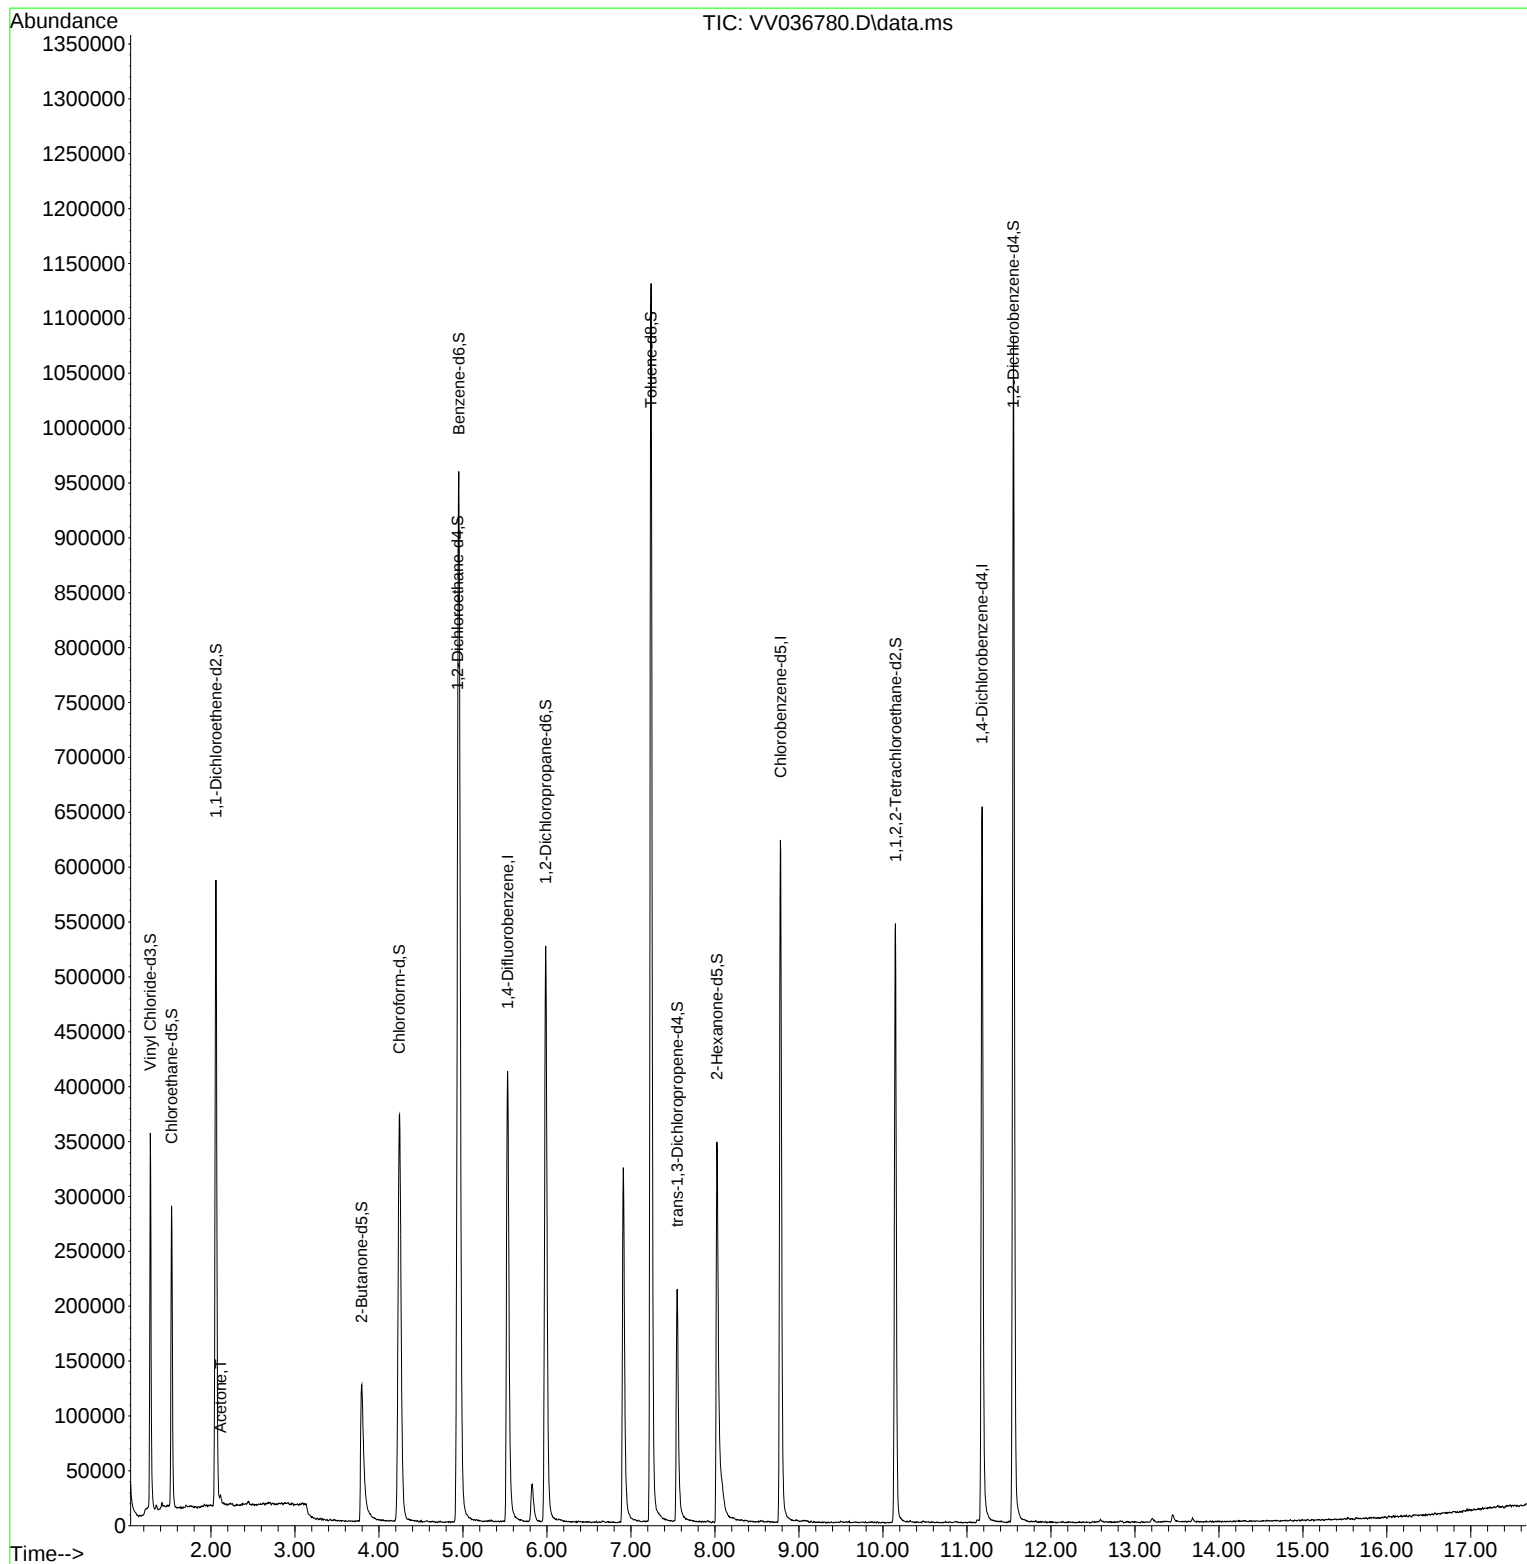

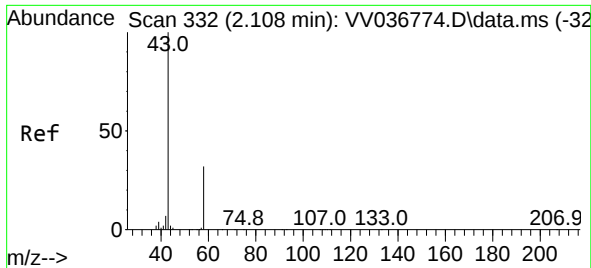

#13
 Acetone
 Concen: 6.695 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: VV036780.D
 Acq: 05 Aug 2024 12:47

Instrument :
 MSVOA_V
 ClientSampleId :
 E05T9

Tgt Ion: 43 Resp: 8476
 Ion Ratio Lower Upper
 43 100
 58 34.0 0.0 63.4

