

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
 Data File : VV036783.D
 Acq On : 05 Aug 2024 13:52
 Operator : SY/MD
 Sample : P3437-05
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05W5

Quant Time: Aug 06 03:10:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 06 02:51:35 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	395019	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	370479	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	179058	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	214881	68.107	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 136.220%#		
7) Chloroethane-d5	1.532	69	168068	67.549	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 135.100%#		
11) 1,1-Dichloroethene-d2	2.060	65	90641	67.162	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 134.320%#		
21) 2-Butanone-d5	3.796	46	199259	119.198	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 119.200%		
24) Chloroform-d	4.246	84	369809	65.316	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 130.640%#		
26) 1,2-Dichloroethane-d4	4.937	65	245539	67.450	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 134.900%#		
32) Benzene-d6	4.953	84	780414	69.743	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 139.480%#		
36) 1,2-Dichloropropane-d6	5.986	67	245890	68.113	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 136.220%#		
41) Toluene-d8	7.239	98	702577	68.447	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 136.900%#		
43) trans-1,3-Dichloroprop...	7.551	79	120860	64.330	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 128.660%#		
47) 2-Hexanone-d5	8.024	63	114146	109.970	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 109.970%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	259283	62.553	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 125.100%#		
66) 1,2-Dichlorobenzene-d4	11.554	152	249783	68.458	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 136.920%#		
Target Compounds						
13) Acetone	2.114	43	5912	4.227	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
Data File : VV036783.D
Acq On : 05 Aug 2024 13:52
Operator : SY/MD
Sample : P3437-05
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05W5

Quant Time: Aug 06 03:10:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 06 02:51:35 2024
Response via : Initial Calibration

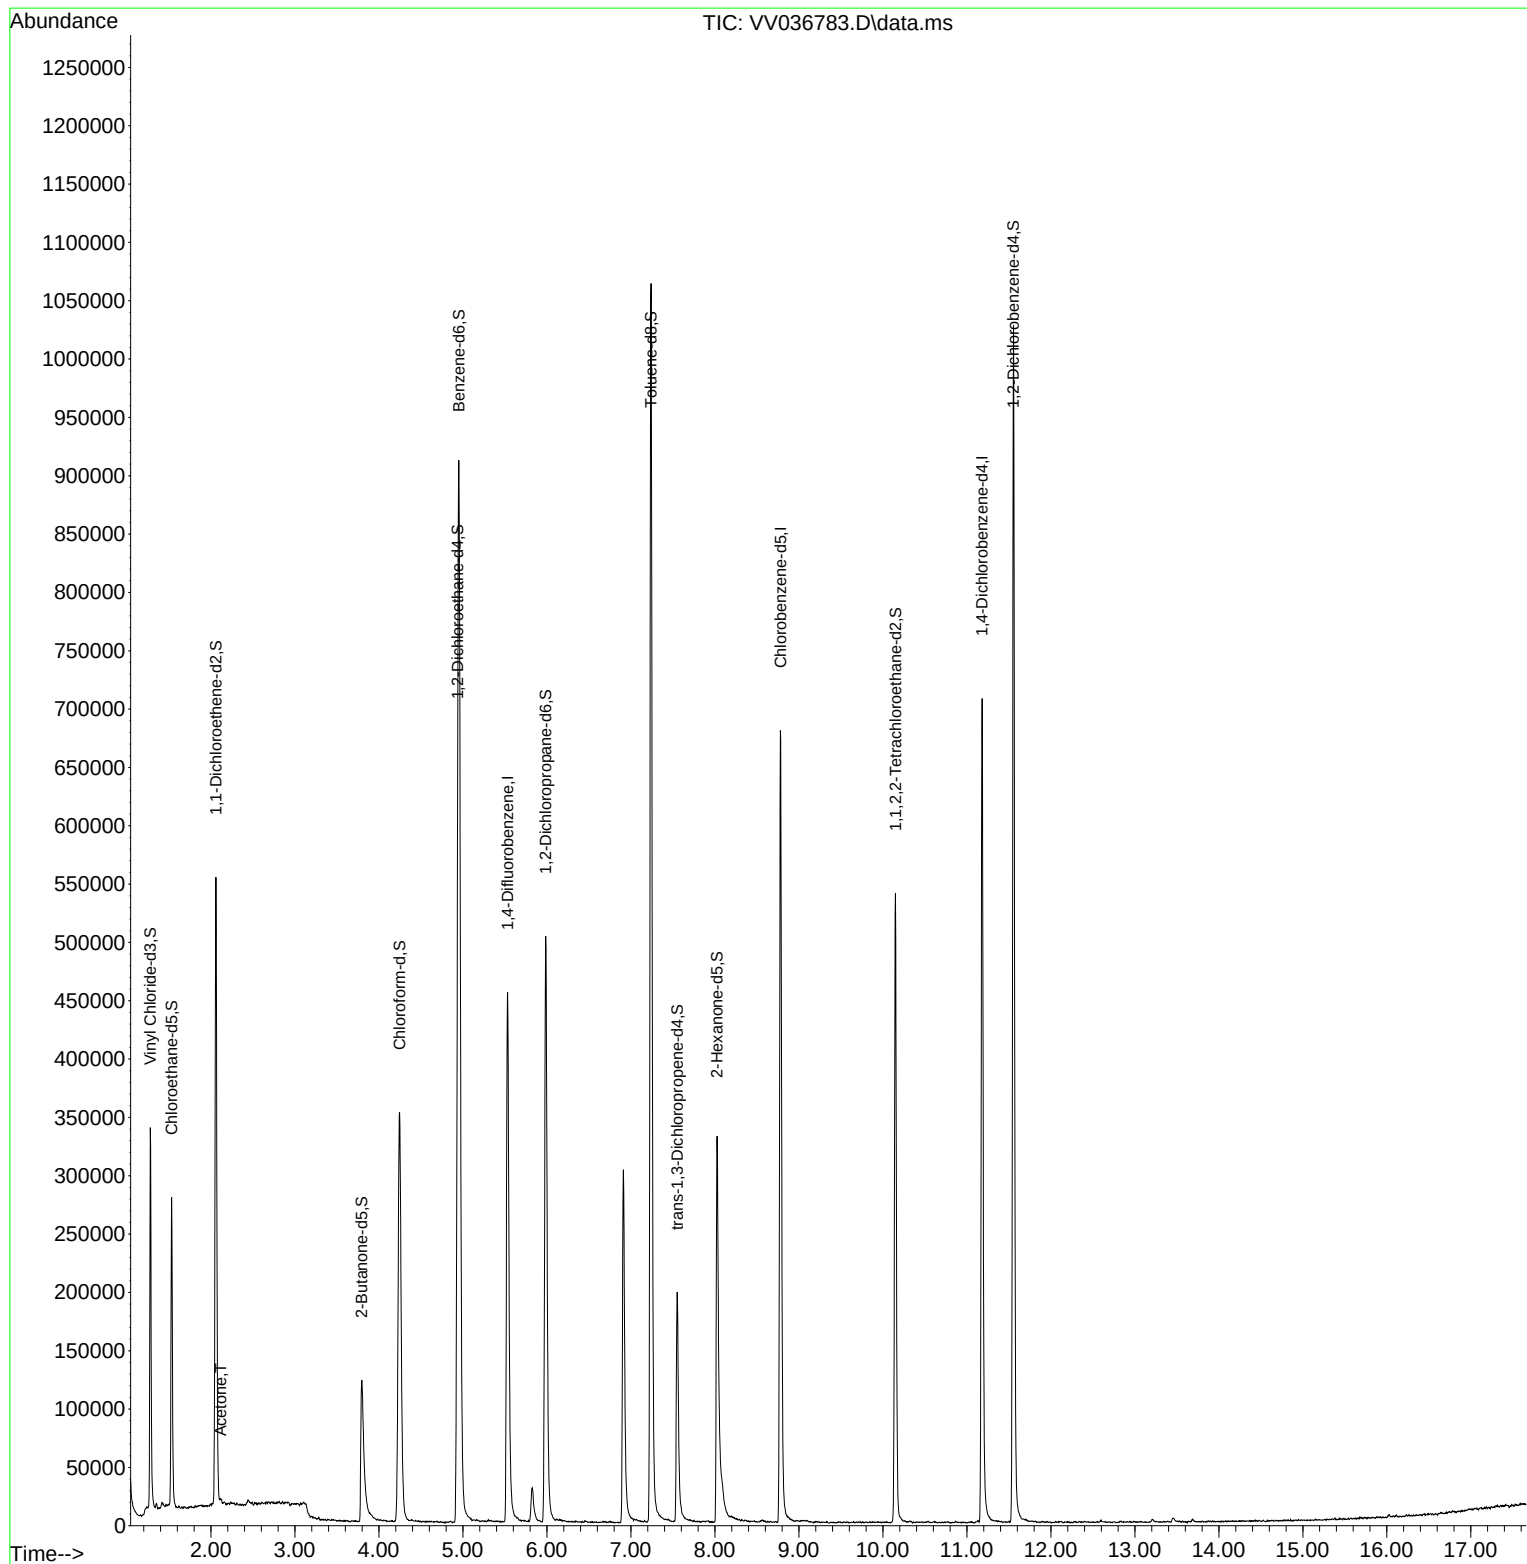

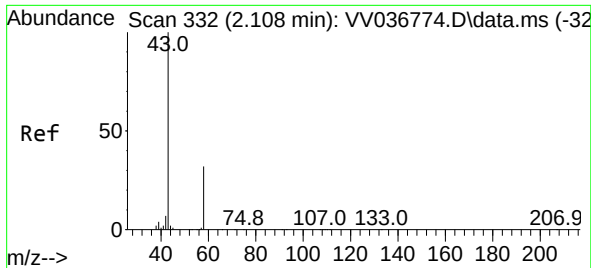

#13

Acetone

Concen: 4.227 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.006 min

Lab File: VV036783.D


Acq: 05 Aug 2024 13:52

Instrument :

MSVOA_V

ClientSampleId :

E05W5

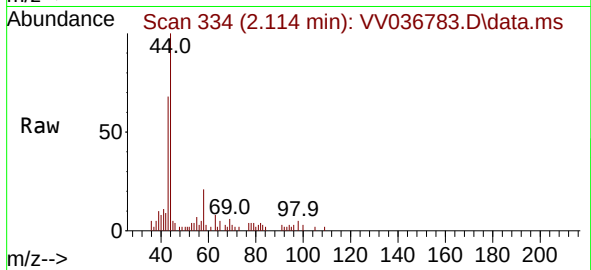

Tgt Ion: 43 Resp: 5912

Ion Ratio Lower Upper

43 100

58 29.5 0.0 63.4

