

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
 Data File : VV036785.D
 Acq On : 05 Aug 2024 14:36
 Operator : SY/MD
 Sample : P3437-10
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05X4

Quant Time: Aug 06 03:10:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 06 02:51:35 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	581535	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	548185	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	261083	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	201038	43.282	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	86.560%		
7) Chloroethane-d5	1.532	69	159030	43.416	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	86.840%		
11) 1,1-Dichloroethene-d2	2.059	65	85694	43.131	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	86.260%		
21) 2-Butanone-d5	3.796	46	193349	78.566	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	78.570%		
24) Chloroform-d	4.246	84	347626	41.705	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.420%		
26) 1,2-Dichloroethane-d4	4.940	65	231938	43.279	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.560%		
32) Benzene-d6	4.953	84	724028	43.729	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.460%		
36) 1,2-Dichloropropane-d6	5.985	67	234203	43.845	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	87.700%		
41) Toluene-d8	7.239	98	659069	43.394	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.780%		
43) trans-1,3-Dichloroprop...	7.551	79	108336	38.971	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	77.940%		
47) 2-Hexanone-d5	8.024	63	109616	71.371	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	71.370%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	246763	40.234	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	80.460%		
66) 1,2-Dichlorobenzene-d4	11.554	152	234238	44.028	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.060%		
Target Compounds					Qvalue	
13) Acetone	2.117	43	11245	5.461	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
Data File : VV036785.D
Acq On : 05 Aug 2024 14:36
Operator : SY/MD
Sample : P3437-10
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05X4


Quant Time: Aug 06 03:10:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 06 02:51:35 2024
Response via : Initial Calibration

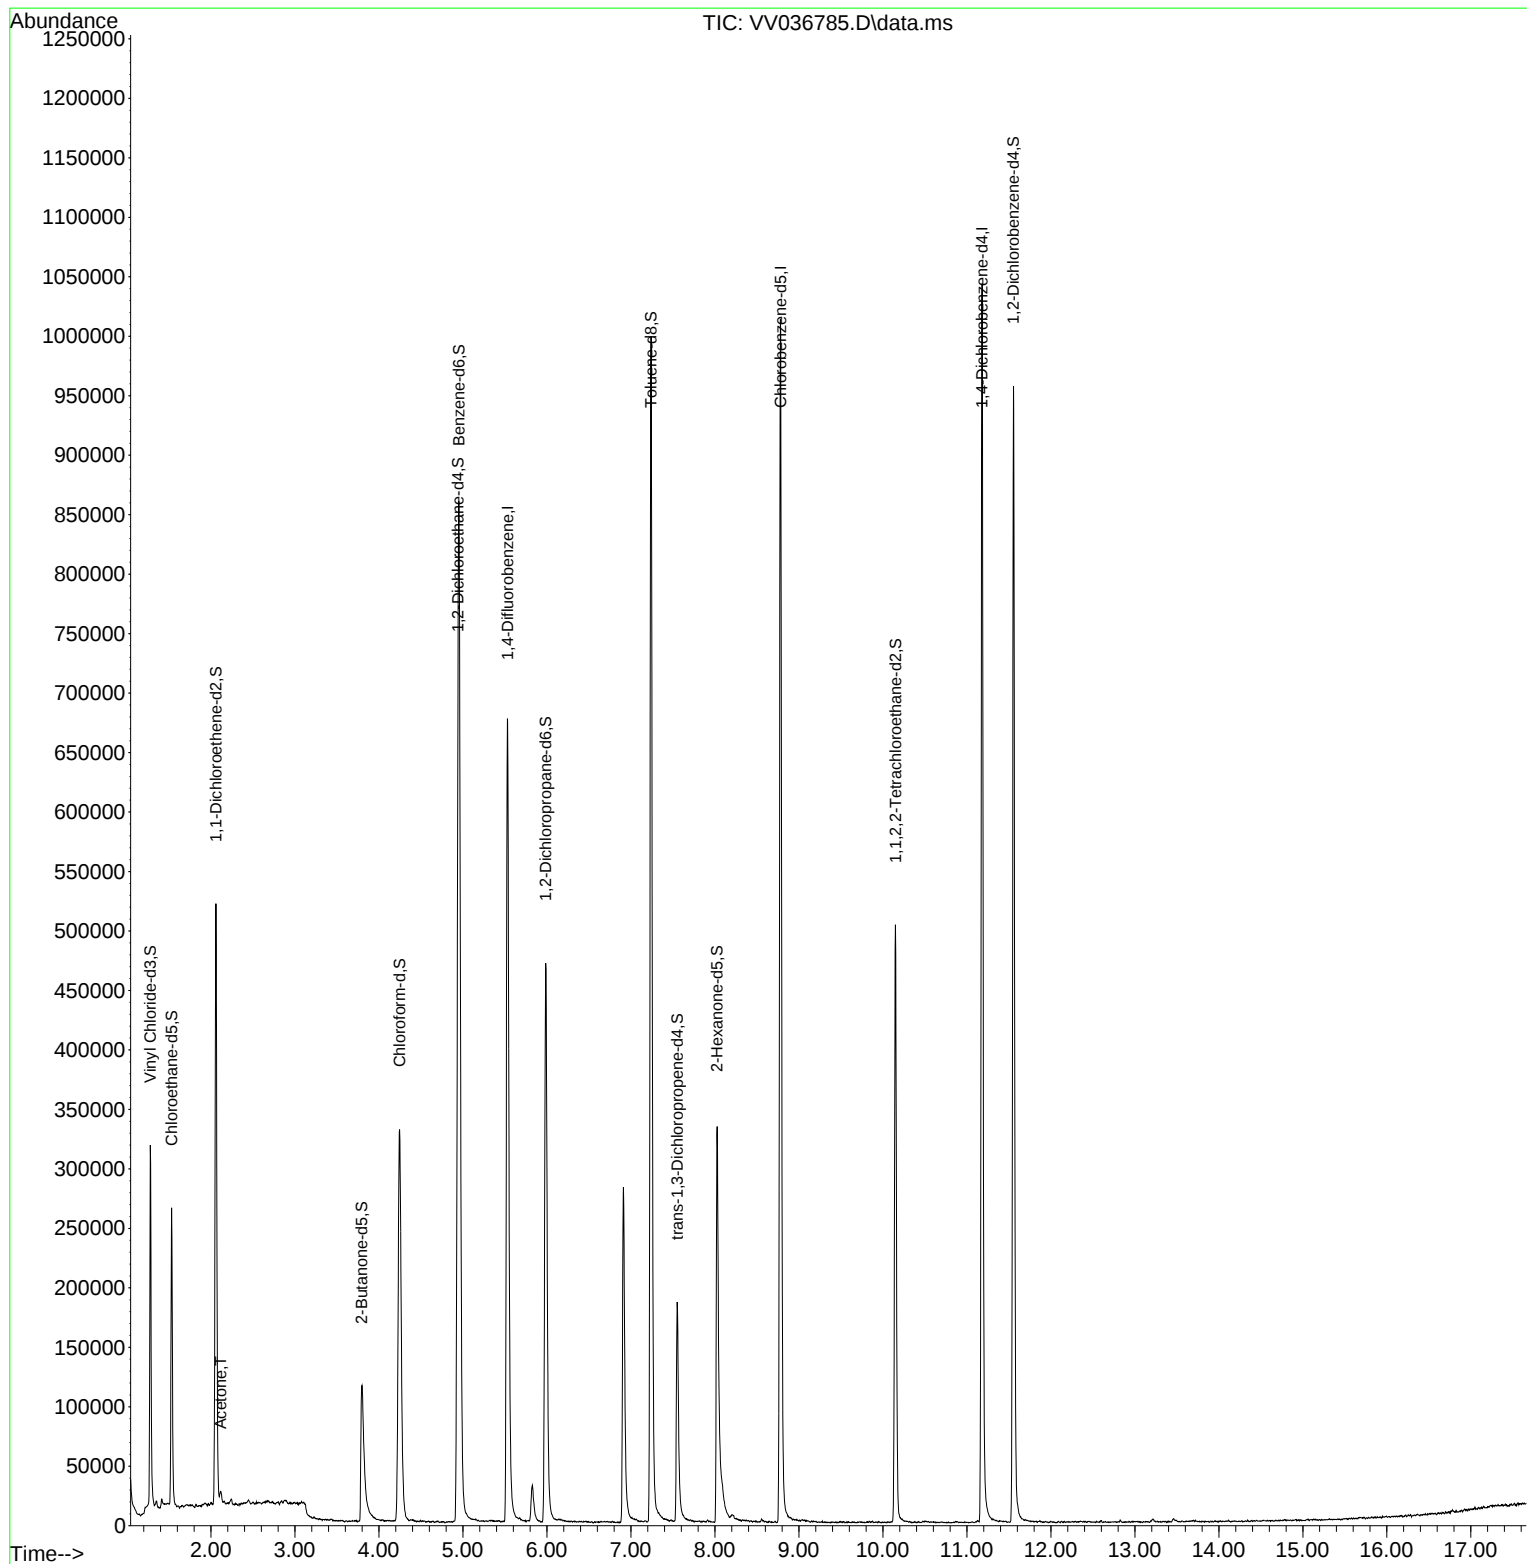

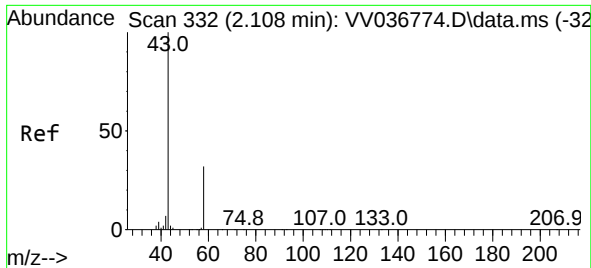

#13
 Acetone
 Concen: 5.461 ug/L
 RT: 2.117 min Scan# 31
 Delta R.T. 0.010 min
 Lab File: VV036785.D
 Acq: 05 Aug 2024 14:36

Instrument :
 MSVOA_V
 ClientSampleId :
 E05X4

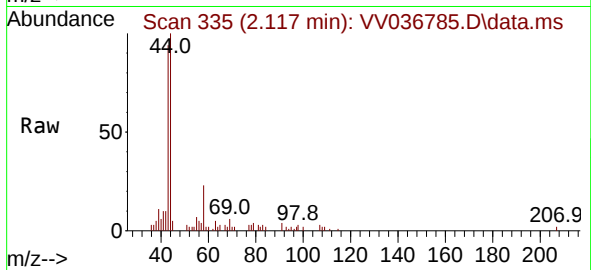

Tgt Ion: 43 Resp: 11245
 Ion Ratio Lower Upper
 43 100
 58 28.9 0.0 63.4

