

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
 Data File : VV036786.D
 Acq On : 05 Aug 2024 14:57
 Operator : SY/MD
 Sample : P3437-11
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05X6

Quant Time: Aug 06 03:10:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 06 02:51:35 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	514002	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	484365	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	233913	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	193604	47.158	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	94.320%		
7) Chloroethane-d5	1.532	69	153277	47.344	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	94.680%		
11) 1,1-Dichloroethene-d2	2.060	65	82799	47.150	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.300%		
21) 2-Butanone-d5	3.796	46	190878	87.753	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	87.750%		
24) Chloroform-d	4.246	84	336055	45.614	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.220%		
26) 1,2-Dichloroethane-d4	4.937	65	223858	47.259	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.520%		
32) Benzene-d6	4.953	84	702650	48.029	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.060%		
36) 1,2-Dichloropropane-d6	5.986	67	223429	47.339	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	94.680%		
41) Toluene-d8	7.239	98	641623	47.811	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.620%		
43) trans-1,3-Dichloroprop...	7.551	79	108110	44.014	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	88.020%		
47) 2-Hexanone-d5	8.024	63	109656	80.804	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	80.800%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	240929	44.458	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	88.920%		
66) 1,2-Dichlorobenzene-d4	11.558	152	228599	47.959	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.920%		
Target Compounds					Qvalue	
13) Acetone	2.114	43	13721	7.539	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
Data File : VV036786.D
Acq On : 05 Aug 2024 14:57
Operator : SY/MD
Sample : P3437-11
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05X6

Quant Time: Aug 06 03:10:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 06 02:51:35 2024
Response via : Initial Calibration

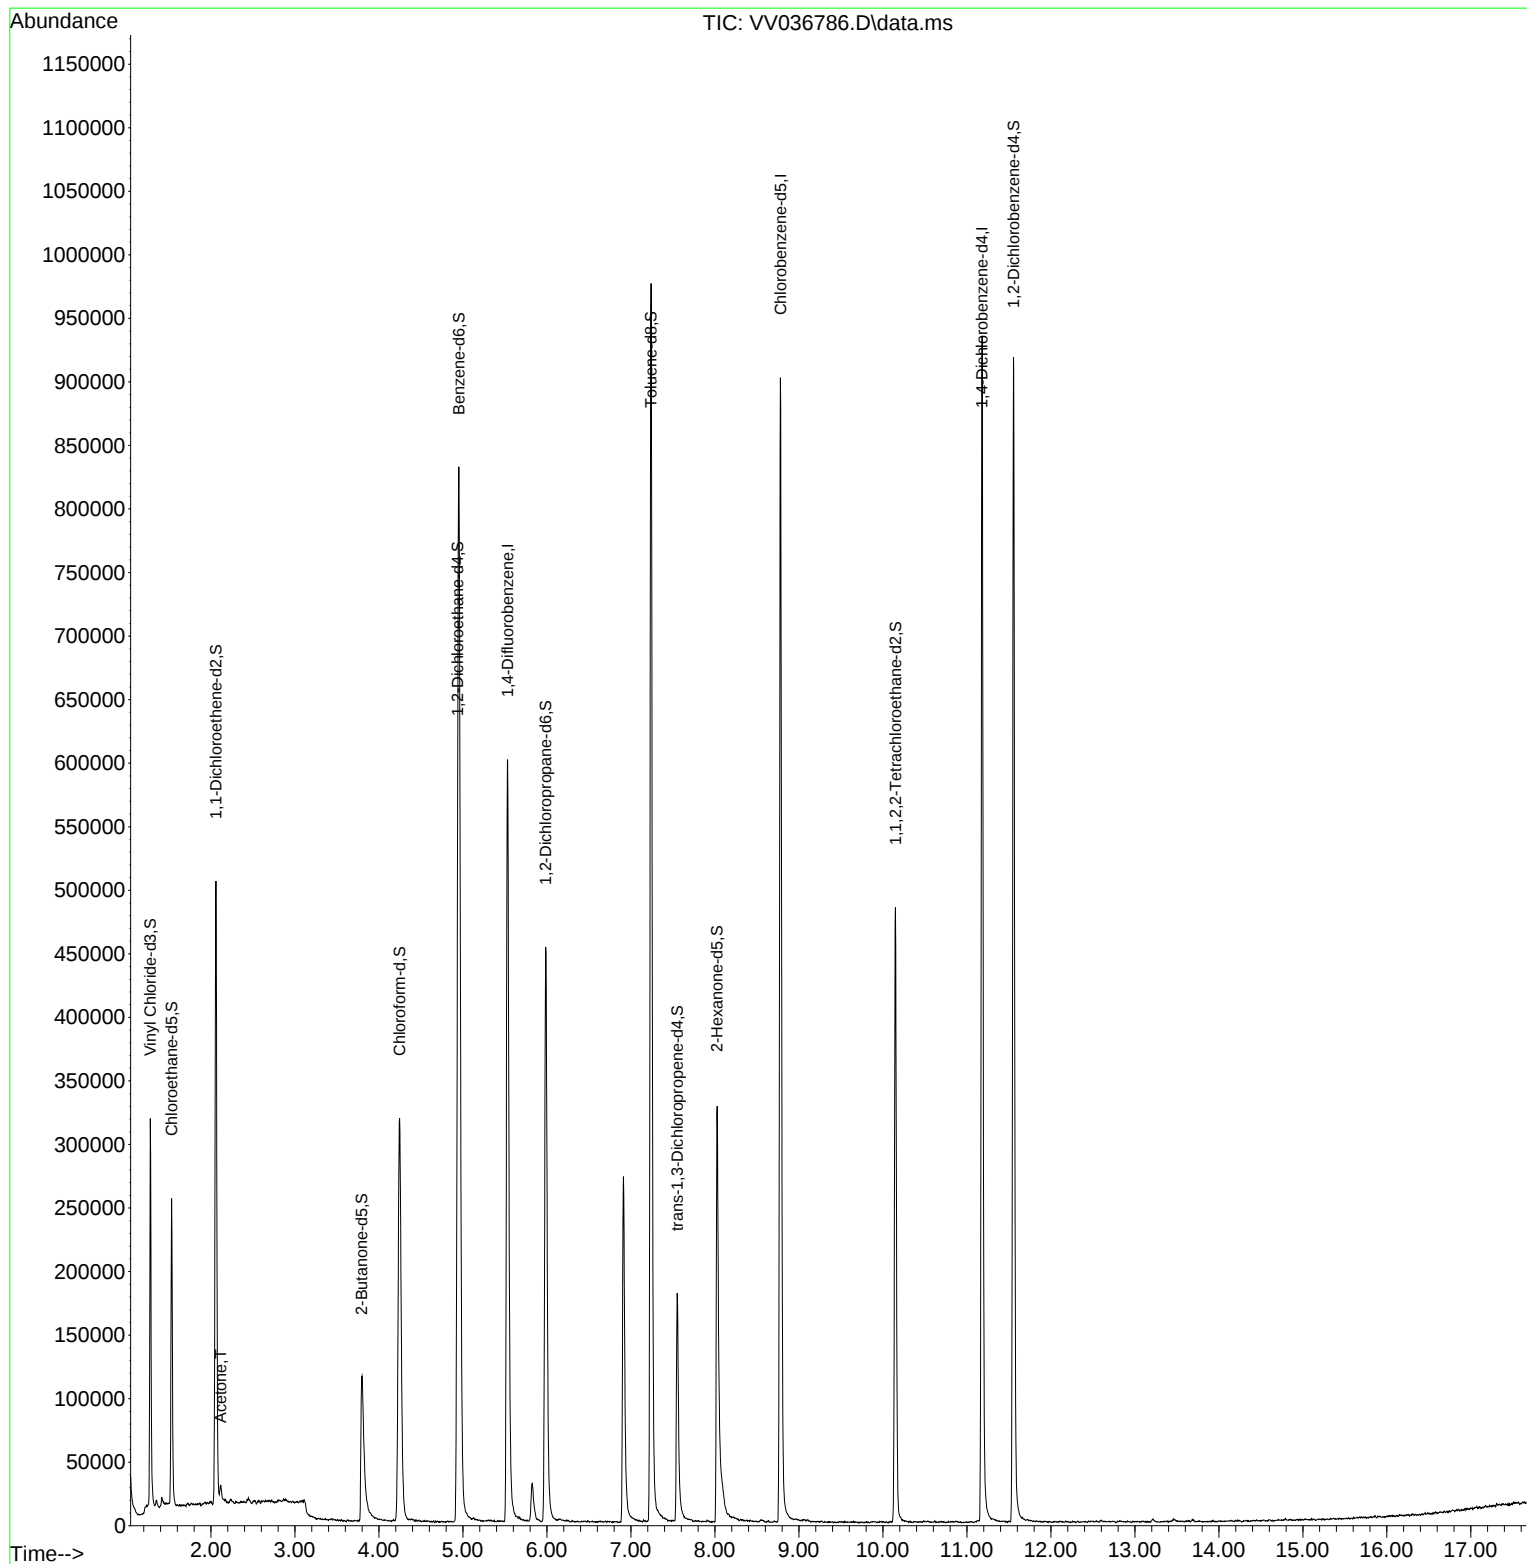

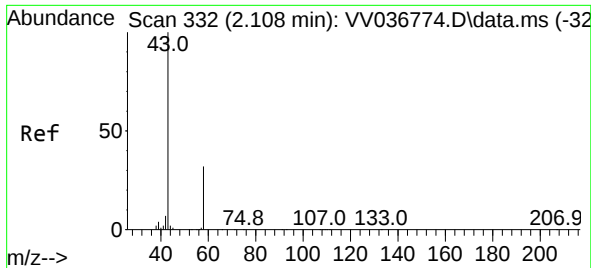

#13

Acetone

Concen: 7.539 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.007 min

Lab File: VV036786.D


Acq: 05 Aug 2024 14:57

Instrument :

MSVOA_V

ClientSampleId :

E05X6

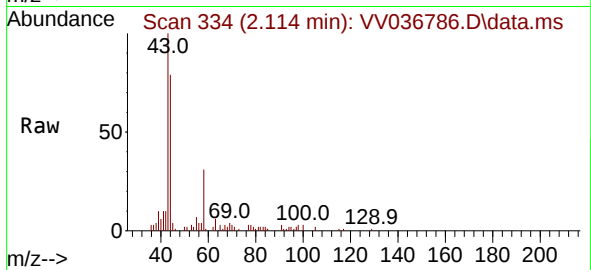

Tgt Ion: 43 Resp: 13721

Ion Ratio Lower Upper

43 100

58 30.4 0.0 63.4

