

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
 Data File : VV036793.D
 Acq On : 05 Aug 2024 17:31
 Operator : SY/MD
 Sample : P3437-18
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0602

Quant Time: Aug 06 03:12:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 06 02:51:35 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	558898	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	521447	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	254691	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	186228	41.718	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	83.440%		
7) Chloroethane-d5	1.532	69	149600	42.496	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	85.000%		
11) 1,1-Dichloroethene-d2	2.056	65	80049	41.922	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.840%		
21) 2-Butanone-d5	3.796	46	198953	84.118	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	84.120%		
24) Chloroform-d	4.246	84	329067	41.078	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.160%		
26) 1,2-Dichloroethane-d4	4.940	65	218886	42.497	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.000%		
32) Benzene-d6	4.953	84	691025	43.876	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.760%		
36) 1,2-Dichloropropane-d6	5.985	67	221920	43.676	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	87.360%		
41) Toluene-d8	7.239	98	623408	43.151	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.300%		
43) trans-1,3-Dichloroprop...	7.551	79	108035	40.855	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.720%		
47) 2-Hexanone-d5	8.024	63	112412	76.945	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	76.940%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	227483	38.992	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	77.980%		
66) 1,2-Dichlorobenzene-d4	11.558	152	226069	43.559	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.120%		
Target Compounds					Qvalue	
13) Acetone	2.114	43	75586	38.196	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
Data File : VV036793.D
Acq On : 05 Aug 2024 17:31
Operator : SY/MD
Sample : P3437-18
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0602

Quant Time: Aug 06 03:12:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 06 02:51:35 2024
Response via : Initial Calibration

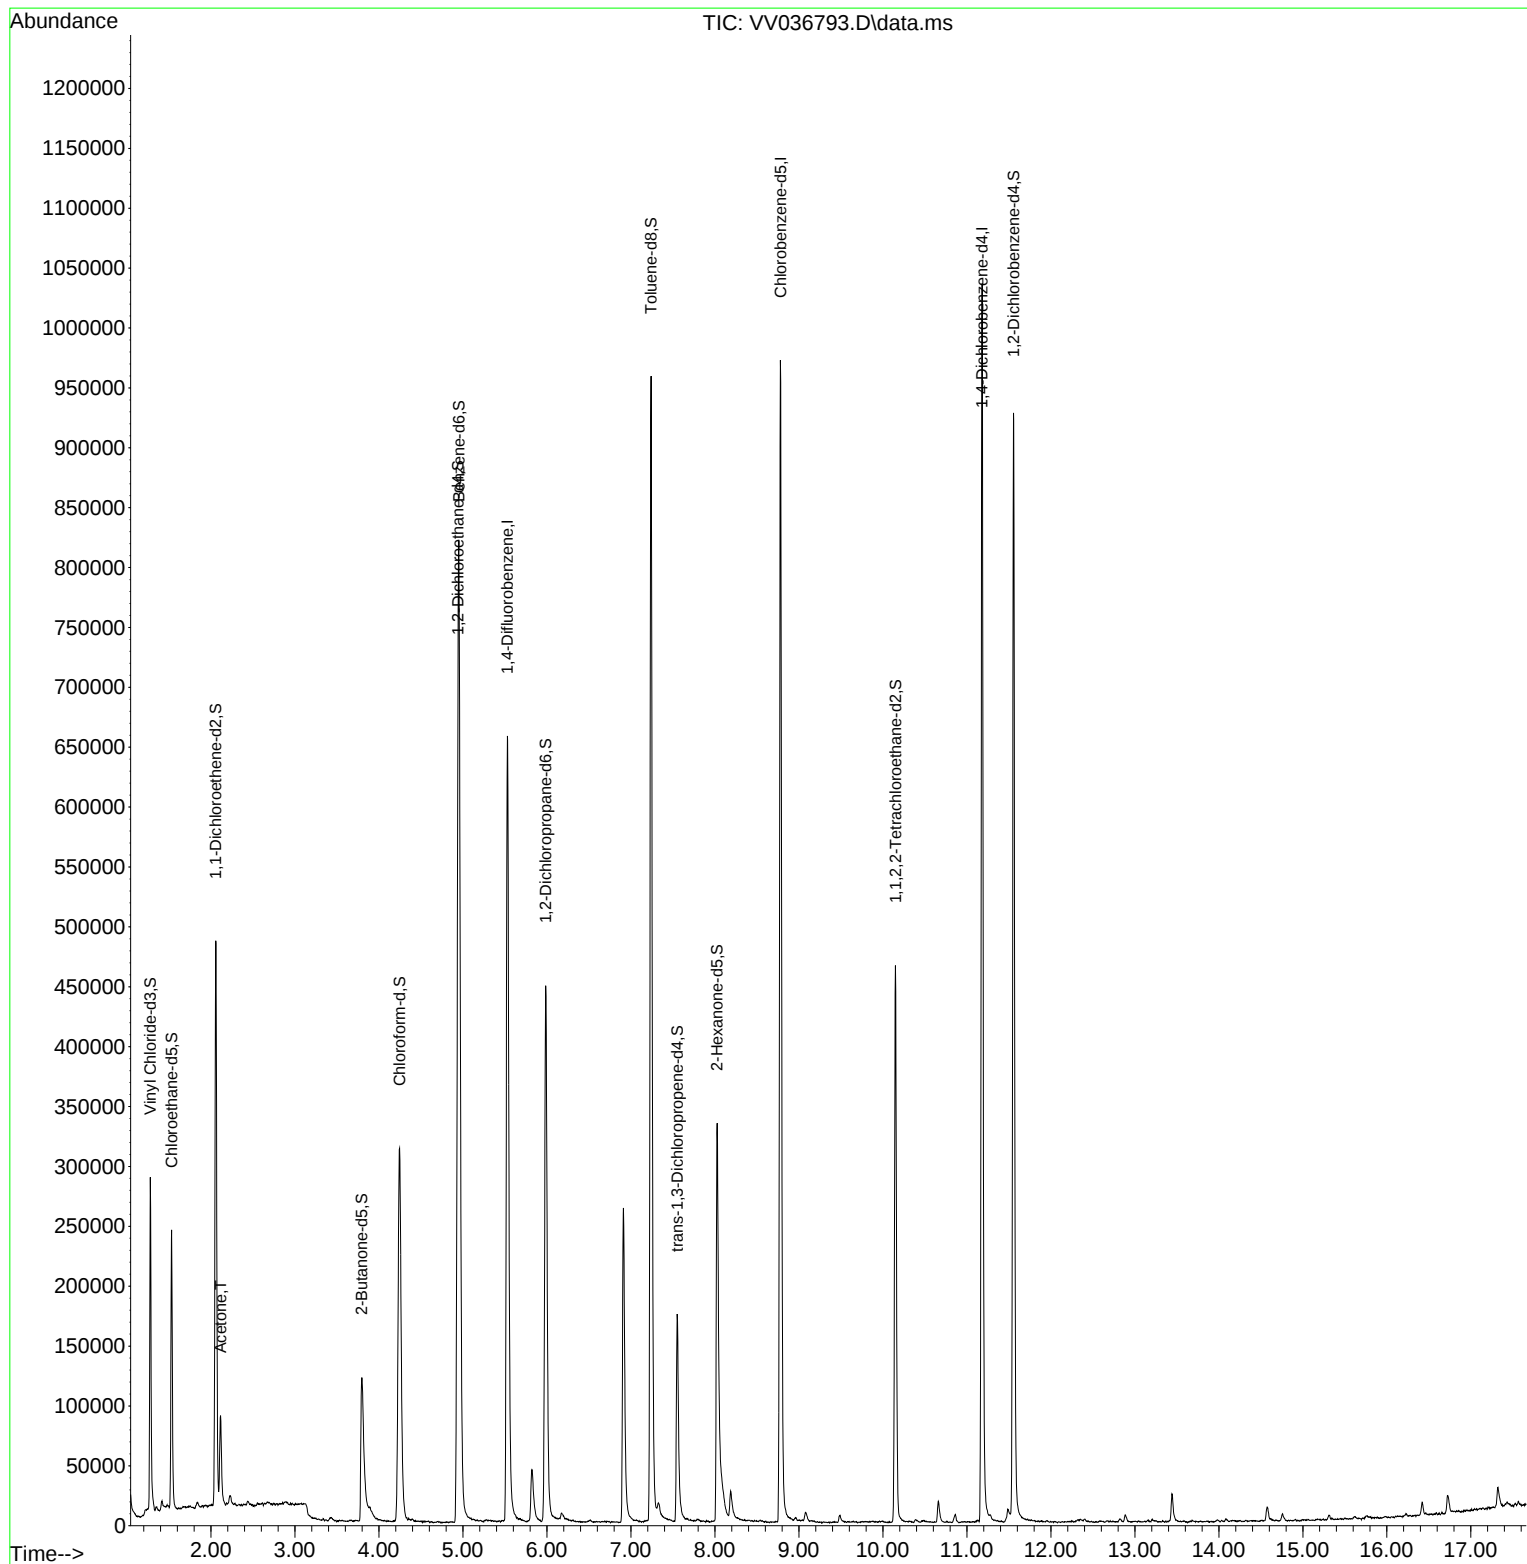

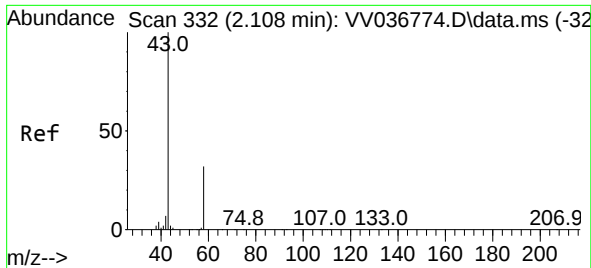

#13

Acetone

Concen: 38.196 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.006 min

Lab File: VV036793.D


Acq: 05 Aug 2024 17:31

Instrument :

MSVOA_V

ClientSampleId :

E0602

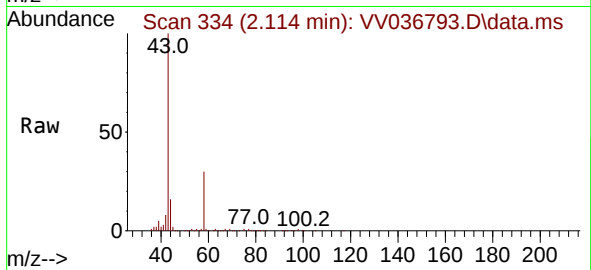

Tgt Ion: 43 Resp: 75586

Ion Ratio Lower Upper

43 100

58 31.6 0.0 63.4

