

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
 Data File : VV036779.D
 Acq On : 05 Aug 2024 12:25
 Operator : SY/MD
 Sample : P3437-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05T8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036779.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rBV	314585	333093	15.15%	2.316%
2	1.532	146	153	167	rVB	251635	294610	13.40%	2.048%
3	2.060	307	317	330	rBV	524294	757525	34.45%	5.267%
4	3.638	806	808	813	rVB6	1004	697	0.03%	0.005%
5	3.793	847	856	890	rBV	107834	302198	13.74%	2.101%
6	4.243	979	996	1022	rBV	336013	869302	39.54%	6.044%
7	4.417	1047	1050	1052	rBV3	1059	758	0.03%	0.005%
8	4.484	1069	1071	1075	rVB5	885	551	0.03%	0.004%
9	4.516	1077	1081	1083	rBV5	1144	628	0.03%	0.004%
10	4.552	1089	1092	1096	rBV6	771	712	0.03%	0.005%
11	4.725	1141	1146	1149	rVV6	736	613	0.03%	0.004%
12	4.806	1166	1171	1172	rBV4	887	563	0.03%	0.004%
13	4.947	1197	1215	1248	rBV2	870814	2198687	100.00%	15.286%
14	5.400	1353	1356	1360	rVB4	1215	713	0.03%	0.005%
15	5.529	1385	1396	1417	rBV	386386	797619	36.28%	5.545%
16	5.773	1468	1472	1474	rBV6	629	584	0.03%	0.004%
17	5.822	1476	1487	1504	rBV	33537	74690	3.40%	0.519%
18	5.982	1523	1537	1573	rBV	477344	993625	45.19%	6.908%
19	6.201	1603	1605	1608	rVB4	1843	957	0.04%	0.007%
20	6.249	1618	1620	1624	rVB3	1133	744	0.03%	0.005%
21	6.285	1628	1631	1633	rVV5	937	612	0.03%	0.004%
22	6.310	1637	1639	1642	rVB4	1250	680	0.03%	0.005%
23	6.420	1669	1673	1676	rBV5	860	738	0.03%	0.005%
24	6.474	1687	1690	1696	rVB4	1098	943	0.04%	0.007%
25	6.603	1727	1730	1734	rVB6	916	652	0.03%	0.005%
26	6.670	1746	1751	1754	rBV7	876	704	0.03%	0.005%
27	6.748	1773	1775	1778	rBV4	890	507	0.02%	0.004%
28	6.838	1800	1803	1808	rVB6	845	616	0.03%	0.004%
29	6.908	1808	1825	1850	rBV	294590	554478	25.22%	3.855%
30	7.236	1916	1927	1954	rBV	1024651	1787520	81.30%	12.428%
31	7.548	2013	2024	2051	rVV	192654	352185	16.02%	2.449%
32	7.809	2101	2105	2107	rBV5	731	546	0.02%	0.004%
33	7.867	2118	2123	2125	rBV6	1092	996	0.05%	0.007%
34	8.024	2164	2172	2218	rBV2	295441	661618	30.09%	4.600%
35	8.384	2282	2284	2287	rBV3	933	614	0.03%	0.004%
36	8.548	2331	2335	2337	rBV5	940	676	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
 Data File : VV036779.D
 Acq On : 05 Aug 2024 12:25
 Operator : SY/MD
 Sample : P3437-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05T8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	8.661	2367	2370	2374	rVB3	902	646	0.03%	0.004%
38	8.780	2395	2407	2434	rBV	590797	989725	45.01%	6.881%
39	9.092	2502	2504	2510	rVB7	1511	1096	0.05%	0.008%
40	9.120	2510	2513	2518	rVB7	1129	793	0.04%	0.006%
41	9.310	2568	2572	2575	rBV5	923	869	0.04%	0.006%
42	9.346	2580	2583	2585	rVB5	859	617	0.03%	0.004%
43	9.426	2603	2608	2610	rBV5	1034	750	0.03%	0.005%
44	9.484	2622	2626	2630	rBV5	1395	1617	0.07%	0.011%
45	9.699	2689	2693	2697	rVB6	703	614	0.03%	0.004%
46	9.735	2702	2704	2708	rBV5	648	530	0.02%	0.004%
47	9.860	2738	2743	2744	rBV6	1298	996	0.05%	0.007%
48	10.047	2794	2801	2804	rBV6	1473	1700	0.08%	0.012%
49	10.104	2814	2819	2820	rBV4	832	627	0.03%	0.004%
50	10.146	2820	2832	2857	rBV	475210	775464	35.27%	5.391%
51	10.317	2879	2885	2888	rBV6	1552	1387	0.06%	0.010%
52	10.362	2896	2899	2903	rVB5	936	783	0.04%	0.005%
53	10.407	2909	2913	2915	rVV3	679	531	0.02%	0.004%
54	10.477	2929	2935	2939	rBV8	1933	2026	0.09%	0.014%
55	10.751	3016	3020	3024	rBV5	944	815	0.04%	0.006%
56	10.812	3036	3039	3043	rVV3	640	503	0.02%	0.003%
57	10.863	3048	3055	3061	rBV9	2284	3318	0.15%	0.023%
58	10.963	3083	3086	3089	rVV3	759	612	0.03%	0.004%
59	11.037	3106	3109	3114	rVB6	580	630	0.03%	0.004%
60	11.066	3114	3118	3122	rBV5	842	842	0.04%	0.006%
61	11.130	3130	3138	3140	rBV6	2967	4131	0.19%	0.029%
62	11.182	3143	3154	3187	rVV	604264	977561	44.46%	6.796%
63	11.400	3220	3222	3227	rVB4	1567	1034	0.05%	0.007%
64	11.429	3227	3231	3237	rVB7	1492	1996	0.09%	0.014%
65	11.458	3237	3240	3241	rBV2	1294	634	0.03%	0.004%
66	11.490	3247	3250	3252	rBV2	1131	803	0.04%	0.006%
67	11.554	3257	3270	3298	rBV	971683	1551117	70.55%	10.784%
68	11.818	3348	3352	3359	rVB9	757	884	0.04%	0.006%
69	12.014	3409	3413	3415	rBV3	956	706	0.03%	0.005%
70	12.226	3470	3479	3480	rBV7	958	1174	0.05%	0.008%
71	12.336	3508	3513	3518	rBV4	1030	835	0.04%	0.006%
72	12.384	3524	3528	3529	rBV3	701	524	0.02%	0.004%
73	12.448	3543	3548	3551	rVB5	1199	977	0.04%	0.007%
74	12.474	3551	3556	3558	rBV4	989	939	0.04%	0.007%
75	12.535	3572	3575	3579	rBV4	888	788	0.04%	0.005%
76	12.587	3584	3591	3602	rVV4	3455	6365	0.29%	0.044%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
 Data File : VV036779.D
 Acq On : 05 Aug 2024 12:25
 Operator : SY/MD
 Sample : P3437-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05T8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	12.632	3602	3605	3609	rVV6	998	879	0.04%	0.006%
78	12.696	3623	3625	3629	rBV2	1137	844	0.04%	0.006%
79	12.821	3656	3664	3667	rBV8	930	1159	0.05%	0.008%
80	12.837	3667	3669	3678	rVB6	1405	1263	0.06%	0.009%
81	12.976	3708	3712	3719	rBV5	944	1014	0.05%	0.007%
82	13.091	3744	3748	3749	rBV4	748	592	0.03%	0.004%
83	13.124	3756	3758	3763	rVB4	697	525	0.02%	0.004%
84	13.152	3765	3767	3772	rVB5	1045	790	0.04%	0.005%
85	13.201	3772	3782	3793	rBV5	5358	10746	0.49%	0.075%
86	13.307	3812	3815	3818	rVV4	675	553	0.03%	0.004%
87	13.445	3851	3858	3866	rBV	9459	16246	0.74%	0.113%
88	13.564	3893	3895	3900	rVB4	841	630	0.03%	0.004%
89	13.622	3909	3913	3917	rVB6	731	622	0.03%	0.004%
90	13.683	3924	3932	3941	rBV9	5657	9270	0.42%	0.064%
91	13.751	3951	3953	3955	rBV3	953	603	0.03%	0.004%
92	13.834	3974	3979	3981	rBV4	1333	1165	0.05%	0.008%
93	13.892	3993	3997	4000	rBV4	902	774	0.04%	0.005%
94	13.947	4011	4014	4018	rBV6	678	699	0.03%	0.005%
95	14.095	4057	4060	4062	rBV3	1070	746	0.03%	0.005%
96	14.204	4089	4094	4095	rBV5	936	849	0.04%	0.006%
97	14.214	4095	4097	4100	rVB3	1077	591	0.03%	0.004%
98	14.249	4105	4108	4109	rBV2	1031	566	0.03%	0.004%
99	14.583	4208	4212	4213	rBV3	1003	746	0.03%	0.005%
100	14.750	4262	4264	4267	rBV5	973	555	0.03%	0.004%




Sum of corrected areas: 14383340

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
Data File : VV036779.D
Acq On : 05 Aug 2024 12:25
Operator : SY/MD
Sample : P3437-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05T8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

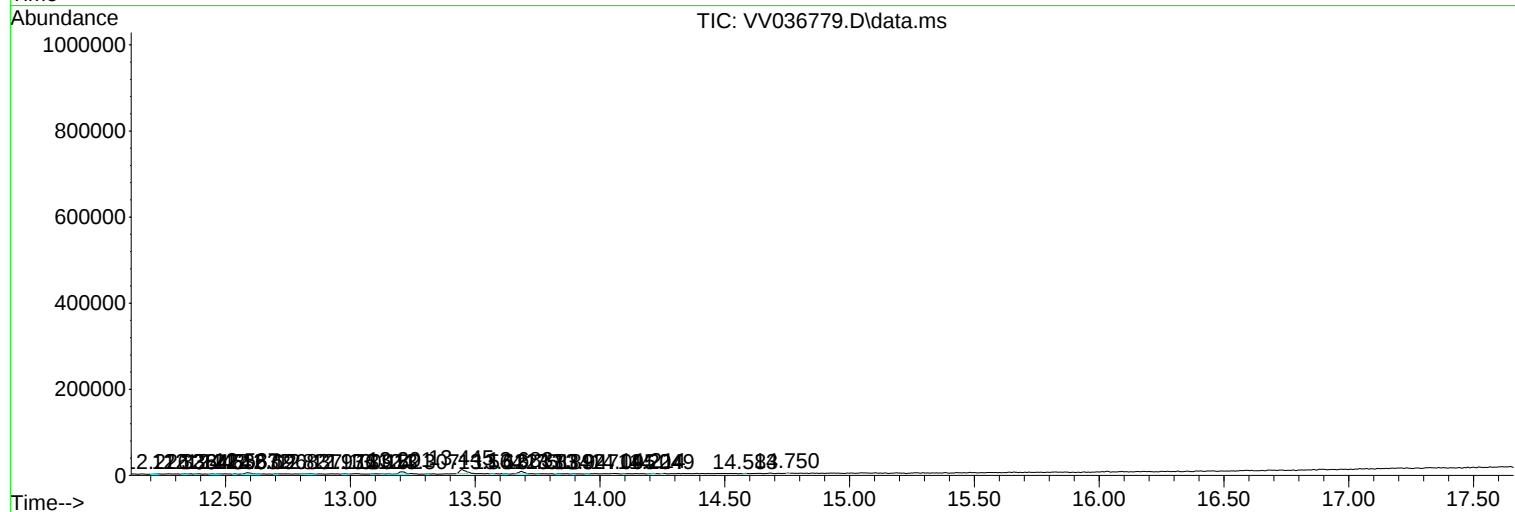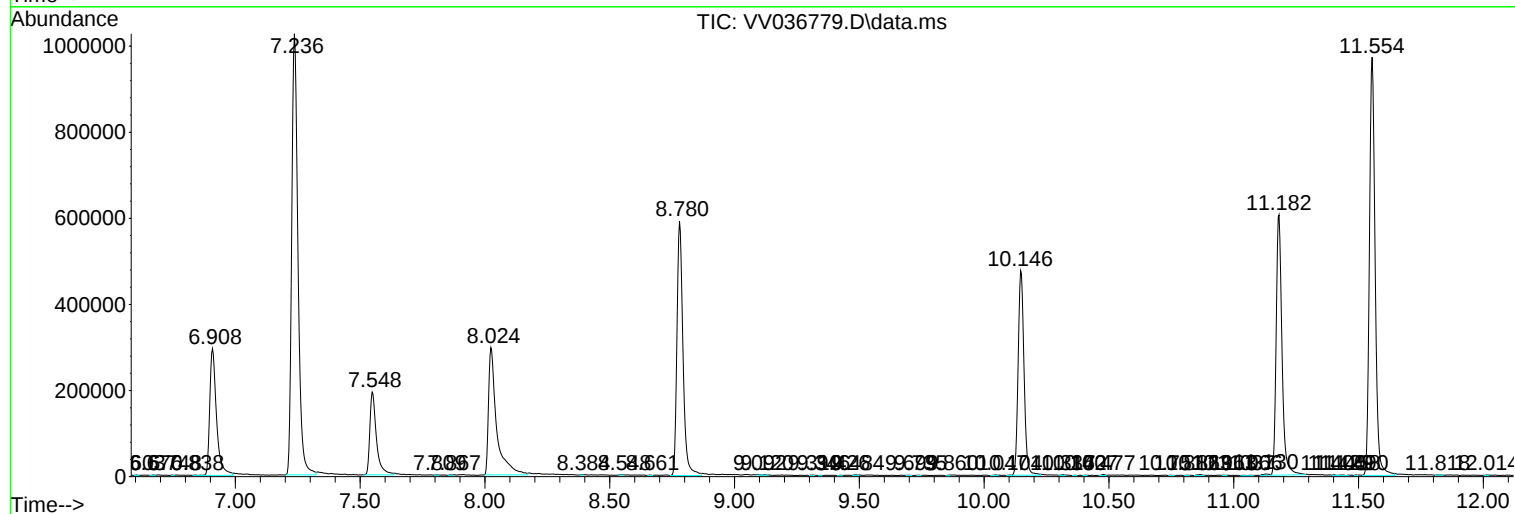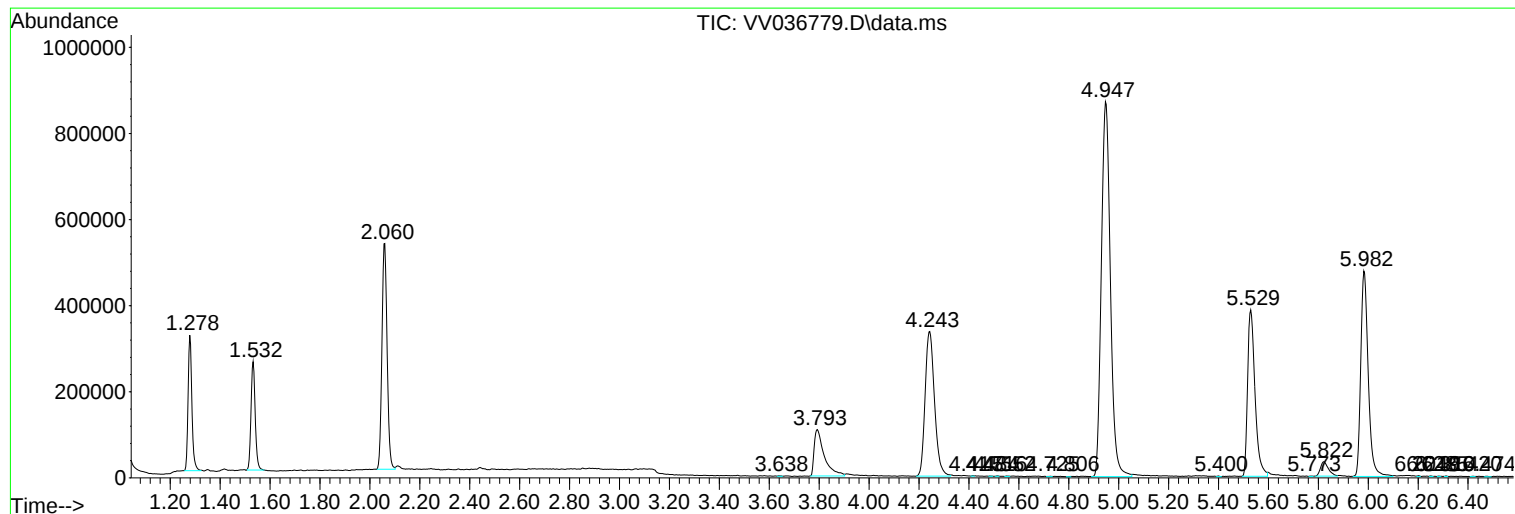

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
Data File : VV036779.D
Acq On : 05 Aug 2024 12:25
Operator : SY/MD
Sample : P3437-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05T8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
Data File : VV036779.D
Acq On : 05 Aug 2024 12:25
Operator : SY/MD
Sample : P3437-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05T8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc