

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
 Data File : VV036783.D
 Acq On : 05 Aug 2024 13:52
 Operator : SY/MD
 Sample : P3437-05
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05W5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036783.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	325664	351603	15.28%	2.303%
2	1.532	147	153	169	rVB	265434	310012	13.47%	2.030%
3	2.060	309	317	331	rVB	533707	757537	32.91%	4.961%
4	3.796	848	857	885	rBV	121073	326283	14.18%	2.137%
5	4.246	981	997	1026	rBV	349998	887922	38.57%	5.815%
6	4.568	1095	1097	1099	rBV2	889	473	0.02%	0.003%
7	4.732	1145	1148	1149	rBV3	780	387	0.02%	0.003%
8	4.757	1154	1156	1162	rVB5	970	1004	0.04%	0.007%
9	4.786	1162	1165	1168	rBV4	1186	763	0.03%	0.005%
10	4.809	1168	1172	1175	rBV7	733	797	0.03%	0.005%
11	4.883	1193	1195	1200	rBV6	832	794	0.03%	0.005%
12	4.950	1200	1216	1259	rVV2	910406	2301814	100.00%	15.076%
13	5.532	1386	1397	1422	rBV	453231	927376	40.29%	6.074%
14	5.825	1478	1488	1506	rBV3	28381	64580	2.81%	0.423%
15	5.986	1525	1538	1572	rBV	502094	1034782	44.96%	6.777%
16	6.256	1620	1622	1625	rVB3	731	317	0.01%	0.002%
17	6.342	1647	1649	1650	rBV	1020	373	0.02%	0.002%
18	6.423	1670	1674	1677	rBV4	1243	1029	0.04%	0.007%
19	6.455	1680	1684	1686	rBV5	1125	763	0.03%	0.005%
20	6.535	1706	1709	1710	rBV4	637	307	0.01%	0.002%
21	6.635	1738	1740	1743	rBV4	570	342	0.01%	0.002%
22	6.815	1794	1796	1798	rBV3	512	231	0.01%	0.002%
23	6.847	1802	1806	1808	rVB4	659	419	0.02%	0.003%
24	6.912	1814	1826	1854	rBV	302559	575124	24.99%	3.767%
25	7.239	1917	1928	1958	rBV	1060413	1868472	81.17%	12.237%
26	7.551	2016	2025	2052	rBV	196192	361840	15.72%	2.370%
27	7.950	2146	2149	2151	rBV3	684	361	0.02%	0.002%
28	8.027	2164	2173	2217	rBV2	330444	728578	31.65%	4.772%
29	8.664	2367	2371	2375	rBV4	1019	972	0.04%	0.006%
30	8.780	2397	2407	2434	rBV	678730	1133101	49.23%	7.421%
31	9.182	2531	2532	2533	rBV	712	247	0.01%	0.002%
32	9.275	2556	2561	2563	rBV4	663	489	0.02%	0.003%
33	9.378	2590	2593	2594	rBV	418	233	0.01%	0.002%
34	9.407	2600	2602	2606	rVB4	663	436	0.02%	0.003%
35	9.461	2615	2619	2620	rBV3	628	369	0.02%	0.002%
36	9.529	2637	2640	2641	rBV2	764	438	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
 Data File : VV036783.D
 Acq On : 05 Aug 2024 13:52
 Operator : SY/MD
 Sample : P3437-05
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05W5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	9.596	2660	2661	2663	rVB	330	65	0.00%	0.000%
38	9.609	2663	2665	2666	rBV2	303	133	0.01%	0.001%
39	9.651	2676	2678	2683	rVB4	1120	801	0.03%	0.005%
40	9.686	2683	2689	2692	rBV6	927	930	0.04%	0.006%
41	9.757	2707	2711	2712	rBV2	903	570	0.02%	0.004%
42	9.786	2717	2720	2722	rBV4	790	611	0.03%	0.004%
43	9.870	2742	2746	2747	rBV3	681	477	0.02%	0.003%
44	9.944	2766	2769	2771	rVB4	720	327	0.01%	0.002%
45	9.998	2782	2786	2789	rBV5	1014	964	0.04%	0.006%
46	10.072	2808	2809	2810	rBV	319	84	0.00%	0.001%
47	10.149	2815	2833	2849	rBV	539685	847623	36.82%	5.551%
48	10.362	2896	2899	2902	rBV4	882	595	0.03%	0.004%
49	10.564	2960	2962	2965	rBV4	491	269	0.01%	0.002%
50	10.603	2970	2974	2978	rBV5	734	714	0.03%	0.005%
51	10.693	3000	3002	3003	rBV3	492	238	0.01%	0.002%
52	10.731	3012	3014	3017	rBV4	621	381	0.02%	0.002%
53	10.808	3036	3038	3040	rBV3	802	425	0.02%	0.003%
54	10.834	3042	3046	3048	rVV4	565	465	0.02%	0.003%
55	10.863	3051	3055	3058	rBV5	1239	936	0.04%	0.006%
56	10.940	3076	3079	3080	rBV3	616	220	0.01%	0.001%
57	10.953	3080	3083	3086	rVV2	707	417	0.02%	0.003%
58	11.040	3108	3110	3111	rBV2	547	205	0.01%	0.001%
59	11.108	3125	3131	3132	rBV4	1067	822	0.04%	0.005%
60	11.181	3143	3154	3179	rBV	705974	1125769	48.91%	7.373%
61	11.445	3230	3236	3237	rBV4	903	826	0.04%	0.005%
62	11.554	3257	3270	3301	rBV	1025971	1635630	71.06%	10.712%
63	11.895	3372	3376	3379	rBV5	1180	1124	0.05%	0.007%
64	12.017	3412	3414	3415	rBV2	532	200	0.01%	0.001%
65	12.162	3456	3459	3461	rBV5	697	467	0.02%	0.003%
66	12.201	3469	3471	3472	rBV3	723	263	0.01%	0.002%
67	12.243	3481	3484	3488	rBV4	872	700	0.03%	0.005%
68	12.262	3488	3490	3492	rBV2	476	309	0.01%	0.002%
69	12.275	3492	3494	3498	rBV5	679	528	0.02%	0.003%
70	12.368	3520	3523	3527	rVB5	853	629	0.03%	0.004%
71	12.538	3574	3576	3577	rBV2	580	248	0.01%	0.002%
72	12.722	3630	3633	3636	rVB4	533	332	0.01%	0.002%
73	12.741	3636	3639	3640	rBV2	702	468	0.02%	0.003%
74	12.779	3650	3651	3655	rBV3	304	205	0.01%	0.001%
75	12.821	3660	3664	3665	rBV5	773	499	0.02%	0.003%
76	13.339	3823	3825	3826	rBV	811	339	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
Data File : VV036783.D
Acq On : 05 Aug 2024 13:52
Operator : SY/MD
Sample : P3437-05
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05W5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Title : VOC Analysis

77	13.622	3911	3913	3914	rVB2	671	203	0.01%	0.001%
78	13.635	3914	3917	3919	rBV2	1295	879	0.04%	0.006%




Sum of corrected areas: 15268458

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
Data File : VV036783.D
Acq On : 05 Aug 2024 13:52
Operator : SY/MD
Sample : P3437-05
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05W5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

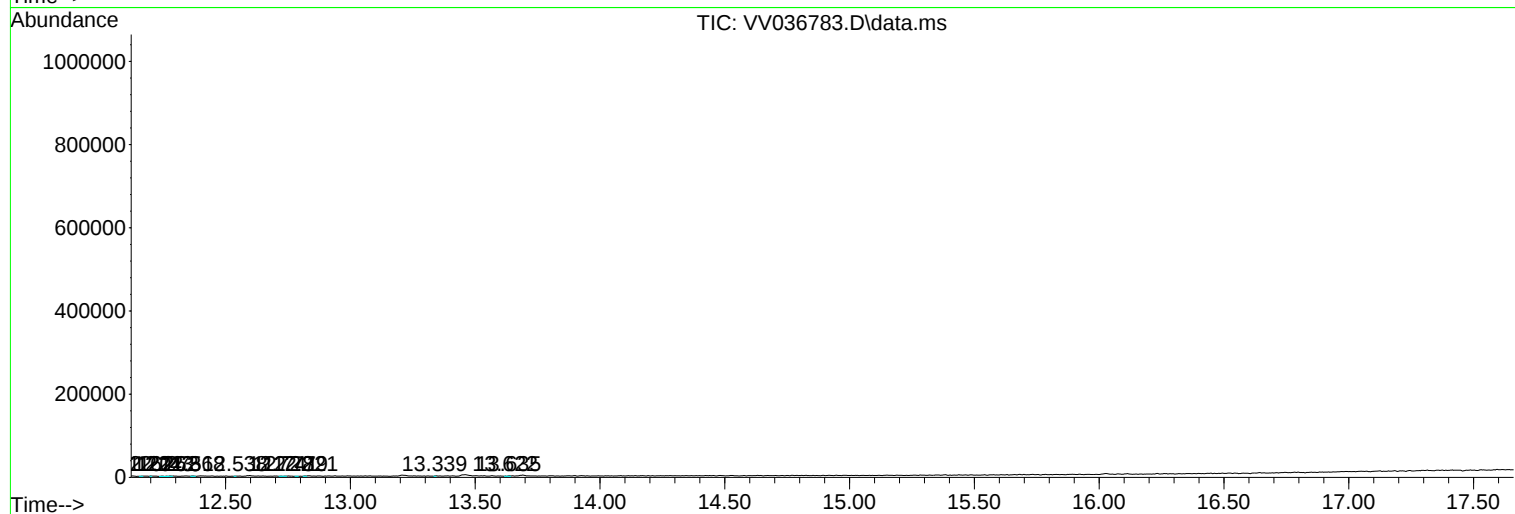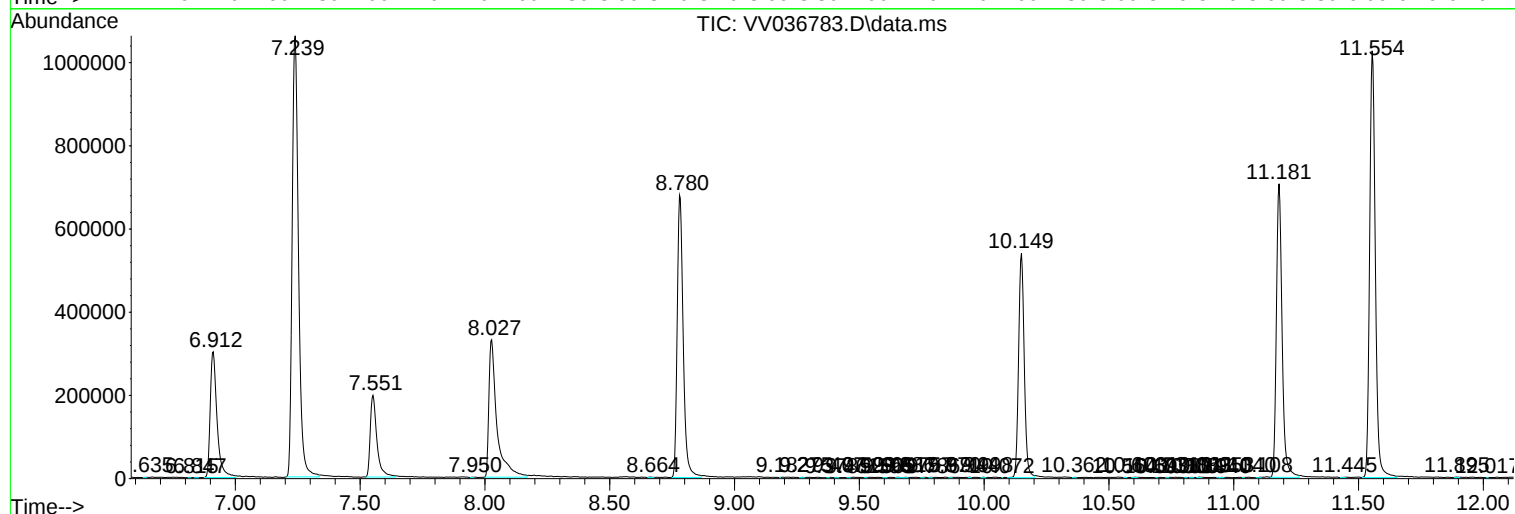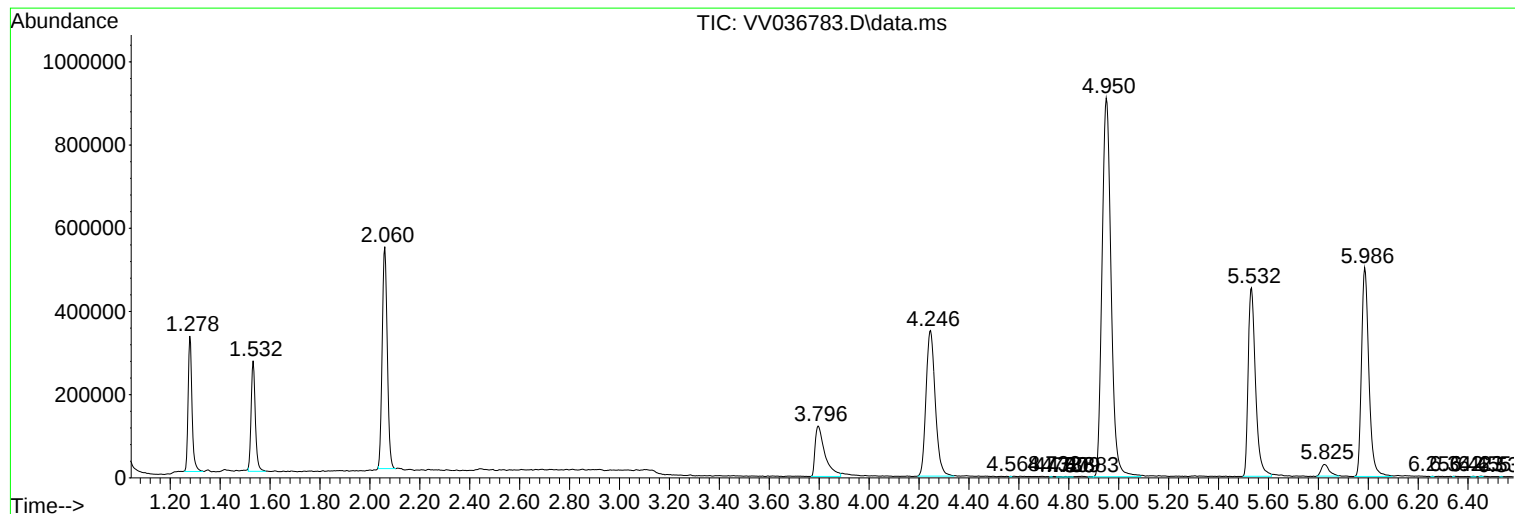

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
Data File : VV036783.D
Acq On : 05 Aug 2024 13:52
Operator : SY/MD
Sample : P3437-05
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05W5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
Data File : VV036783.D
Acq On : 05 Aug 2024 13:52
Operator : SY/MD
Sample : P3437-05
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05W5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc