

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
 Data File : VV036786.D
 Acq On : 05 Aug 2024 14:57
 Operator : SY/MD
 Sample : P3437-11
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036786.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	304706	316250	15.24%	2.072%
2	1.532	146	153	171	rVB	241702	283125	13.65%	1.855%
3	2.060	307	317	329	rBV	488875	702139	33.84%	4.600%
4	3.507	765	767	771	rVB4	1014	582	0.03%	0.004%
5	3.548	778	780	785	rBV5	1331	999	0.05%	0.007%
6	3.622	800	803	804	rBV3	1214	774	0.04%	0.005%
7	3.799	849	858	887	rBV	113620	312014	15.04%	2.044%
8	4.246	980	997	1027	rBV	316585	809789	39.03%	5.305%
9	4.474	1064	1068	1072	rBV4	928	707	0.03%	0.005%
10	4.519	1079	1082	1084	rBV3	694	588	0.03%	0.004%
11	4.654	1118	1124	1126	rVB6	1536	1479	0.07%	0.010%
12	4.677	1127	1131	1134	rBV5	1306	844	0.04%	0.006%
13	4.699	1134	1138	1141	rBV6	887	681	0.03%	0.004%
14	4.818	1171	1175	1178	rVB5	982	823	0.04%	0.005%
15	4.950	1198	1216	1254	rBV2	830053	2074613	100.00%	13.591%
16	5.371	1345	1347	1350	rVB3	997	476	0.02%	0.003%
17	5.532	1385	1397	1428	rBV	599530	1225209	59.06%	8.026%
18	5.825	1476	1488	1505	rBV2	29536	67548	3.26%	0.443%
19	5.986	1524	1538	1570	rBV	452065	940403	45.33%	6.161%
20	6.487	1691	1694	1695	rBV2	1151	650	0.03%	0.004%
21	6.696	1757	1759	1764	rVB3	1005	847	0.04%	0.006%
22	6.722	1764	1767	1770	rBV3	926	649	0.03%	0.004%
23	6.783	1784	1786	1789	rBV3	1021	697	0.03%	0.005%
24	6.831	1799	1801	1805	rVB4	923	705	0.03%	0.005%
25	6.912	1816	1826	1853	rBV	271793	511354	24.65%	3.350%
26	7.098	1882	1884	1889	rVB4	912	534	0.03%	0.003%
27	7.149	1897	1900	1903	rBV5	1602	996	0.05%	0.007%
28	7.240	1917	1928	1963	rVV	973717	1705080	82.19%	11.170%
29	7.551	2016	2025	2051	rBV	178924	324371	15.64%	2.125%
30	7.767	2089	2092	2094	rBV3	832	554	0.03%	0.004%
31	7.850	2115	2118	2121	rBV4	699	493	0.02%	0.003%
32	7.905	2132	2135	2141	rBV7	1420	1577	0.08%	0.010%
33	7.928	2141	2142	2147	rVB4	1041	526	0.03%	0.003%
34	7.976	2152	2157	2158	rBV4	672	532	0.03%	0.003%
35	8.027	2163	2173	2211	rBV2	327265	702360	33.85%	4.601%
36	8.545	2328	2334	2336	rBV6	1399	1472	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
 Data File : VV036786.D
 Acq On : 05 Aug 2024 14:57
 Operator : SY/MD
 Sample : P3437-11
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	8.635	2359	2362	2366	rVB4	1369	1030	0.05%	0.007%
38	8.709	2379	2385	2389	rBV7	987	1415	0.07%	0.009%
39	8.780	2396	2407	2442	rBV	900285	1493948	72.01%	9.787%
40	9.098	2502	2506	2508	rBV4	950	872	0.04%	0.006%
41	9.217	2539	2543	2545	rBV4	636	499	0.02%	0.003%
42	9.365	2585	2589	2591	rVB5	704	452	0.02%	0.003%
43	9.378	2591	2593	2598	rBV4	672	606	0.03%	0.004%
44	9.487	2622	2627	2630	rBV6	720	694	0.03%	0.005%
45	9.548	2643	2646	2649	rBV2	1328	845	0.04%	0.006%
46	9.648	2674	2677	2680	rVB6	1190	799	0.04%	0.005%
47	9.667	2680	2683	2688	rBV6	933	665	0.03%	0.004%
48	9.825	2729	2732	2737	rVB4	897	752	0.04%	0.005%
49	9.863	2737	2744	2747	rBV5	1056	1409	0.07%	0.009%
50	10.001	2785	2787	2793	rBV6	747	508	0.02%	0.003%
51	10.043	2798	2800	2806	rVB6	1226	960	0.05%	0.006%
52	10.069	2806	2808	2810	rBV3	996	579	0.03%	0.004%
53	10.149	2821	2833	2857	rBV	483504	778647	37.53%	5.101%
54	10.317	2882	2885	2887	rBV5	1017	609	0.03%	0.004%
55	10.442	2920	2924	2927	rBV4	723	517	0.02%	0.003%
56	10.484	2933	2937	2939	rBV5	1204	888	0.04%	0.006%
57	10.500	2939	2942	2948	rVV6	795	677	0.03%	0.004%
58	10.535	2949	2953	2956	rVV6	809	566	0.03%	0.004%
59	10.619	2973	2979	2981	rVV4	1256	916	0.04%	0.006%
60	10.927	3069	3075	3078	rVB5	977	1054	0.05%	0.007%
61	10.995	3094	3096	3100	rVB5	690	452	0.02%	0.003%
62	11.098	3123	3128	3132	rBV6	993	1011	0.05%	0.007%
63	11.127	3132	3137	3140	rBV7	1370	1611	0.08%	0.011%
64	11.181	3143	3154	3187	rVV	932027	1464341	70.58%	9.593%
65	11.474	3243	3245	3248	rVB2	1037	528	0.03%	0.003%
66	11.493	3248	3251	3253	rBV3	1319	885	0.04%	0.006%
67	11.554	3259	3270	3300	rBV	916250	1482481	71.46%	9.712%
68	11.828	3351	3355	3356	rBV4	606	459	0.02%	0.003%
69	11.976	3398	3401	3404	rBV4	1136	832	0.04%	0.005%
70	12.111	3438	3443	3448	rVV4	981	1097	0.05%	0.007%
71	12.178	3461	3464	3467	rVB4	936	539	0.03%	0.004%
72	12.210	3472	3474	3480	rVB6	841	729	0.04%	0.005%
73	12.255	3483	3488	3490	rBV6	1150	895	0.04%	0.006%
74	12.284	3494	3497	3501	rVB3	1157	794	0.04%	0.005%
75	12.323	3501	3509	3513	rBV7	1388	1854	0.09%	0.012%
76	12.355	3513	3519	3523	rBV7	609	704	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
 Data File : VV036786.D
 Acq On : 05 Aug 2024 14:57
 Operator : SY/MD
 Sample : P3437-11
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	12.452	3543	3549	3551	rBV6	1236	1168	0.06%	0.008%
78	12.474	3554	3556	3560	rBV5	674	548	0.03%	0.004%
79	12.529	3569	3573	3576	rBV3	692	654	0.03%	0.004%
80	12.587	3588	3591	3593	rBV3	1066	682	0.03%	0.004%
81	12.792	3650	3655	3657	rBV3	1423	1063	0.05%	0.007%
82	12.979	3708	3713	3717	rBV7	1237	1422	0.07%	0.009%
83	13.005	3717	3721	3725	rVV6	744	717	0.03%	0.005%
84	13.027	3725	3728	3733	rBV6	725	683	0.03%	0.004%
85	13.085	3743	3746	3748	rBV3	919	606	0.03%	0.004%
86	13.149	3764	3766	3769	rBV4	908	502	0.02%	0.003%
87	13.217	3778	3787	3791	rBV6	2527	4183	0.20%	0.027%
88	13.458	3858	3862	3864	rBV3	1747	1272	0.06%	0.008%
89	13.570	3894	3897	3902	rVB7	772	720	0.03%	0.005%
90	13.599	3903	3906	3910	rBV3	874	705	0.03%	0.005%
91	13.648	3920	3921	3925	rVB4	918	505	0.02%	0.003%
92	13.683	3925	3932	3935	rBV7	1976	1998	0.10%	0.013%
93	13.918	4002	4005	4007	rBV3	875	631	0.03%	0.004%
94	13.931	4007	4009	4011	rVV3	1046	484	0.02%	0.003%
95	13.998	4025	4030	4036	rBV5	900	1314	0.06%	0.009%
96	14.194	4087	4091	4093	rBV4	984	768	0.04%	0.005%
97	14.593	4212	4215	4216	rBV3	1270	643	0.03%	0.004%
98	14.641	4228	4230	4235	rVB4	937	672	0.03%	0.004%
99	14.792	4274	4277	4281	rVB5	1323	806	0.04%	0.005%
100	15.104	4371	4374	4376	rBV4	1344	687	0.03%	0.005%




Sum of corrected areas: 15264992

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
Data File : VV036786.D
Acq On : 05 Aug 2024 14:57
Operator : SY/MD
Sample : P3437-11
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

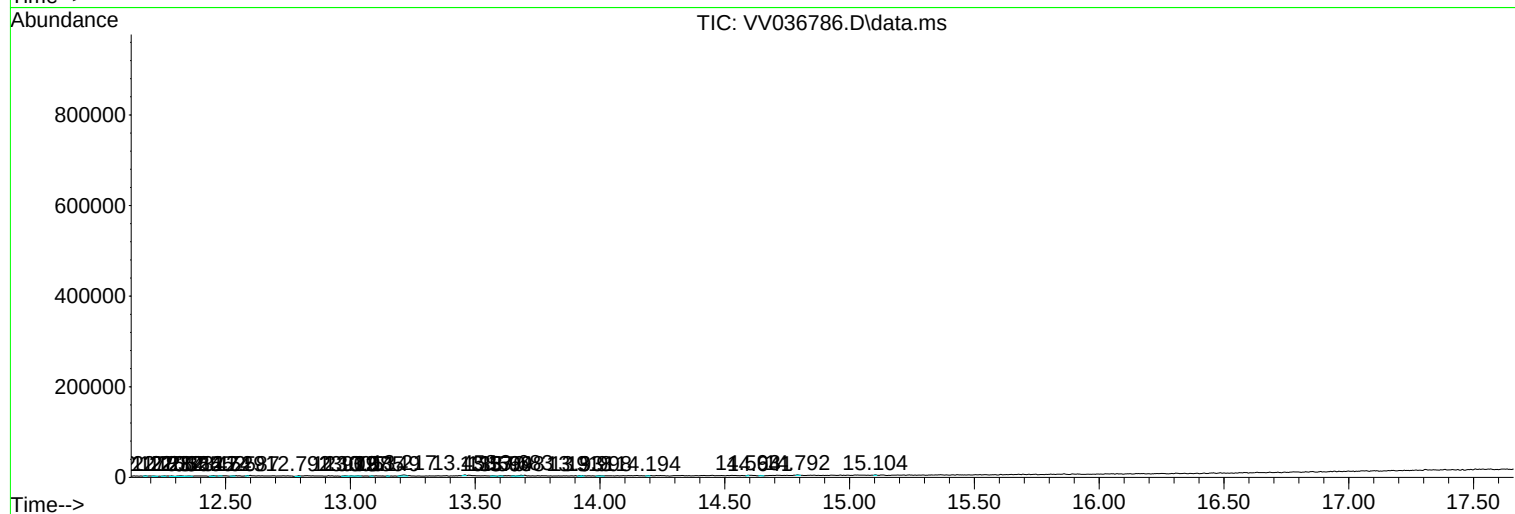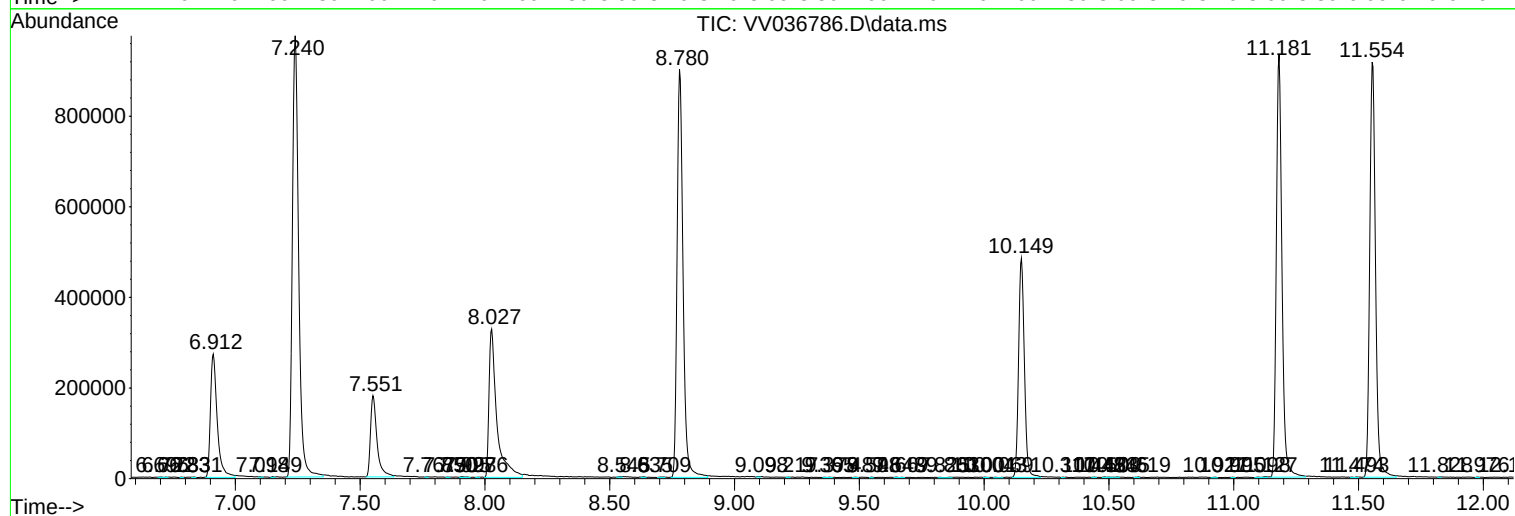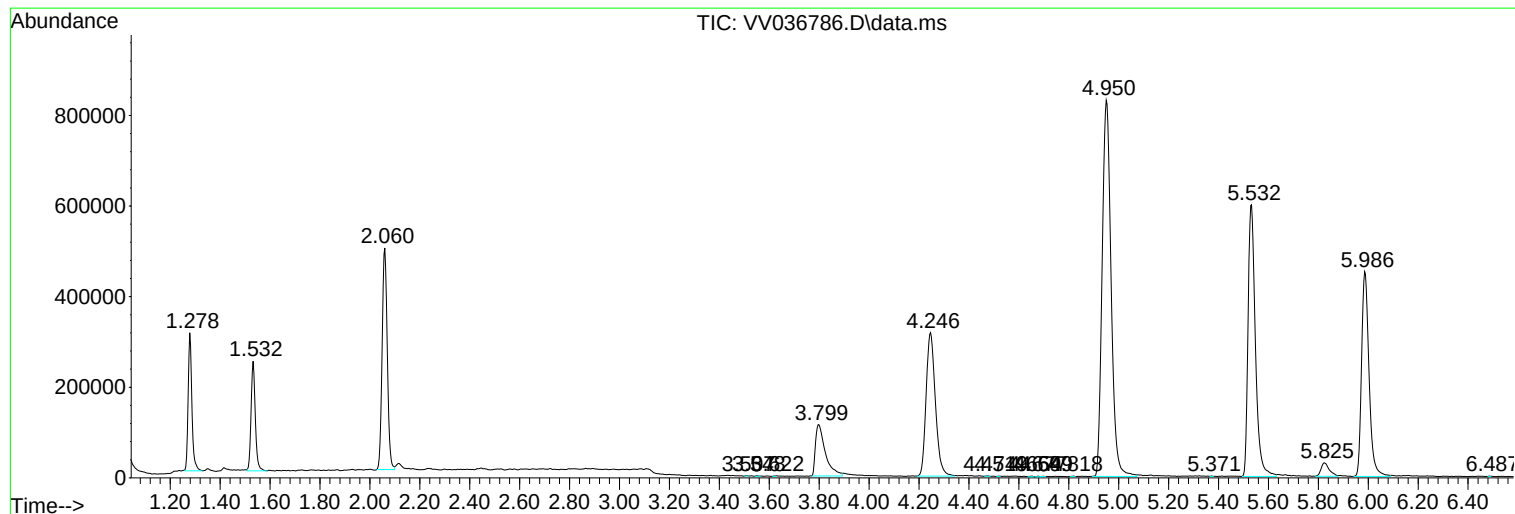

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
Data File : VV036786.D
Acq On : 05 Aug 2024 14:57
Operator : SY/MD
Sample : P3437-11
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
Data File : VV036786.D
Acq On : 05 Aug 2024 14:57
Operator : SY/MD
Sample : P3437-11
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc