
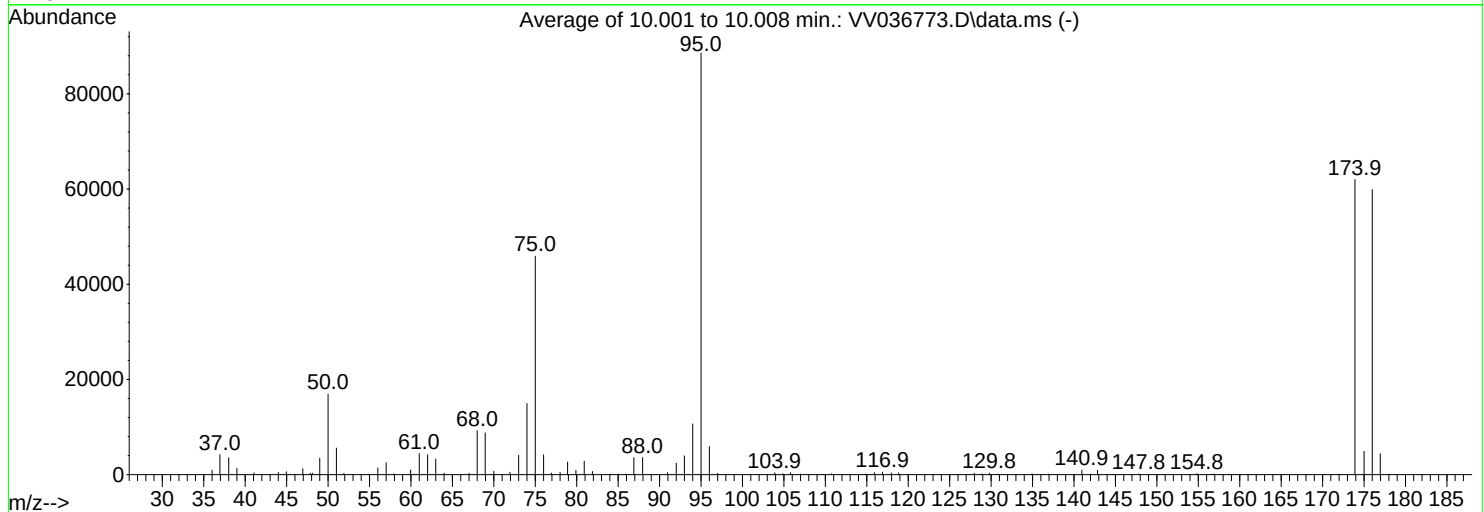


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080524\
Data File : VV036773.D
Acq On : 05 Aug 2024 08:49
Operator : SY/MD
Sample : BFB354
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB354

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR010422WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Jan 11 01:51:56 2022

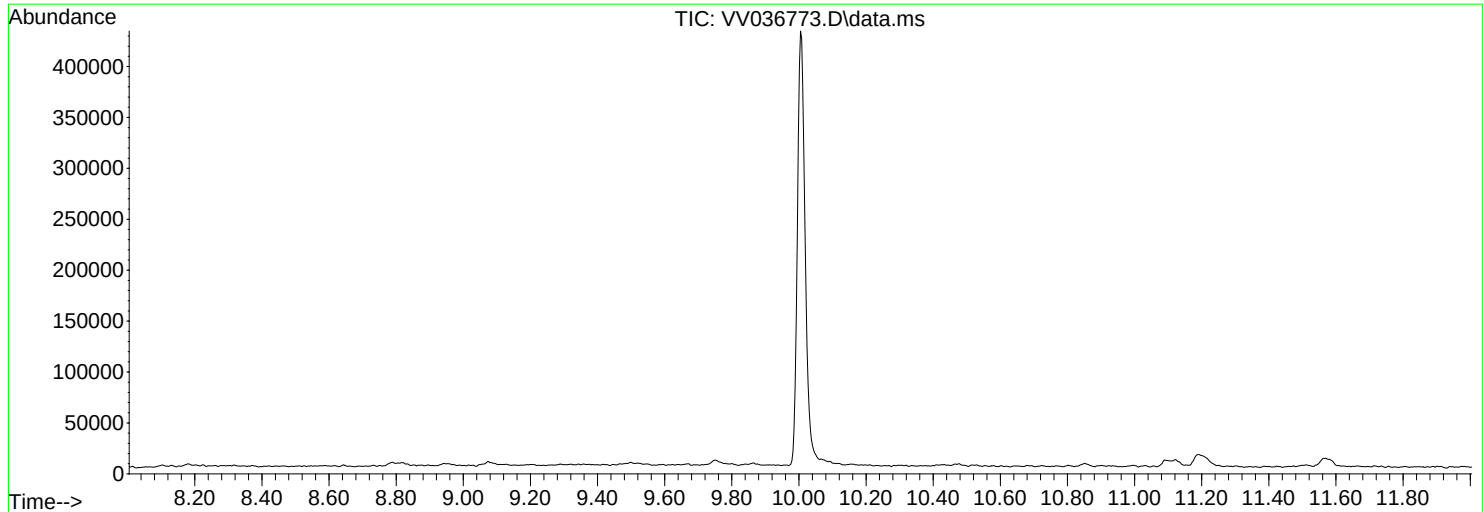

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2773

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	16920	PASS
75	95	30	80	51.8	45869	PASS
95	95	100	100	100.0	88608	PASS
96	95	5	9	6.7	5905	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.0	62005	PASS
175	174	5	9	7.9	4896	PASS
176	174	95	105	96.6	59888	PASS
177	176	5	10	7.3	4374	PASS

m/z	Abundance
36.00	2505.0
36.90	255.0
38.00	866.0
39.10	277.0
40.00	255.0
40.80	350.0
42.00	165.0
43.00	378.0
44.00	990.0
44.90	161.0
54.80	367.0
56.00	104.0
57.00	155.0
59.70	106.0
67.00	189.0
68.10	152.0
68.90	269.0
70.10	228.0
71.00	130.0
76.90	236.0
78.90	158.0
81.00	114.0
83.00	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB354

m/z	Abundance
36.00	3301.0
37.00	4434.0
38.00	4229.0
39.00	1518.0
40.00	311.0
41.10	433.0
42.00	158.0
43.10	446.0
44.00	1448.0
45.00	781.0
45.90	120.0
47.00	1281.0
47.90	447.0
49.00	3262.0
50.00	16664.0
51.00	5501.0
51.90	272.0
54.00	126.0
55.00	454.0
56.00	1358.0
57.00	2565.0
57.90	164.0
60.00	981.0
61.00	4277.0
62.00	4208.0
63.00	3214.0
64.00	348.0
67.00	564.0
68.00	8850.0
69.00	8943.0
70.00	857.0
71.10	167.0
71.90	513.0
73.00	3959.0
74.00	14162.0
75.00	43824.0
76.00	4132.0
77.00	533.0
78.00	468.0
78.90	2786.0
79.90	822.0
80.90	2756.0
81.90	681.0
82.90	197.0
84.10	106.0
85.10	135.0
85.90	128.0
86.90	3531.0
87.90	3561.0
91.00	437.0
92.00	2269.0
93.00	3884.0
94.00	9972.0
95.00	84704.0
96.00	5634.0
97.00	311.0
103.00	106.0
103.90	409.0
104.90	201.0
105.80	377.0
106.90	126.0
109.80	131.0
110.80	172.0
115.90	439.0
116.90	557.0
117.90	342.0
118.90	356.0
128.00	297.0
128.90	173.0
129.80	364.0
130.90	116.0
134.90	182.0
136.90	136.0
140.90	950.0
142.00	120.0
142.80	749.0
145.10	106.0
147.90	166.0
154.80	224.0
156.80	136.0
160.90	108.0
171.80	181.0
173.90	57600.0
175.00	4544.0
176.00	55704.0
177.00	4100.0
178.00	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB354

m/z	Abundance
36.00	3482.0
37.00	4632.0
38.00	4566.0
39.00	1609.0
40.00	300.0
41.00	401.0
42.10	136.0
43.10	471.0
44.00	1437.0
45.00	779.0
45.90	111.0
47.00	1300.0
48.10	466.0
49.00	3566.0
50.00	17344.0
51.00	5723.0
51.90	280.0
55.00	487.0
56.00	1582.0
57.00	2789.0
57.90	186.0
59.90	1024.0
61.00	4577.0
62.00	4273.0
63.00	3372.0
64.00	335.0
67.00	496.0
68.00	9740.0
69.00	9349.0
70.00	949.0
71.20	178.0
72.00	540.0
73.00	4153.0
74.00	15452.0
75.00	47464.0
76.00	4326.0
77.00	603.0
78.00	538.0
78.90	2892.0
79.90	919.0
80.90	3041.0
81.90	727.0
82.80	242.0
84.10	144.0
85.00	125.0
85.90	140.0
86.90	3690.0
88.00	3800.0
91.00	464.0
92.00	2496.0
93.00	4108.0
94.00	11066.0
95.00	91616.0
96.00	6073.0
97.00	280.0
103.00	112.0
103.90	434.0
104.80	202.0
105.80	409.0
107.00	128.0
110.70	197.0
114.80	129.0
115.90	442.0
116.90	548.0
118.00	400.0
118.80	356.0
127.90	286.0
128.80	174.0
129.80	367.0
130.90	135.0
134.90	187.0
136.90	150.0
141.00	1013.0
142.00	139.0
142.90	897.0
144.70	120.0
146.80	112.0
147.80	162.0
148.90	107.0
154.90	238.0
156.80	129.0
158.70	143.0
171.10	103.0
171.90	227.0
173.90	64080.0
175.00	5092.0
176.00	62096.0
176.90	4518.0
178.00	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB354

m/z	Abundance
36.00	3446.0
37.00	4272.0
38.00	4549.0
39.00	1603.0
40.10	272.0
41.00	360.0
42.00	141.0
43.10	465.0
44.00	1463.0
45.00	779.0
46.00	126.0
46.90	1134.0
47.80	424.0
48.10	477.0
49.00	3534.0
50.00	16752.0
51.00	5472.0
51.90	255.0
55.00	491.0
56.00	1613.0
57.00	2725.0
57.90	187.0
60.00	956.0
61.00	4402.0
62.00	4008.0
63.00	3253.0
64.00	285.0
67.00	376.0
68.00	9645.0
69.00	8799.0
70.00	993.0
71.20	170.0
72.00	517.0
73.00	4046.0
74.00	15269.0
75.00	46320.0
76.00	4055.0
77.00	608.0
78.00	494.0
78.90	2746.0
79.90	954.0
80.90	3062.0
81.90	644.0
82.90	257.0
84.10	136.0
84.90	115.0
85.90	131.0
86.90	3496.0
88.00	3483.0
90.90	421.0
92.00	2458.0
93.00	3847.0
94.00	10977.0
95.00	89504.0
96.00	6009.0
97.00	216.0
103.90	399.0
104.80	174.0
105.80	401.0
107.10	120.0
110.70	187.0
112.70	101.0
114.80	146.0
115.90	390.0
116.90	499.0
117.90	388.0
118.80	369.0
124.00	108.0
127.90	305.0
128.80	184.0
129.80	302.0
130.90	157.0
135.00	210.0
137.00	135.0
141.00	979.0
142.00	122.0
142.90	1015.0
144.80	125.0
146.80	140.0
147.80	154.0
150.10	113.0
154.90	207.0
156.80	133.0
158.70	156.0
171.20	110.0
172.10	209.0
173.90	64336.0
175.00	5051.0
176.00	61864.0
176.90	4505.0
178.00	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB354