


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036808.D
 Acq On : 06 Aug 2024 12:49
 Operator : SY/MD
 Sample : P3433-07 50X
 Misc : 1.26G/5 mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 07 05:01:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 07 04:57:18 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	437023	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	404692	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	198668	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	162225	46.475	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	92.960%	
7) Chloroethane-d5	1.529	69	134109	48.720	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	97.440%	
11) 1,1-Dichloroethene-d2	2.056	65	71767	48.066	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	96.140%	
21) 2-Butanone-d5	3.796	46	186170	100.664	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	100.660%	
24) Chloroform-d	4.243	84	309533	49.415	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.840%	
26) 1,2-Dichloroethane-d4	4.937	65	211489	52.512	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	105.020%	
32) Benzene-d6	4.953	84	645864	52.839	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	105.680%	
36) 1,2-Dichloropropane-d6	5.985	67	209740	53.188	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	106.380%	
41) Toluene-d8	7.239	98	574989	51.281	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	102.560%	
43) trans-1,3-Dichloroprop...	7.551	79	100147	48.799	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	97.600%	
47) 2-Hexanone-d5	8.024	63	114585	101.060	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	101.060%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	240577	53.133	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	106.260%	
66) 1,2-Dichlorobenzene-d4	11.557	152	217735	53.784	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	107.560%	
Target Compounds						
10) 1,1,2-Trichloro-1,2,2-...	2.059	101	2101	0.727	ug/L #	25
39) cis-1,3-Dichloropropene	6.911	75	6572	1.197	ug/L #	67

(#) = qualifier out of range (m) = manual integration (+) = signals summed



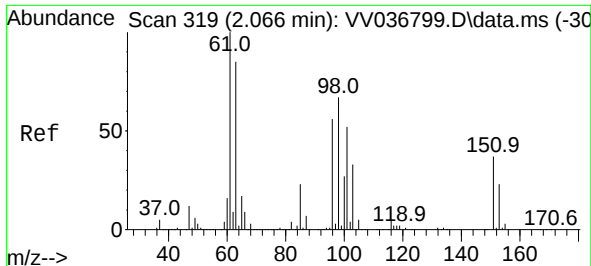


#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 0.727 ug/L
RT: 2.059 min Scan# 319
Delta R.T. -0.007 min
Lab File: VV036808.D
Acq: 06 Aug 2024 12:49

Instrument :
MSVOA_V
ClientSampleId :

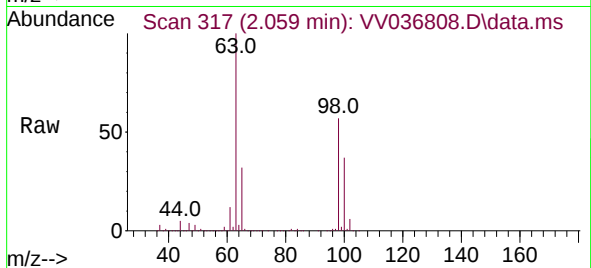

Tgt Ion:101 Resp: 2101
Ion Ratio Lower Upper
101 100
85 5.9 34.6 51.8#
151 0.0 55.9 83.9#

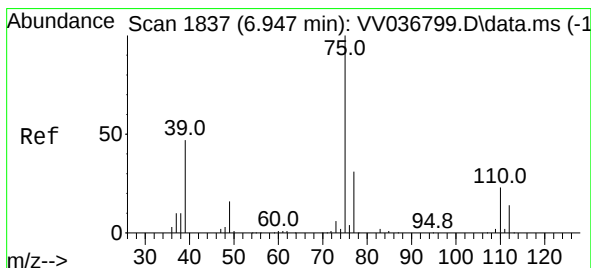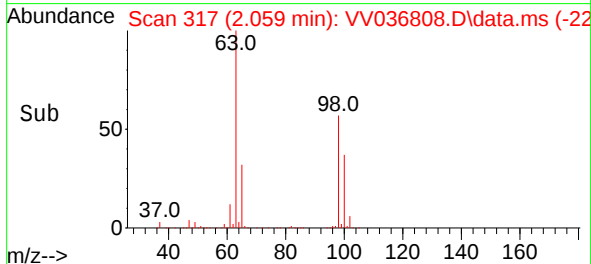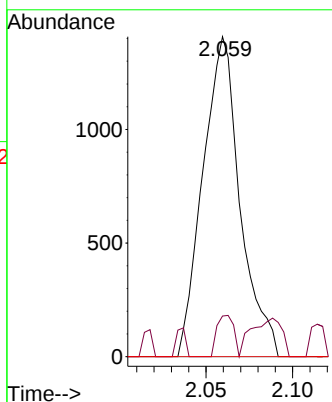

#39
cis-1,3-Dichloropropene
Concen: 1.197 ug/L
RT: 6.911 min Scan# 1826
Delta R.T. -0.036 min
Lab File: VV036808.D
Acq: 06 Aug 2024 12:49

Tgt Ion: 75 Resp: 6572
Ion Ratio Lower Upper
75 100
77 49.8 22.2 41.2#

