

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036803.D
 Acq On : 06 Aug 2024 10:58
 Operator : SY/MD
 Sample : P3437-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05T8

Quant Time: Aug 07 05:00:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 07 04:57:18 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	389875	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	368575	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.182	152	179812	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	176376	56.640	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery	= 113.280%		
7) Chloroethane-d5	1.532	69	144901	59.006	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery	= 118.020%		
11) 1,1-Dichloroethene-d2	2.060	65	79303	59.536	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery	= 119.080%		
21) 2-Butanone-d5	3.796	46	178538	108.212	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery	= 108.210%		
24) Chloroform-d	4.246	84	333346	59.652	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery	= 119.300%		
26) 1,2-Dichloroethane-d4	4.937	65	223889	62.314	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery	= 124.620%		
32) Benzene-d6	4.953	84	692984	62.250	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery	= 124.500%		
36) 1,2-Dichloropropane-d6	5.986	67	225918	62.904	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery	= 125.800%#		
41) Toluene-d8	7.240	98	620851	60.798	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery	= 121.600%#		
43) trans-1,3-Dichloroprop...	7.551	79	109840	58.767	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery	= 117.540%		
47) 2-Hexanone-d5	8.024	63	112808	109.242	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery	= 109.240%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	242405	58.783	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery	= 117.560%		
66) 1,2-Dichlorobenzene-d4	11.554	152	228520	62.367	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery	= 124.740%#		
Target Compounds						
13) Acetone	2.114	43	8752	6.340	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036803.D
Acq On : 06 Aug 2024 10:58
Operator : SY/MD
Sample : P3437-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05T8

Quant Time: Aug 07 05:00:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 07 04:57:18 2024
Response via : Initial Calibration

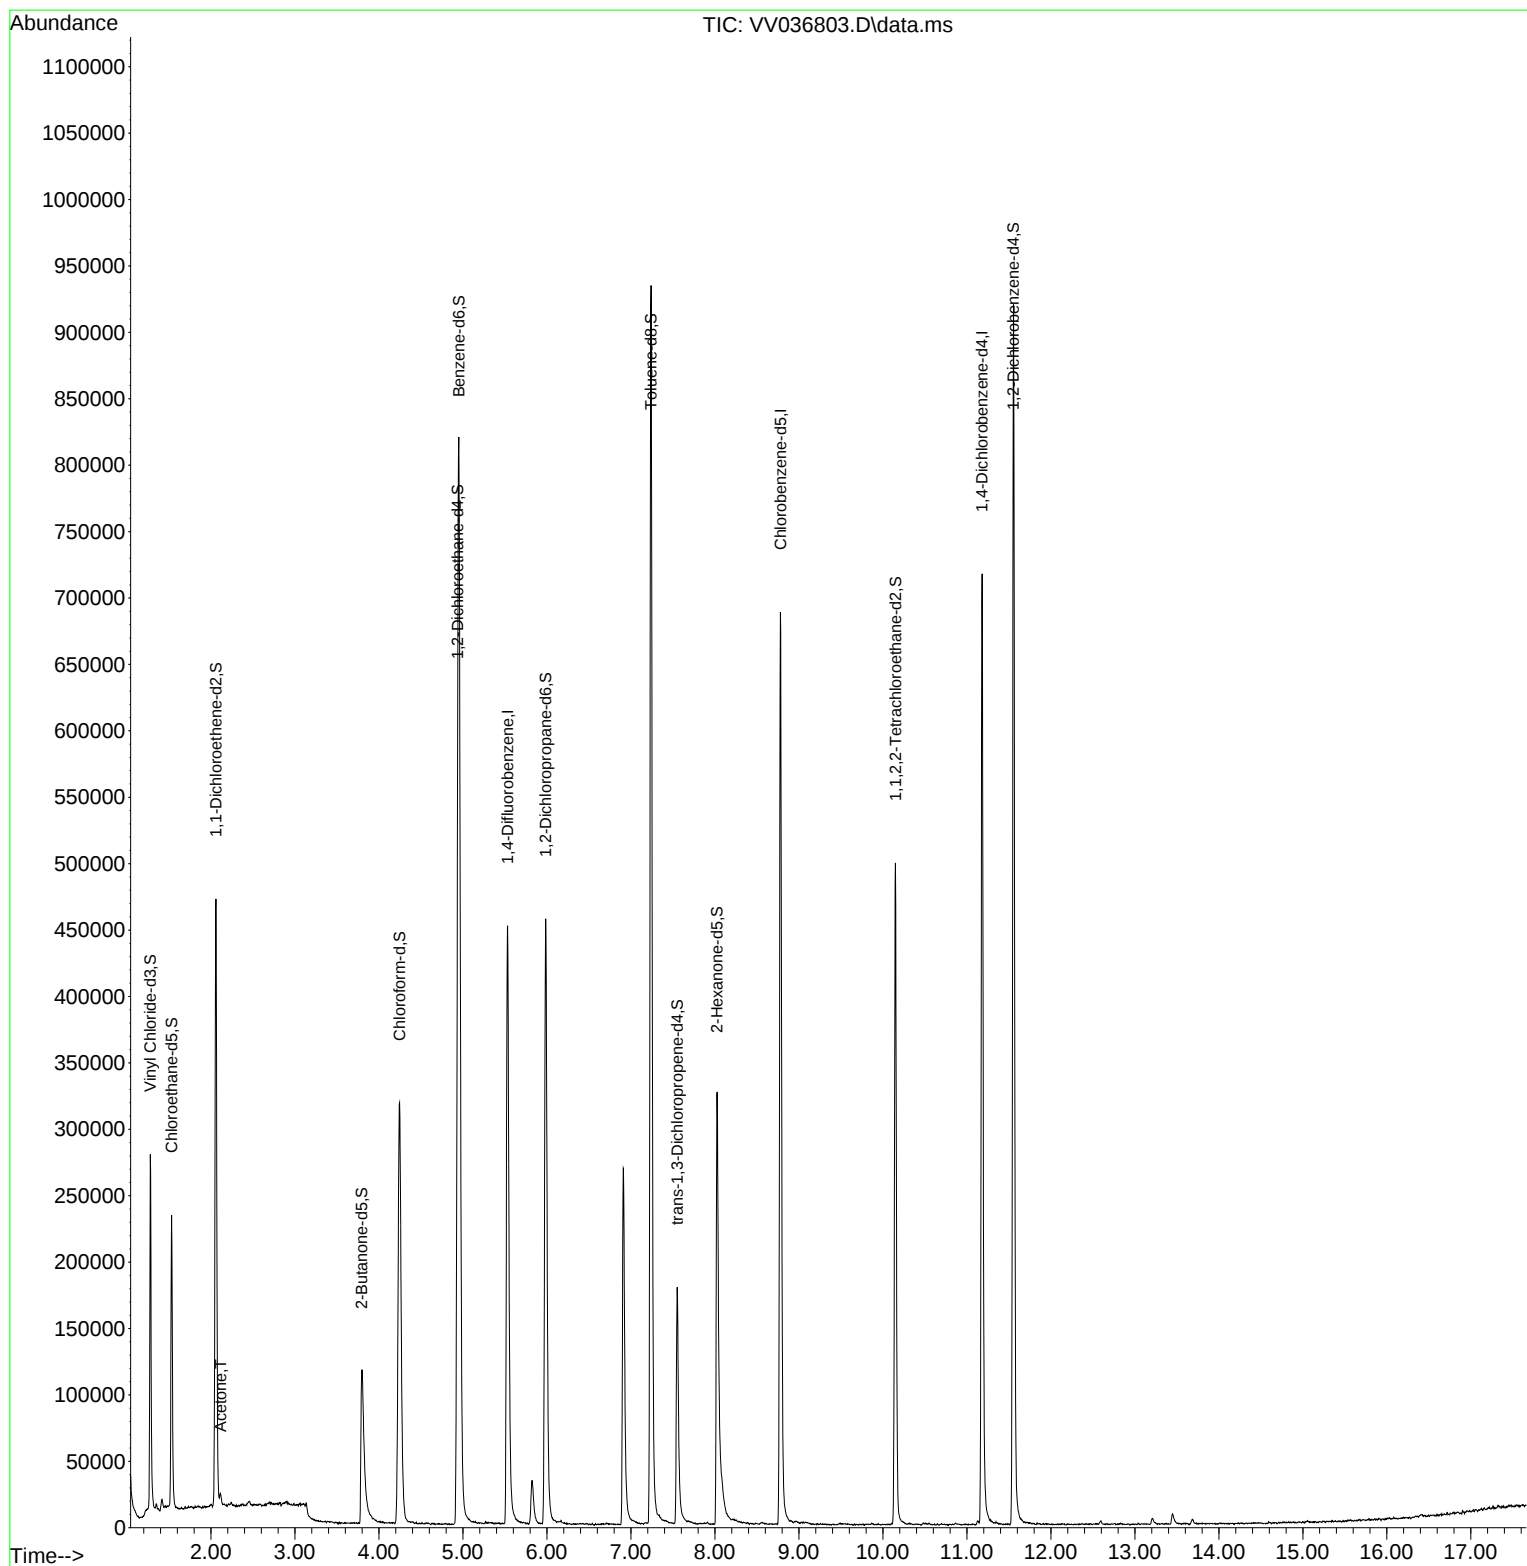

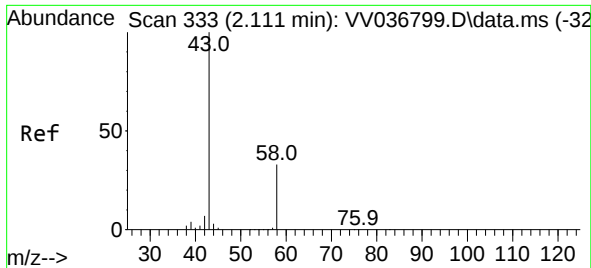

#13
 Acetone
 Concen: 6.340 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV036803.D
 Acq: 06 Aug 2024 10:58

Instrument :
 MSVOA_V
 ClientSampleId :
 E05T8

Tgt Ion: 43 Resp: 8752
 Ion Ratio Lower Upper
 43 100
 58 36.6 0.0 63.4

