

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036804.D
 Acq On : 06 Aug 2024 11:20
 Operator : SY/MD
 Sample : P3437-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05T9

Quant Time: Aug 07 05:00:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 07 04:57:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	449080	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	420022	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	203577	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	168012	46.841	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	93.680%	
7) Chloroethane-d5	1.532	69	137921	48.759	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	97.520%	
11) 1,1-Dichloroethene-d2	2.059	65	74371	48.473	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	96.940%	
21) 2-Butanone-d5	3.799	46	180535	94.997	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	95.000%	
24) Chloroform-d	4.246	84	317534	49.331	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.660%	
26) 1,2-Dichloroethane-d4	4.940	65	212658	51.385	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	102.760%	
32) Benzene-d6	4.953	84	655834	51.697	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	103.400%	
36) 1,2-Dichloropropane-d6	5.985	67	215085	52.552	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	105.100%	
41) Toluene-d8	7.239	98	588478	50.569	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	101.140%	
43) trans-1,3-Dichloroprop...	7.551	79	102012	47.893	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	95.780%	
47) 2-Hexanone-d5	8.024	63	107241	91.131	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	91.130%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	235723	50.161	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	100.320%	
66) 1,2-Dichlorobenzene-d4	11.554	152	217076	52.328	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	104.660%	
Target Compounds						
					Qvalue	
13) Acetone	2.114	43	9578	6.024	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036804.D
Acq On : 06 Aug 2024 11:20
Operator : SY/MD
Sample : P3437-02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05T9

Quant Time: Aug 07 05:00:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 07 04:57:18 2024
Response via : Initial Calibration

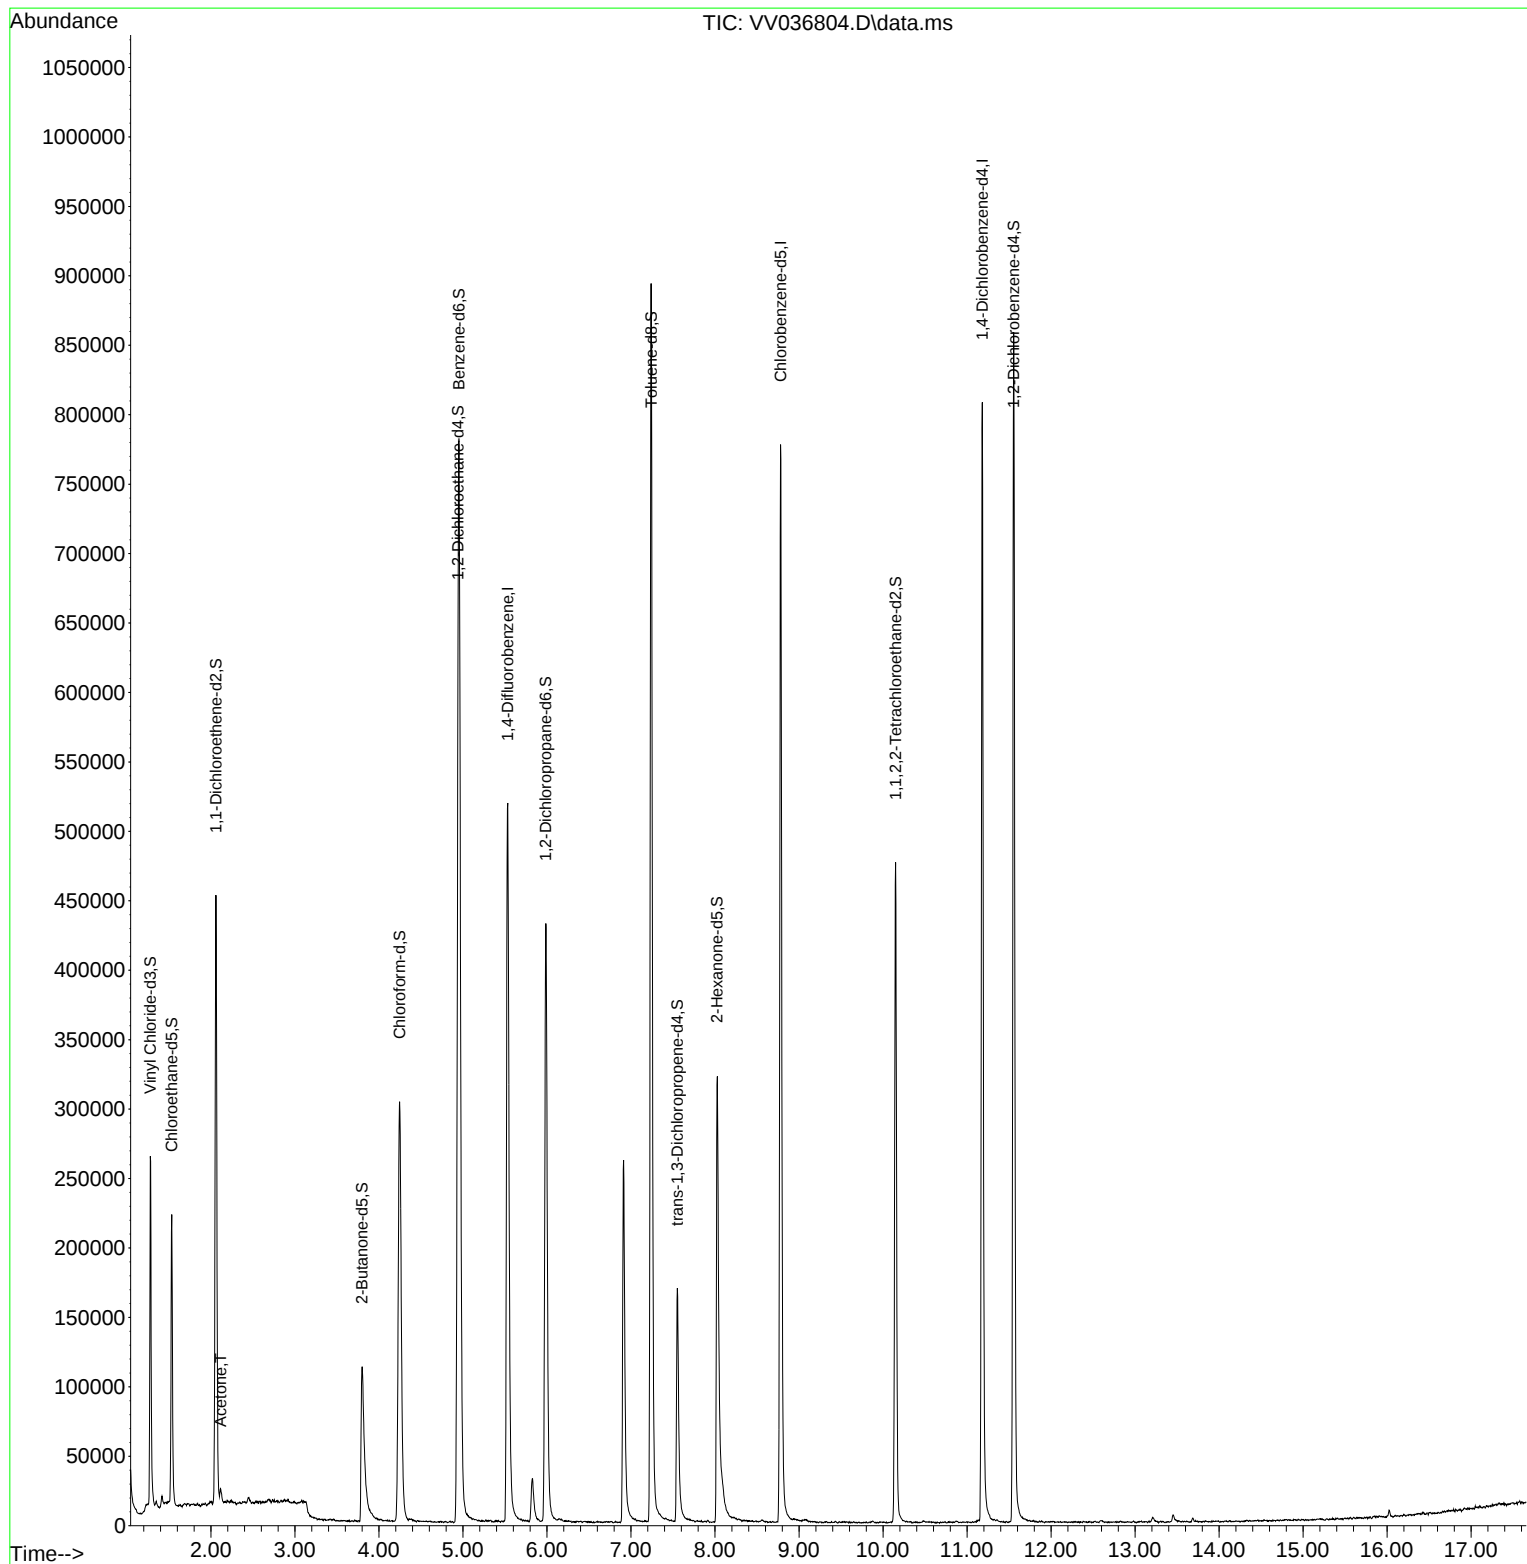

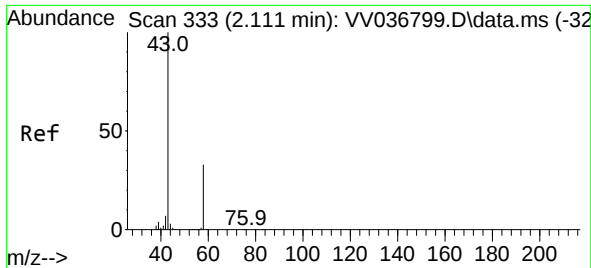

#13

Acetone

Concen: 6.024 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV036804.D


Acq: 06 Aug 2024 11:20

Instrument :

MSVOA_V

ClientSampleId :

E05T9

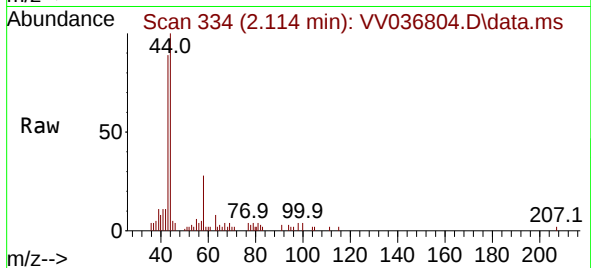

Tgt Ion: 43 Resp: 9578

Ion Ratio Lower Upper

43 100

58 30.4 0.0 63.4

