

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036805.D
 Acq On : 06 Aug 2024 11:42
 Operator : SY/MD
 Sample : P3437-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05W2

Quant Time: Aug 07 05:00:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 07 04:57:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	395380	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	368180	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	177447	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	175131	55.457	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	110.920%	
7) Chloroethane-d5	1.532	69	145610	58.469	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	116.940%	
11) 1,1-Dichloroethene-d2	2.060	65	75642	55.997	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	112.000%	
21) 2-Butanone-d5	3.799	46	185196	110.685	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	110.680%	
24) Chloroform-d	4.246	84	331620	58.517	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	117.040%	
26) 1,2-Dichloroethane-d4	4.940	65	222256	60.998	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	122.000%	
32) Benzene-d6	4.953	84	688102	61.878	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	123.760%	
36) 1,2-Dichloropropane-d6	5.985	67	222167	61.926	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	123.860%#	
41) Toluene-d8	7.239	98	613086	60.102	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	120.200%#	
43) trans-1,3-Dichloroprop...	7.551	79	108155	57.927	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	115.860%	
47) 2-Hexanone-d5	8.024	63	114188	110.697	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	110.700%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	242961	58.981	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	117.960%	
66) 1,2-Dichlorobenzene-d4	11.558	152	226789	62.720	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	125.440%#	
Target Compounds						
13) Acetone	2.114	43	9386	6.705	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036805.D
Acq On : 06 Aug 2024 11:42
Operator : SY/MD
Sample : P3437-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05W2

Quant Time: Aug 07 05:00:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 07 04:57:18 2024
Response via : Initial Calibration

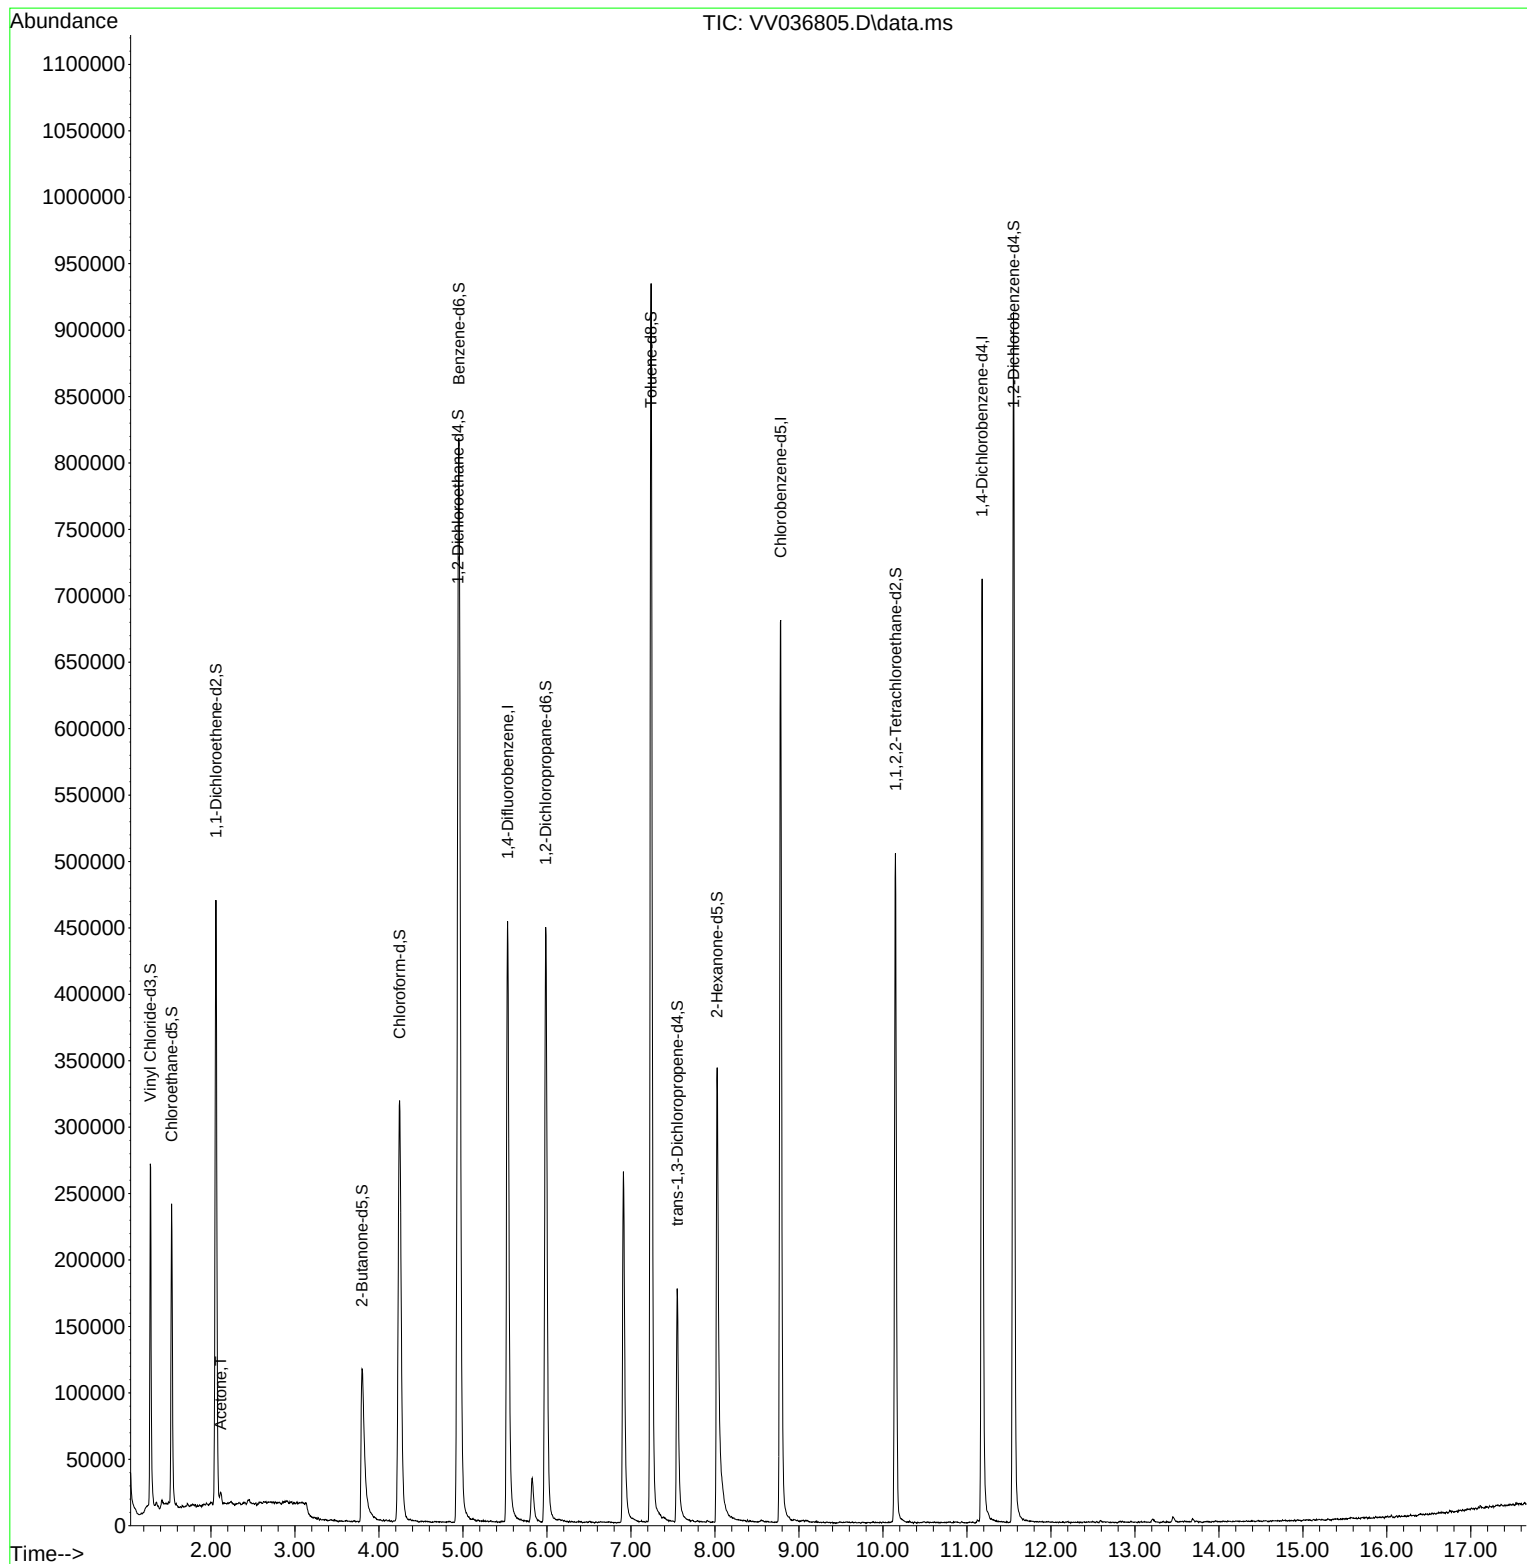

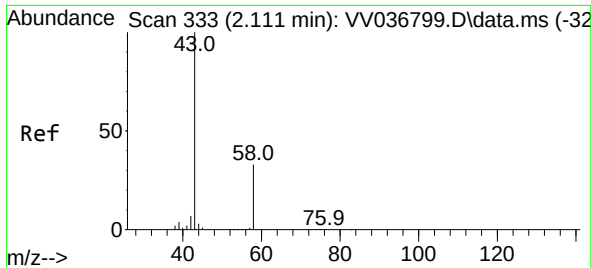

#13

Acetone

Concen: 6.705 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV036805.D

Acq: 06 Aug 2024 11:42

Instrument :

MSVOA_V

ClientSampleId :

E05W2

Tgt Ion: 43 Resp: 9386

Ion Ratio Lower Upper

43 100

58 30.1 0.0 63.4

