

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036806.D
 Acq On : 06 Aug 2024 12:05
 Operator : SY/MD
 Sample : P3437-05
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05W5

Quant Time: Aug 07 05:01:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 07 04:57:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	219122	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	203252	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.182	152	101310	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	117867	67.347	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 134.700%			
7) Chloroethane-d5	1.532	69	94963	68.805	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 137.600%#			
11) 1,1-Dichloroethene-d2	2.060	65	50900	67.991	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 135.980%#			
21) 2-Butanone-d5	3.799	46	128766	138.863	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 138.860%#			
24) Chloroform-d	4.246	84	219153	69.778	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 139.560%#			
26) 1,2-Dichloroethane-d4	4.941	65	148005	73.294	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 146.580%#			
32) Benzene-d6	4.953	84	452358	73.687	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 147.380%#			
36) 1,2-Dichloropropane-d6	5.986	67	147048	74.247	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 148.500%#			
41) Toluene-d8	7.240	98	402484	71.472	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 142.940%#			
43) trans-1,3-Dichloroprop...	7.555	79	69950	67.865	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 135.740%#			
47) 2-Hexanone-d5	8.027	63	72583	127.460	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 127.460%			
56) 1,1,2,2-Tetrachloroeth...	10.149	84	160542	70.598	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 141.200%#			
66) 1,2-Dichlorobenzene-d4	11.558	152	151062	73.174	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 146.340%#			
Target Compounds					Qvalue	
13) Acetone	2.114	43	7842	10.108	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036806.D
Acq On : 06 Aug 2024 12:05
Operator : SY/MD
Sample : P3437-05
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05W5

Quant Time: Aug 07 05:01:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 07 04:57:18 2024
Response via : Initial Calibration

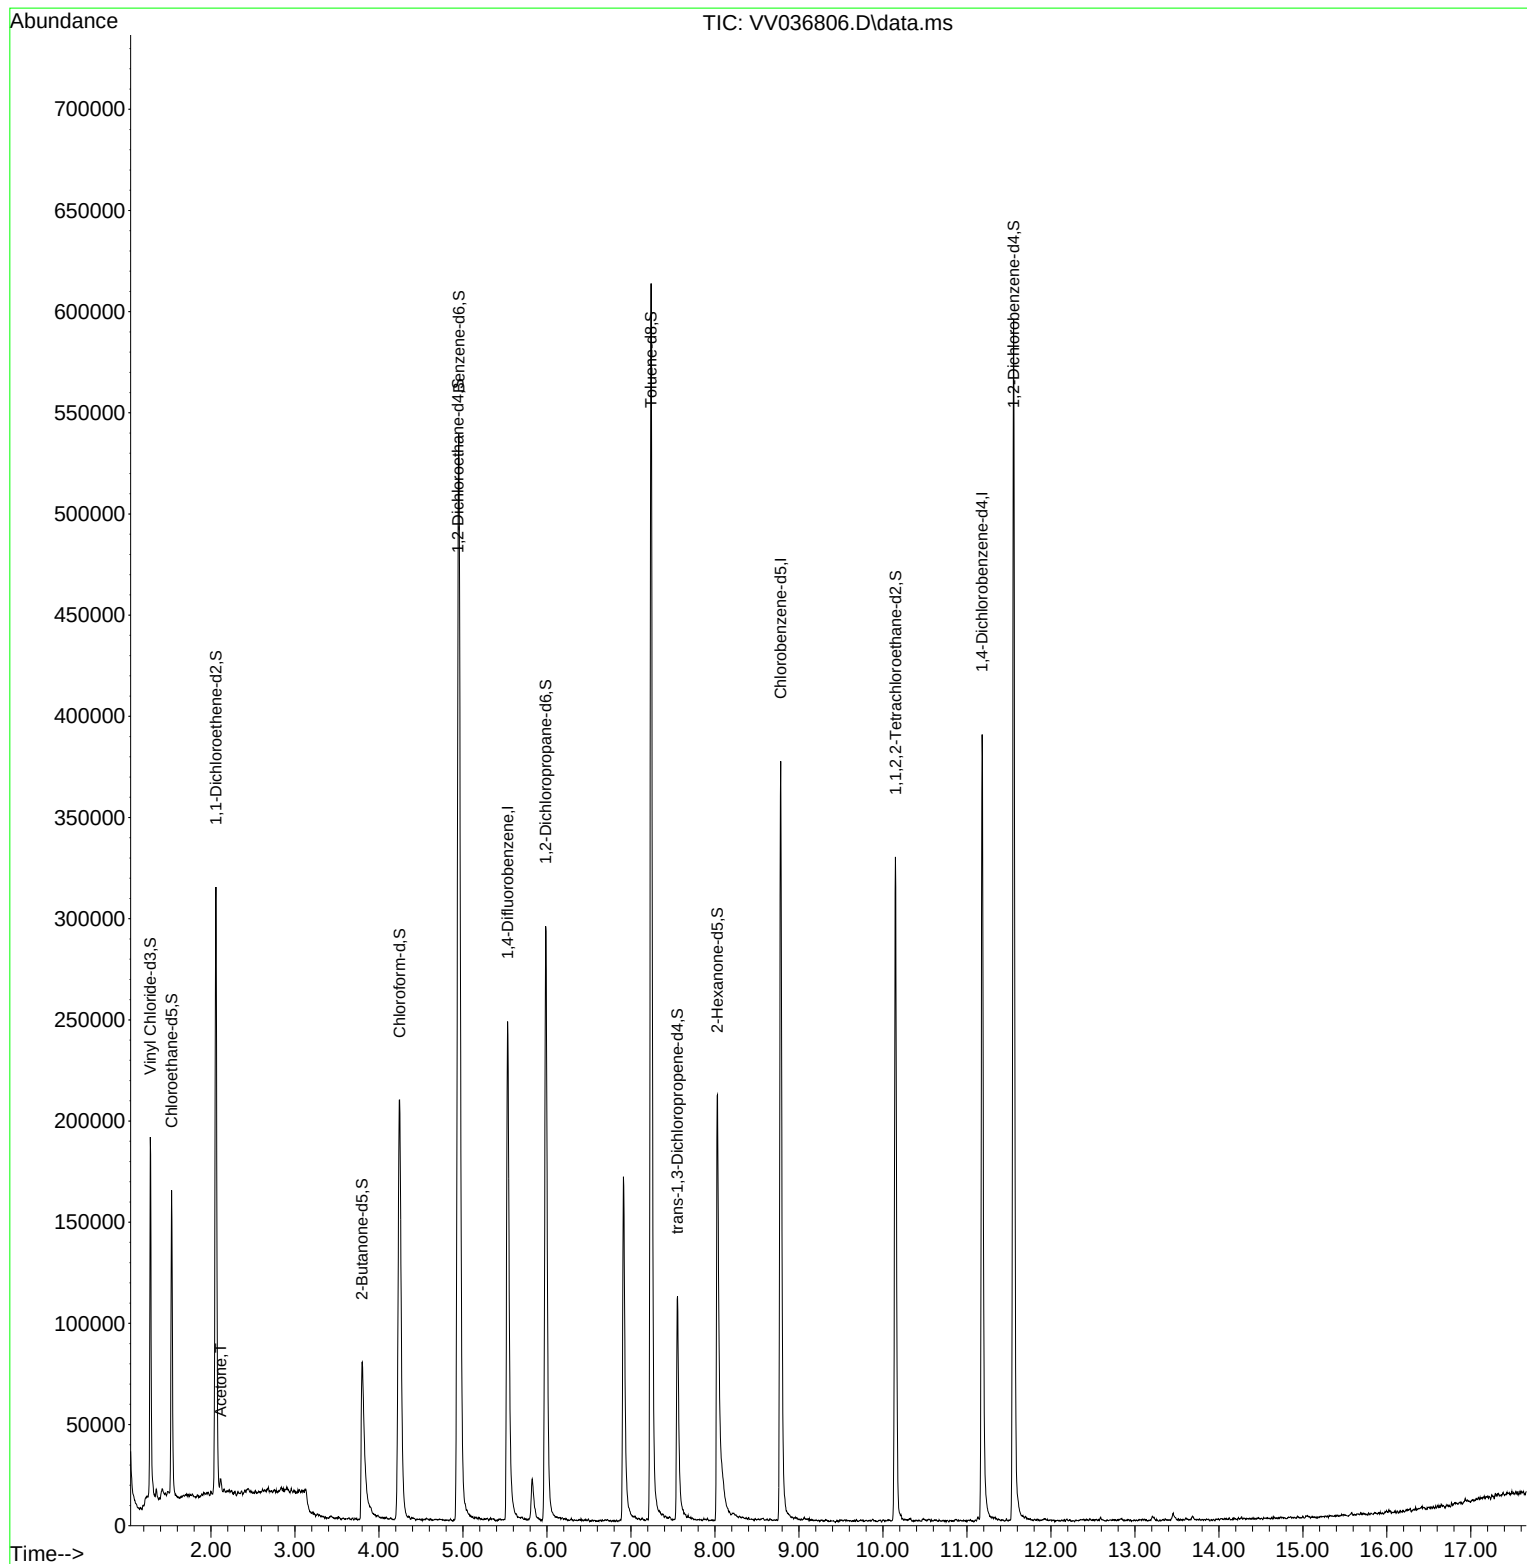

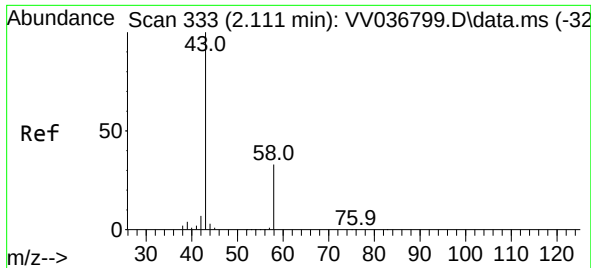

#13
 Acetone
 Concen: 10.108 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV036806.D
 Acq: 06 Aug 2024 12:05

Instrument :
 MSVOA_V
 ClientSampleId :
 E05W5

Tgt Ion: 43 Resp: 7842
 Ion Ratio Lower Upper
 43 100
 58 32.3 0.0 63.4

