

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036801.D
 Acq On : 06 Aug 2024 09:55
 Operator : SY/MD
 Sample : VV0806WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK360

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036801.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	260016	278138	13.82%	1.901%
2	1.532	146	153	170	rVB	225412	262703	13.05%	1.796%
3	2.060	307	317	332	rBV	445282	644797	32.03%	4.408%
4	3.574	786	788	793	rVB4	1096	686	0.03%	0.005%
5	3.616	799	801	803	rBV3	918	519	0.03%	0.004%
6	3.738	833	839	841	rBV5	681	736	0.04%	0.005%
7	3.799	849	858	889	rBV	117065	347328	17.25%	2.374%
8	4.246	980	997	1030	rBV	308356	787504	39.12%	5.384%
9	4.519	1079	1082	1085	rVB5	854	548	0.03%	0.004%
10	4.568	1092	1097	1102	rBV8	1096	1309	0.07%	0.009%
11	4.635	1115	1118	1120	rVB3	894	526	0.03%	0.004%
12	4.716	1140	1143	1146	rBV4	983	623	0.03%	0.004%
13	4.863	1187	1189	1195	rVB5	871	548	0.03%	0.004%
14	4.950	1200	1216	1252	rBV2	804941	2013118	100.00%	13.762%
15	5.217	1296	1299	1301	rBV4	812	581	0.03%	0.004%
16	5.529	1385	1396	1421	rBV	544201	1118988	55.58%	7.650%
17	5.825	1477	1488	1512	rBV2	27808	65310	3.24%	0.446%
18	5.986	1524	1538	1565	rBV	449132	924098	45.90%	6.317%
19	6.217	1608	1610	1616	rVB6	1295	881	0.04%	0.006%
20	6.246	1616	1619	1623	rVB7	976	834	0.04%	0.006%
21	6.275	1623	1628	1630	rVB3	803	549	0.03%	0.004%
22	6.291	1630	1633	1635	rBV3	649	478	0.02%	0.003%
23	6.564	1716	1718	1722	rVB5	771	644	0.03%	0.004%
24	6.629	1735	1738	1743	rBV7	713	584	0.03%	0.004%
25	6.735	1769	1771	1775	rVV4	943	703	0.03%	0.005%
26	6.767	1778	1781	1787	rVB5	1072	938	0.05%	0.006%
27	6.796	1787	1790	1793	rBV3	656	492	0.02%	0.003%
28	6.850	1805	1807	1813	rBV6	649	527	0.03%	0.004%
29	6.912	1813	1826	1865	rBV	264926	507178	25.19%	3.467%
30	7.240	1917	1928	1950	rBV	931144	1607324	79.84%	10.988%
31	7.513	2011	2013	2015	rVB3	1104	481	0.02%	0.003%
32	7.551	2015	2025	2051	rBV	175708	320033	15.90%	2.188%
33	7.751	2085	2087	2092	rBV6	689	570	0.03%	0.004%
34	7.957	2146	2151	2156	rBV6	856	827	0.04%	0.006%
35	8.027	2164	2173	2209	rBV2	327785	692721	34.41%	4.736%
36	8.490	2313	2317	2320	rVB3	1012	810	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036801.D
 Acq On : 06 Aug 2024 09:55
 Operator : SY/MD
 Sample : VV0806WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK360

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	8.535	2327	2331	2332	rBV4	952	463	0.02%	0.003%
38	8.551	2334	2336	2345	rVV9	982	1186	0.06%	0.008%
39	8.654	2365	2368	2371	rVB4	808	527	0.03%	0.004%
40	8.780	2397	2407	2440	rBV	819168	1365594	67.83%	9.336%
41	9.182	2530	2532	2536	rBV5	730	512	0.03%	0.004%
42	9.365	2587	2589	2592	rBV3	731	472	0.02%	0.003%
43	9.403	2597	2601	2605	rVB6	880	763	0.04%	0.005%
44	9.493	2624	2629	2630	rBV5	678	518	0.03%	0.004%
45	9.590	2656	2659	2663	rVB6	881	699	0.03%	0.005%
46	9.767	2709	2714	2717	rBV6	559	613	0.03%	0.004%
47	9.805	2725	2726	2732	rVB4	846	460	0.02%	0.003%
48	9.838	2732	2736	2739	rBV3	545	543	0.03%	0.004%
49	9.863	2739	2744	2745	rBV3	1128	925	0.05%	0.006%
50	9.947	2767	2770	2772	rBV3	716	519	0.03%	0.004%
51	10.149	2820	2833	2853	rBV	496658	793348	39.41%	5.424%
52	10.291	2875	2877	2880	rVB2	987	586	0.03%	0.004%
53	10.307	2880	2882	2886	rBV5	627	596	0.03%	0.004%
54	10.416	2913	2916	2920	rVB6	759	444	0.02%	0.003%
55	10.628	2980	2982	2985	rVB2	1002	547	0.03%	0.004%
56	10.728	3009	3013	3015	rBV4	805	600	0.03%	0.004%
57	10.841	3043	3048	3050	rBV4	804	656	0.03%	0.004%
58	10.866	3054	3056	3059	rVV3	950	610	0.03%	0.004%
59	10.882	3059	3061	3067	rVB6	880	758	0.04%	0.005%
60	10.937	3074	3078	3083	rBV5	869	732	0.04%	0.005%
61	11.098	3122	3128	3131	rBV6	1005	1081	0.05%	0.007%
62	11.130	3131	3138	3143	rBV10	2415	3272	0.16%	0.022%
63	11.182	3143	3154	3187	rBV	851578	1363858	67.75%	9.324%
64	11.554	3258	3270	3299	rBV	895627	1448529	71.95%	9.902%
65	11.786	3339	3342	3346	rVB6	1290	811	0.04%	0.006%
66	11.834	3354	3357	3361	rBV5	1042	957	0.05%	0.007%
67	11.902	3375	3378	3381	rVB4	760	462	0.02%	0.003%
68	12.062	3425	3428	3431	rVB6	878	665	0.03%	0.005%
69	12.088	3431	3436	3440	rBV3	730	638	0.03%	0.004%
70	12.114	3442	3444	3449	rVB5	963	767	0.04%	0.005%
71	12.143	3449	3453	3454	rBV3	851	607	0.03%	0.004%
72	12.188	3461	3467	3470	rBV7	957	972	0.05%	0.007%
73	12.233	3478	3481	3484	rBV4	812	525	0.03%	0.004%
74	12.262	3488	3490	3494	rBV4	902	704	0.03%	0.005%
75	12.307	3500	3504	3505	rBV3	734	553	0.03%	0.004%
76	12.333	3510	3512	3518	rVB6	850	804	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036801.D
 Acq On : 06 Aug 2024 09:55
 Operator : SY/MD
 Sample : VV0806WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK360

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	12.439	3539	3545	3548	rBV4	1067	988	0.05%	0.007%
78	12.455	3548	3550	3554	rVV3	791	538	0.03%	0.004%
79	12.506	3562	3566	3571	rBV5	703	702	0.03%	0.005%
80	12.529	3571	3573	3578	rBV5	616	526	0.03%	0.004%
81	12.590	3586	3592	3600	rBV6	3004	4034	0.20%	0.028%
82	12.686	3620	3622	3627	rVB4	665	451	0.02%	0.003%
83	12.799	3654	3657	3659	rBV2	593	455	0.02%	0.003%
84	12.898	3685	3688	3689	rBV4	877	495	0.02%	0.003%
85	13.053	3732	3736	3737	rBV2	973	778	0.04%	0.005%
86	13.165	3767	3771	3773	rBV3	848	589	0.03%	0.004%
87	13.207	3777	3784	3791	rBV5	3738	5288	0.26%	0.036%
88	13.297	3809	3812	3816	rVV3	865	513	0.03%	0.004%
89	13.371	3832	3835	3837	rVV3	947	478	0.02%	0.003%
90	13.406	3841	3846	3848	rBV5	861	782	0.04%	0.005%
91	13.448	3852	3859	3875	rBV3	7426	16570	0.82%	0.113%
92	13.612	3905	3910	3914	rBV2	1166	1170	0.06%	0.008%
93	13.686	3925	3933	3945	rBV2	3532	6164	0.31%	0.042%
94	13.744	3945	3951	3954	rBV6	1005	861	0.04%	0.006%
95	13.995	4026	4029	4030	rBV2	763	467	0.02%	0.003%
96	14.255	4105	4110	4114	rBV4	990	822	0.04%	0.006%
97	14.320	4126	4130	4134	rBV5	932	965	0.05%	0.007%
98	14.358	4139	4142	4145	rVB4	952	675	0.03%	0.005%
99	14.477	4176	4179	4181	rBV3	666	443	0.02%	0.003%
100	14.545	4197	4200	4203	rVB5	1009	683	0.03%	0.005%




Sum of corrected areas: 14627947

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036801.D
Acq On : 06 Aug 2024 09:55
Operator : SY/MD
Sample : VV0806WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK360

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

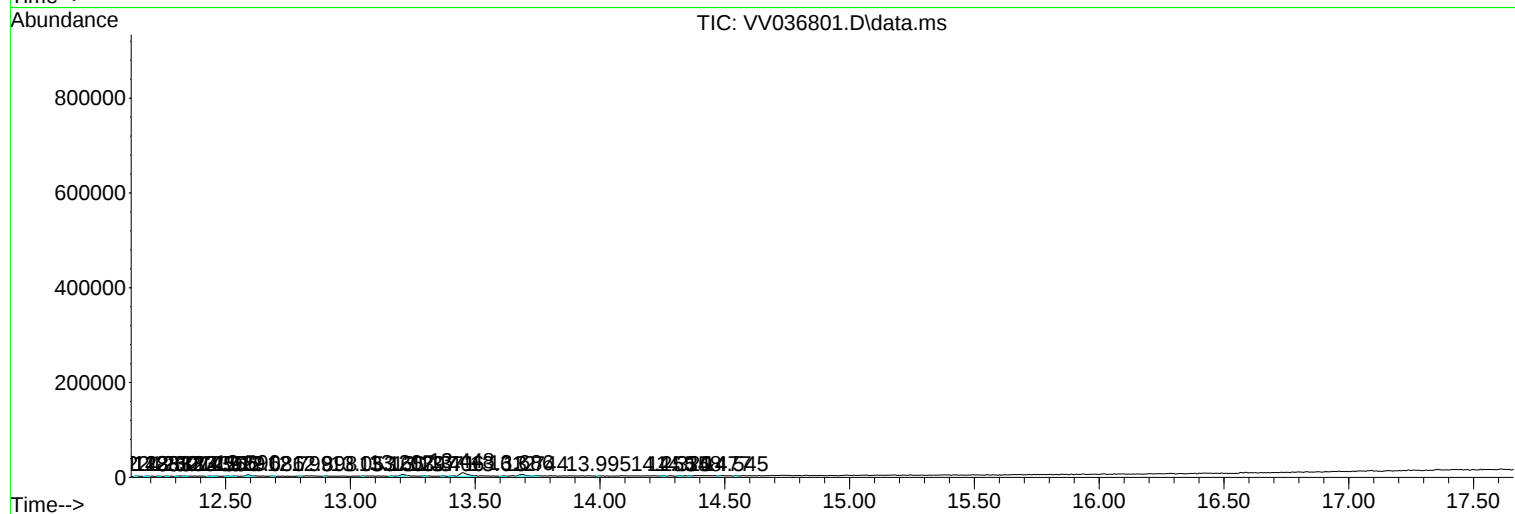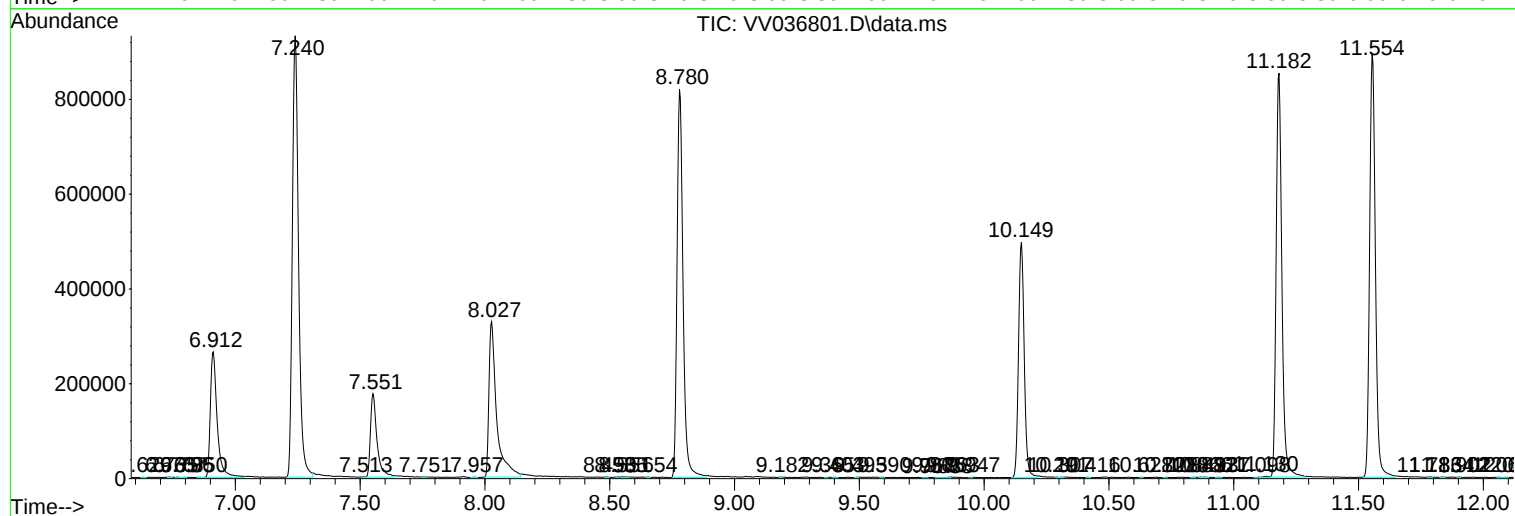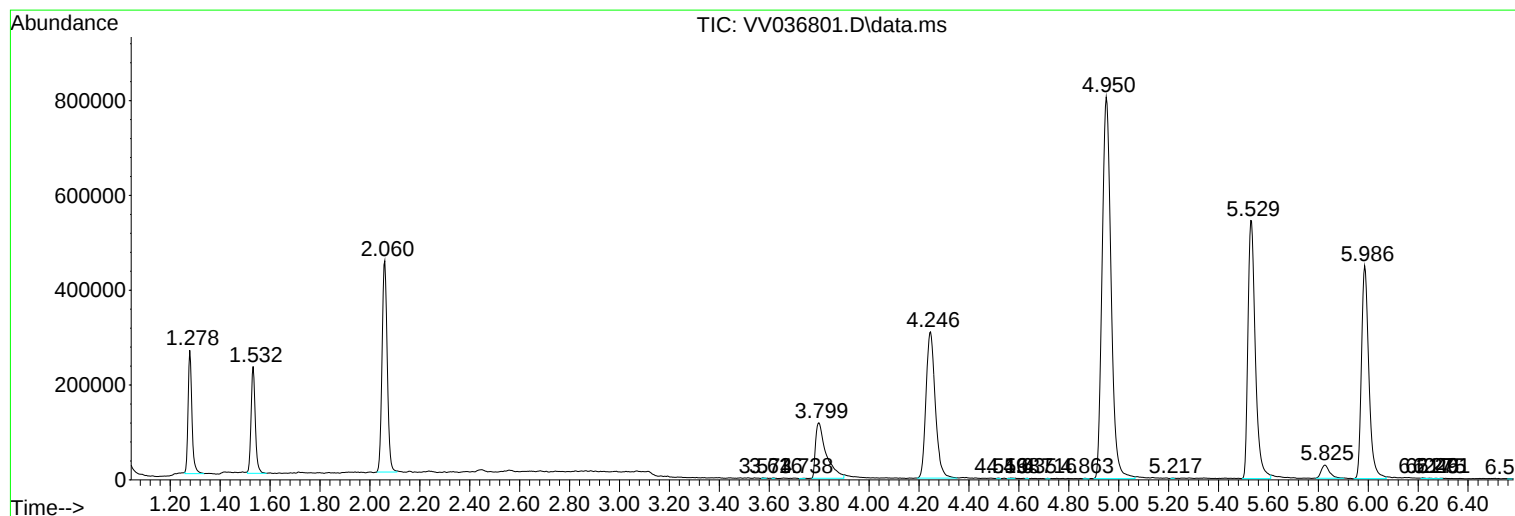

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036801.D
Acq On : 06 Aug 2024 09:55
Operator : SY/MD
Sample : VV0806WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK360

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036801.D
Acq On : 06 Aug 2024 09:55
Operator : SY/MD
Sample : VV0806WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK360

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------