

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036805.D
 Acq On : 06 Aug 2024 11:42
 Operator : SY/MD
 Sample : P3437-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05W2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036805.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	257194	279392	13.73%	1.977%
2	1.532	146	153	168	rVB	226648	266610	13.10%	1.886%
3	2.060	307	317	330	rBV	454154	652609	32.06%	4.618%
4	3.275	692	695	700	rVB5	2155	1907	0.09%	0.013%
5	3.468	752	755	757	rBV3	1060	637	0.03%	0.005%
6	3.526	771	773	775	rBV2	814	443	0.02%	0.003%
7	3.696	823	826	828	rBV2	773	501	0.02%	0.004%
8	3.799	849	858	901	rBV3	115162	349192	17.15%	2.471%
9	4.053	935	937	940	rVB2	1241	676	0.03%	0.005%
10	4.175	970	975	976	rBV5	829	683	0.03%	0.005%
11	4.246	981	997	1021	rVV	316266	805455	39.57%	5.699%
12	4.503	1072	1077	1079	rBV4	836	728	0.04%	0.005%
13	4.558	1092	1094	1100	rVB5	661	507	0.02%	0.004%
14	4.635	1116	1118	1123	rBV5	694	585	0.03%	0.004%
15	4.950	1200	1216	1249	rBV2	816207	2035552	100.00%	14.403%
16	5.330	1332	1334	1339	rVB5	934	720	0.04%	0.005%
17	5.400	1355	1356	1359	rVB3	1085	529	0.03%	0.004%
18	5.455	1369	1373	1375	rBV4	1243	934	0.05%	0.007%
19	5.532	1386	1397	1426	rBV	451439	931008	45.74%	6.588%
20	5.825	1476	1488	1509	rBV4	33201	76750	3.77%	0.543%
21	5.985	1525	1538	1570	rBV	447811	932245	45.80%	6.596%
22	6.410	1668	1670	1674	rVB4	1106	661	0.03%	0.005%
23	6.580	1718	1723	1724	rBV3	962	629	0.03%	0.004%
24	6.911	1811	1826	1856	rBV	264311	505827	24.85%	3.579%
25	7.182	1908	1910	1913	rBV4	759	436	0.02%	0.003%
26	7.239	1917	1928	1962	rBV	932093	1637908	80.47%	11.589%
27	7.551	2015	2025	2051	rBV	175904	325035	15.97%	2.300%
28	7.908	2132	2136	2140	rBV4	1393	1455	0.07%	0.010%
29	8.027	2164	2173	2216	rBV2	342194	733104	36.01%	5.187%
30	8.387	2283	2285	2291	rVB5	1552	1102	0.05%	0.008%
31	8.416	2291	2294	2296	rBV3	1090	715	0.04%	0.005%
32	8.551	2332	2336	2339	rBV7	1099	926	0.05%	0.007%
33	8.783	2394	2408	2437	rBV	679155	1142806	56.14%	8.086%
34	9.230	2544	2547	2551	rVB5	754	520	0.03%	0.004%
35	9.390	2593	2597	2599	rBV2	577	454	0.02%	0.003%
36	9.423	2602	2607	2609	rBV4	719	593	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036805.D
 Acq On : 06 Aug 2024 11:42
 Operator : SY/MD
 Sample : P3437-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05W2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	9.490	2621	2628	2632	rBV5	953	1170	0.06%	0.008%
38	9.561	2648	2650	2652	rVV2	822	538	0.03%	0.004%
39	9.587	2656	2658	2660	rVV2	681	415	0.02%	0.003%
40	9.603	2660	2663	2666	rVV4	802	457	0.02%	0.003%
41	9.635	2670	2673	2677	rVV6	853	610	0.03%	0.004%
42	9.673	2682	2685	2688	rVB4	570	418	0.02%	0.003%
43	9.715	2695	2698	2703	rVB5	803	765	0.04%	0.005%
44	9.747	2703	2708	2709	rBV3	737	501	0.02%	0.004%
45	9.828	2727	2733	2736	rBV4	777	1003	0.05%	0.007%
46	9.860	2740	2743	2746	rBV4	667	520	0.03%	0.004%
47	9.879	2746	2749	2750	rBV2	772	427	0.02%	0.003%
48	9.969	2775	2777	2782	rVB5	728	500	0.02%	0.004%
49	10.001	2782	2787	2791	rBV5	780	978	0.05%	0.007%
50	10.149	2822	2833	2854	rBV	503033	790013	38.81%	5.590%
51	10.320	2884	2886	2892	rVB6	1126	759	0.04%	0.005%
52	10.349	2892	2895	2899	rVB4	1065	885	0.04%	0.006%
53	10.374	2899	2903	2911	rBV5	1152	1565	0.08%	0.011%
54	10.416	2913	2916	2917	rBV2	961	618	0.03%	0.004%
55	10.480	2931	2936	2938	rBV5	750	710	0.03%	0.005%
56	10.493	2938	2940	2946	rVB4	945	779	0.04%	0.006%
57	10.522	2946	2949	2951	rBV3	590	435	0.02%	0.003%
58	10.657	2987	2991	2994	rVB5	845	616	0.03%	0.004%
59	10.693	2999	3002	3006	rBV4	742	504	0.02%	0.004%
60	10.940	3072	3079	3082	rBV6	1079	1103	0.05%	0.008%
61	11.069	3115	3119	3126	rVB5	862	1014	0.05%	0.007%
62	11.111	3129	3132	3133	rBV2	861	543	0.03%	0.004%
63	11.127	3133	3137	3141	rBV5	1741	1842	0.09%	0.013%
64	11.181	3143	3154	3184	rVV	709480	1128720	55.45%	7.987%
65	11.474	3243	3245	3249	rBV4	1043	698	0.03%	0.005%
66	11.554	3257	3270	3304	rBV	911123	1467494	72.09%	10.384%
67	11.866	3363	3367	3370	rBV3	600	514	0.03%	0.004%
68	11.914	3380	3382	3385	rBV3	637	423	0.02%	0.003%
69	11.976	3397	3401	3405	rVB4	617	478	0.02%	0.003%
70	12.078	3430	3433	3437	rVB6	589	474	0.02%	0.003%
71	12.178	3460	3464	3466	rBV4	809	734	0.04%	0.005%
72	12.226	3476	3479	3482	rVB4	828	622	0.03%	0.004%
73	12.249	3482	3486	3489	rBV5	789	673	0.03%	0.005%
74	12.320	3506	3508	3513	rVB2	816	701	0.03%	0.005%
75	12.355	3517	3519	3524	rVB3	866	682	0.03%	0.005%
76	12.548	3575	3579	3583	rVB5	1031	817	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036805.D
 Acq On : 06 Aug 2024 11:42
 Operator : SY/MD
 Sample : P3437-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05W2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	12.593	3587	3593	3597	rBV6	1660	2090	0.10%	0.015%
78	12.808	3658	3660	3663	rVV3	1037	807	0.04%	0.006%
79	12.828	3663	3666	3669	rVV3	1311	997	0.05%	0.007%
80	12.850	3669	3673	3676	rVV6	1141	1054	0.05%	0.007%
81	12.953	3701	3705	3707	rVV5	811	508	0.02%	0.004%
82	13.040	3728	3732	3735	rBV5	920	766	0.04%	0.005%
83	13.213	3779	3786	3796	rBV5	2336	4252	0.21%	0.030%
84	13.336	3820	3824	3830	rVV5	994	990	0.05%	0.007%
85	13.381	3835	3838	3841	rBV2	1005	578	0.03%	0.004%
86	13.451	3852	3860	3872	rBV5	4129	7597	0.37%	0.054%
87	13.538	3884	3887	3890	rBV4	660	488	0.02%	0.003%
88	13.593	3900	3904	3907	rBV5	972	840	0.04%	0.006%
89	13.686	3927	3933	3935	rBV5	2648	2492	0.12%	0.018%
90	13.773	3956	3960	3964	rBV7	1050	1097	0.05%	0.008%
91	13.818	3970	3974	3975	rBV3	660	427	0.02%	0.003%
92	13.918	4002	4005	4006	rBV3	837	484	0.02%	0.003%
93	13.943	4011	4013	4016	rVV4	768	560	0.03%	0.004%
94	13.963	4016	4019	4025	rVB5	987	1024	0.05%	0.007%
95	14.049	4042	4046	4048	rBV3	727	618	0.03%	0.004%
96	14.107	4061	4064	4067	rBV5	776	603	0.03%	0.004%
97	14.168	4080	4083	4087	rBV4	587	426	0.02%	0.003%
98	14.448	4164	4170	4171	rBV4	670	546	0.03%	0.004%
99	14.757	4264	4266	4269	rBV4	891	446	0.02%	0.003%
100	14.901	4309	4311	4314	rVB4	945	479	0.02%	0.003%




Sum of corrected areas: 14132721

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036805.D
Acq On : 06 Aug 2024 11:42
Operator : SY/MD
Sample : P3437-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05W2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

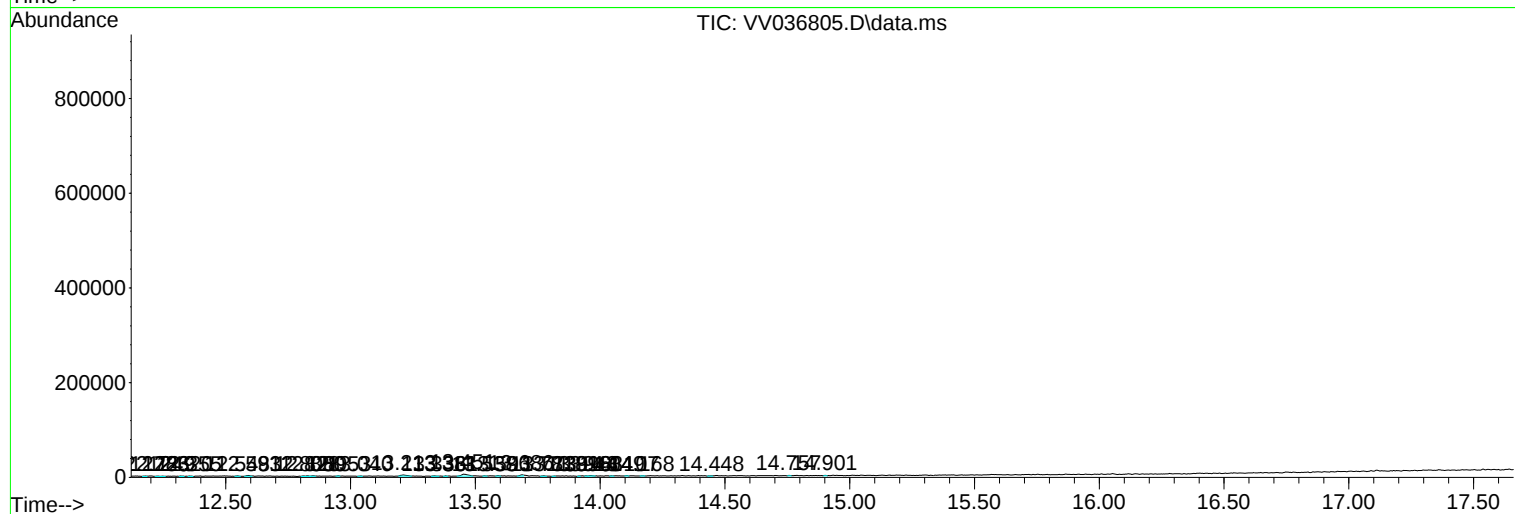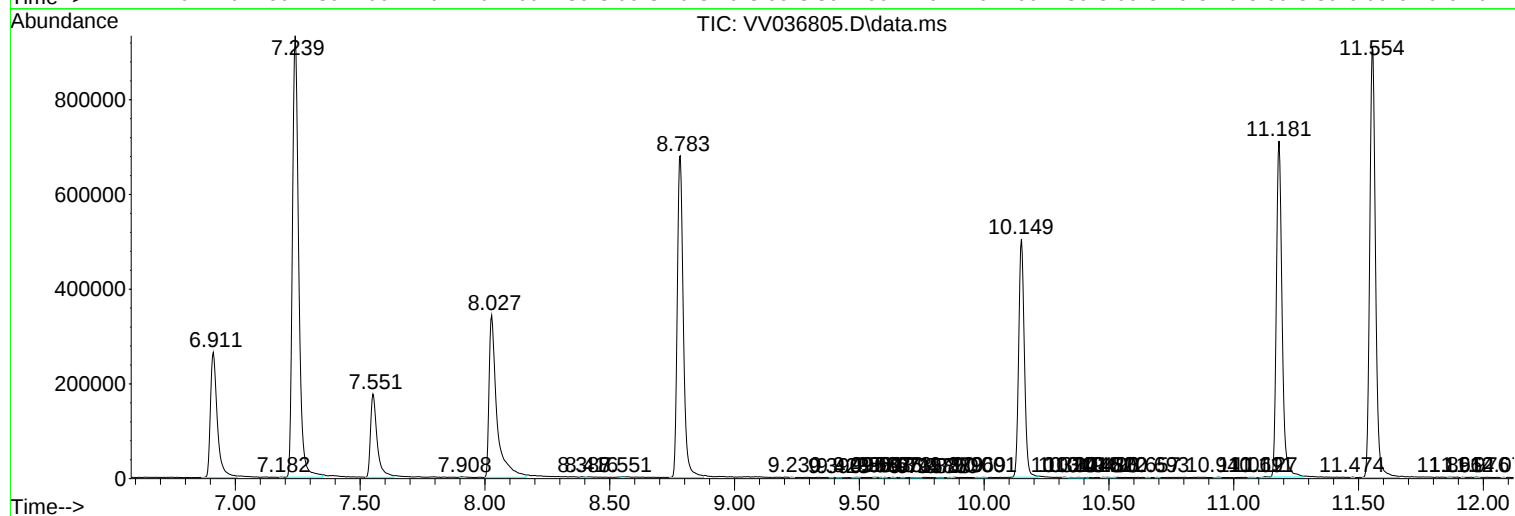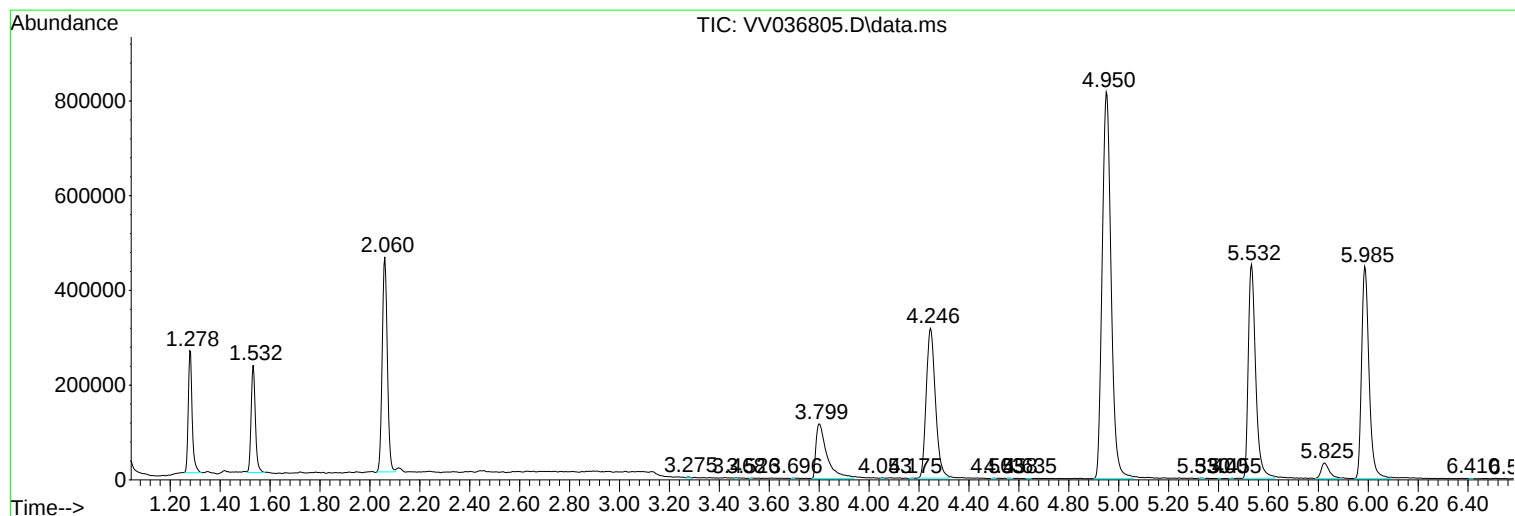

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036805.D
Acq On : 06 Aug 2024 11:42
Operator : SY/MD
Sample : P3437-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05W2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036805.D
Acq On : 06 Aug 2024 11:42
Operator : SY/MD
Sample : P3437-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05W2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc