

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036806.D
 Acq On : 06 Aug 2024 12:05
 Operator : SY/MD
 Sample : P3437-05
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05W5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036806.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	177684	191343	14.25%	2.123%
2	1.532	146	153	167	rVB	150755	176557	13.15%	1.959%
3	2.060	308	317	330	rVB	296558	420870	31.34%	4.669%
4	3.516	766	770	771	rBV4	938	649	0.05%	0.007%
5	3.757	842	845	848	rBV4	480	396	0.03%	0.004%
6	3.802	850	859	899	rVV	77753	227275	16.93%	2.521%
7	4.246	980	997	1027	rBV	207123	536513	39.95%	5.952%
8	4.391	1039	1042	1046	rBV4	969	888	0.07%	0.010%
9	4.513	1077	1080	1082	rVB5	855	497	0.04%	0.006%
10	4.613	1107	1111	1114	rBV4	807	607	0.05%	0.007%
11	4.950	1201	1216	1244	rBV2	536493	1342813	100.00%	14.896%
12	5.140	1273	1275	1277	rBV2	949	485	0.04%	0.005%
13	5.330	1329	1334	1337	rBV7	1140	841	0.06%	0.009%
14	5.420	1359	1362	1363	rBV3	746	449	0.03%	0.005%
15	5.532	1387	1397	1434	rBV	246195	526344	39.20%	5.839%
16	5.773	1469	1472	1474	rBV2	704	475	0.04%	0.005%
17	5.825	1476	1488	1507	rVV2	20203	46155	3.44%	0.512%
18	5.986	1524	1538	1568	rBV	293782	616167	45.89%	6.835%
19	6.207	1604	1607	1612	rBV7	608	516	0.04%	0.006%
20	6.326	1640	1644	1646	rBV3	720	594	0.04%	0.007%
21	6.384	1660	1662	1667	rVB5	550	445	0.03%	0.005%
22	6.407	1667	1669	1672	rVB3	1197	527	0.04%	0.006%
23	6.455	1679	1684	1686	rBV4	791	544	0.04%	0.006%
24	6.494	1694	1696	1701	rVB4	1350	937	0.07%	0.010%
25	6.571	1715	1720	1724	rVB4	591	640	0.05%	0.007%
26	6.658	1744	1747	1750	rBV3	818	500	0.04%	0.006%
27	6.873	1810	1814	1816	rBV4	796	558	0.04%	0.006%
28	6.912	1816	1826	1860	rBV	169795	330773	24.63%	3.669%
29	7.240	1917	1928	1956	rBV	611139	1071016	79.76%	11.881%
30	7.555	2017	2026	2050	rBV2	110120	206644	15.39%	2.292%
31	7.680	2063	2065	2069	rVB4	1146	444	0.03%	0.005%
32	7.870	2118	2124	2125	rBV6	1091	755	0.06%	0.008%
33	8.031	2164	2174	2217	rBV2	210531	485031	36.12%	5.381%
34	8.400	2287	2289	2293	rVB3	1047	681	0.05%	0.008%
35	8.654	2365	2368	2373	rBV5	768	638	0.05%	0.007%
36	8.783	2397	2408	2434	rBV	375226	635409	47.32%	7.049%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036806.D
 Acq On : 06 Aug 2024 12:05
 Operator : SY/MD
 Sample : P3437-05
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05W5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	9.030	2482	2485	2489	rBV3	695	429	0.03%	0.005%
38	9.063	2492	2495	2501	rVB6	1147	829	0.06%	0.009%
39	9.108	2507	2509	2512	rVB3	781	484	0.04%	0.005%
40	9.143	2516	2520	2523	rBV4	633	554	0.04%	0.006%
41	9.204	2537	2539	2544	rVB6	587	422	0.03%	0.005%
42	9.236	2547	2549	2552	rVB3	701	417	0.03%	0.005%
43	9.487	2624	2627	2631	rBV5	984	829	0.06%	0.009%
44	9.542	2641	2644	2647	rBV4	570	506	0.04%	0.006%
45	9.612	2663	2666	2670	rVB6	568	420	0.03%	0.005%
46	9.686	2684	2689	2692	rBV4	1041	859	0.06%	0.010%
47	9.764	2712	2713	2716	rVB2	879	424	0.03%	0.005%
48	9.834	2731	2735	2737	rBV4	535	385	0.03%	0.004%
49	9.879	2742	2749	2753	rVV5	1103	1270	0.09%	0.014%
50	9.950	2766	2771	2773	rBV4	627	528	0.04%	0.006%
51	9.998	2782	2786	2787	rBV2	871	596	0.04%	0.007%
52	10.149	2821	2833	2852	rBV	328021	524299	39.04%	5.816%
53	10.262	2864	2868	2871	rBV4	603	515	0.04%	0.006%
54	10.471	2930	2933	2935	rBV3	1071	731	0.05%	0.008%
55	10.580	2964	2967	2972	rBV6	988	754	0.06%	0.008%
56	10.747	3017	3019	3021	rVB3	773	393	0.03%	0.004%
57	10.767	3021	3025	3031	rVB5	797	921	0.07%	0.010%
58	10.796	3031	3034	3038	rBV3	839	764	0.06%	0.008%
59	10.989	3092	3094	3097	rVB3	801	394	0.03%	0.004%
60	11.021	3097	3104	3107	rBV7	943	1519	0.11%	0.017%
61	11.101	3124	3129	3133	rBV5	871	988	0.07%	0.011%
62	11.130	3133	3138	3144	rBV7	2024	2594	0.19%	0.029%
63	11.182	3144	3154	3184	rVV	387978	638447	47.55%	7.082%
64	11.378	3211	3215	3219	rBV6	635	502	0.04%	0.006%
65	11.416	3224	3227	3228	rBV2	719	395	0.03%	0.004%
66	11.471	3239	3244	3250	rVB5	1253	983	0.07%	0.011%
67	11.558	3257	3271	3300	rBV	593623	971784	72.37%	10.780%
68	11.809	3344	3349	3351	rBV4	730	696	0.05%	0.008%
69	11.837	3357	3358	3363	rBV2	610	465	0.03%	0.005%
70	12.037	3418	3420	3423	rVB2	949	579	0.04%	0.006%
71	12.159	3454	3458	3462	rVB2	1136	825	0.06%	0.009%
72	12.191	3462	3468	3473	rBV7	1309	1632	0.12%	0.018%
73	12.265	3487	3491	3496	rVB6	617	771	0.06%	0.009%
74	12.294	3496	3500	3501	rBV3	893	634	0.05%	0.007%
75	12.426	3538	3541	3543	rBV3	801	501	0.04%	0.006%
76	12.529	3571	3573	3576	rBV3	633	451	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036806.D
 Acq On : 06 Aug 2024 12:05
 Operator : SY/MD
 Sample : P3437-05
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E05W5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	12.593	3588	3593	3597	rVV4	1515	1461	0.11%	0.016%
78	12.763	3644	3646	3652	rVB5	644	393	0.03%	0.004%
79	12.792	3652	3655	3658	rBV4	625	531	0.04%	0.006%
80	12.950	3699	3704	3706	rVB4	829	697	0.05%	0.008%
81	13.056	3734	3737	3742	rVV3	712	680	0.05%	0.008%
82	13.091	3745	3748	3751	rBV3	846	602	0.04%	0.007%
83	13.111	3751	3754	3758	rVB4	811	667	0.05%	0.007%
84	13.210	3779	3785	3788	rBV6	2032	2410	0.18%	0.027%
85	13.300	3809	3813	3815	rBV4	694	512	0.04%	0.006%
86	13.362	3829	3832	3837	rBV4	929	779	0.06%	0.009%
87	13.458	3852	3862	3874	rBV8	3688	7284	0.54%	0.081%
88	13.577	3896	3899	3902	rBV4	559	392	0.03%	0.004%
89	13.606	3905	3908	3910	rBV4	762	431	0.03%	0.005%
90	13.686	3928	3933	3942	rVB6	1886	2782	0.21%	0.031%
91	13.770	3957	3959	3964	rVB4	833	638	0.05%	0.007%
92	13.825	3973	3976	3981	rBV5	698	679	0.05%	0.008%
93	13.857	3981	3986	3991	rBV5	689	915	0.07%	0.010%
94	13.937	4008	4011	4016	rVB7	832	757	0.06%	0.008%
95	13.960	4016	4018	4020	rBV2	946	579	0.04%	0.006%
96	14.120	4066	4068	4073	rVB5	1048	751	0.06%	0.008%
97	14.178	4083	4086	4090	rBV4	1180	922	0.07%	0.010%
98	14.233	4100	4103	4105	rBV3	1091	717	0.05%	0.008%
99	14.271	4112	4115	4118	rVB5	1214	796	0.06%	0.009%
100	14.660	4234	4236	4241	rVB5	786	625	0.05%	0.007%




Sum of corrected areas: 9014465

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036806.D
Acq On : 06 Aug 2024 12:05
Operator : SY/MD
Sample : P3437-05
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05W5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

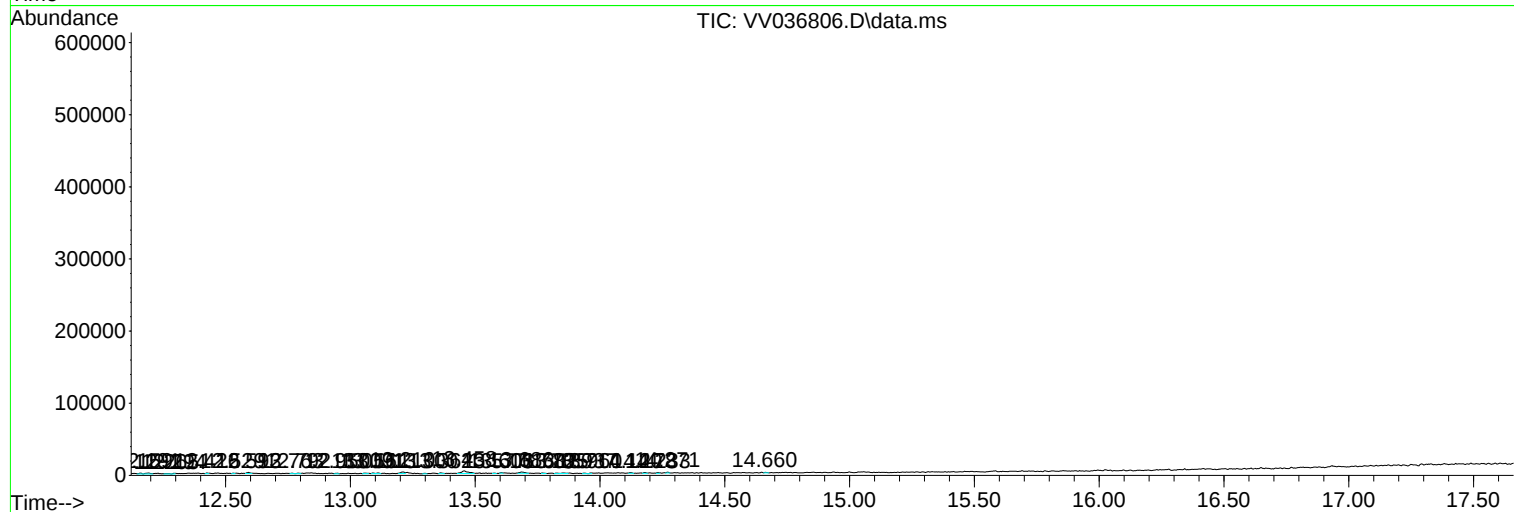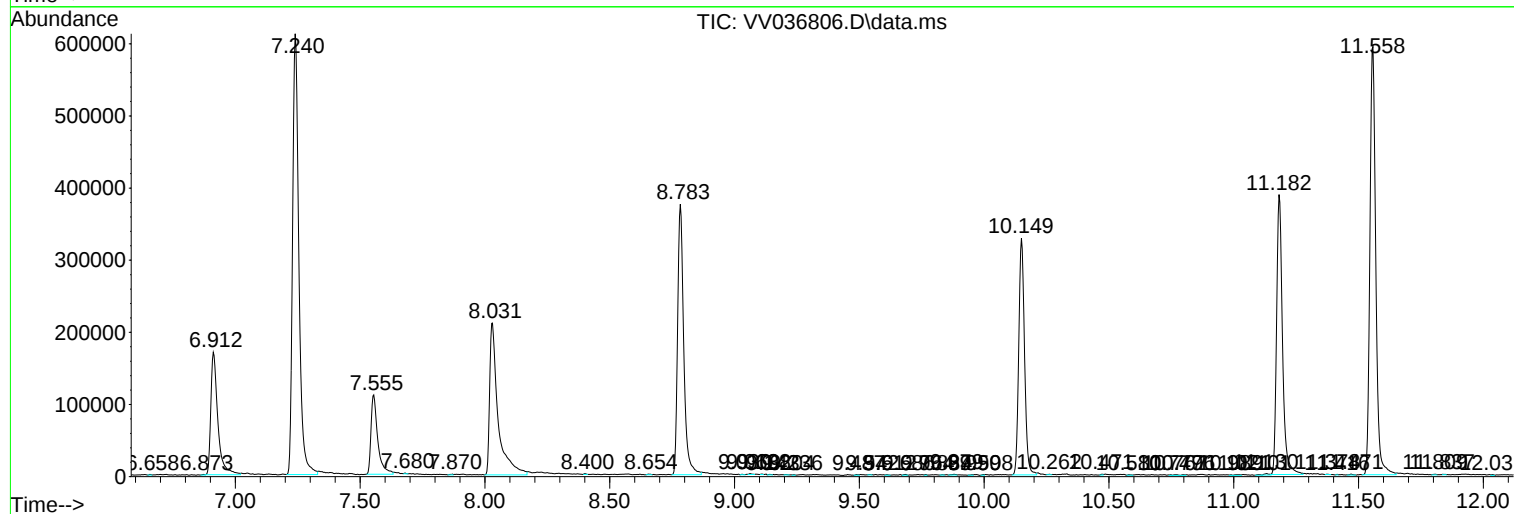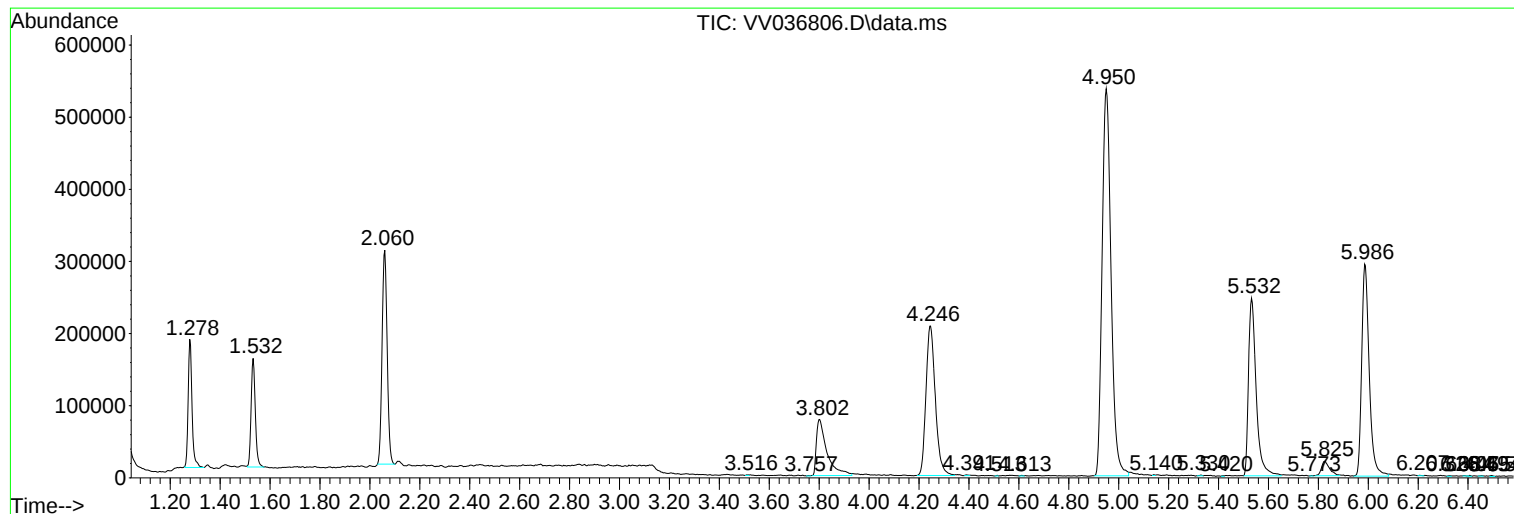

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036806.D
Acq On : 06 Aug 2024 12:05
Operator : SY/MD
Sample : P3437-05
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05W5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036806.D
Acq On : 06 Aug 2024 12:05
Operator : SY/MD
Sample : P3437-05
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E05W5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc