

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036809.D
 Acq On : 06 Aug 2024 13:51
 Operator : SY/MD
 Sample : P3398-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036809.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	93	rVB	224018	243300	13.49%	1.812%
2	1.532	146	153	171	rVB	187772	232081	12.87%	1.728%
3	2.057	307	316	330	rBV	394280	561952	31.16%	4.184%
4	3.413	734	738	740	rBV3	669	463	0.03%	0.003%
5	3.426	740	742	744	rBV3	928	431	0.02%	0.003%
6	3.571	784	787	791	rBV4	923	823	0.05%	0.006%
7	3.590	791	793	799	rVB4	864	676	0.04%	0.005%
8	3.616	799	801	804	rBV2	844	453	0.03%	0.003%
9	3.745	838	841	844	rVB4	723	489	0.03%	0.004%
10	3.793	847	856	884	rBV	108862	301852	16.74%	2.248%
11	4.240	978	995	1022	rBV	275770	713578	39.57%	5.313%
12	4.539	1085	1088	1092	rVB3	746	589	0.03%	0.004%
13	4.661	1123	1126	1129	rBV4	686	531	0.03%	0.004%
14	4.683	1130	1133	1135	rBV3	870	504	0.03%	0.004%
15	4.947	1197	1215	1255	rBV2	715059	1803164	100.00%	13.426%
16	5.253	1308	1310	1313	rBV3	1005	685	0.04%	0.005%
17	5.330	1329	1334	1335	rBV4	1392	1018	0.06%	0.008%
18	5.465	1369	1376	1378	rBV5	1571	1710	0.09%	0.013%
19	5.526	1384	1395	1423	rBV	534733	1093170	60.63%	8.140%
20	5.738	1459	1461	1464	rVB3	932	559	0.03%	0.004%
21	5.822	1476	1487	1507	rBV2	23259	53414	2.96%	0.398%
22	5.982	1524	1537	1564	rBV	400416	822993	45.64%	6.128%
23	6.207	1604	1607	1616	rVB8	1350	1546	0.09%	0.012%
24	6.249	1616	1620	1623	rBV4	892	659	0.04%	0.005%
25	6.371	1654	1658	1661	rBV5	801	719	0.04%	0.005%
26	6.433	1674	1677	1678	rBV2	671	463	0.03%	0.003%
27	6.558	1713	1716	1717	rBV3	909	606	0.03%	0.005%
28	6.699	1758	1760	1766	rVB5	697	626	0.03%	0.005%
29	6.908	1814	1825	1855	rBV	234546	451149	25.02%	3.359%
30	7.236	1912	1927	1961	rBV	813111	1431155	79.37%	10.656%
31	7.548	2015	2024	2059	rBV2	155018	289286	16.04%	2.154%
32	7.818	2105	2108	2110	rBV4	695	456	0.03%	0.003%
33	7.873	2117	2125	2133	rBV2	4607	7437	0.41%	0.055%
34	8.024	2163	2172	2219	rBV2	309749	666466	36.96%	4.962%
35	8.629	2354	2360	2366	rVB6	789	1128	0.06%	0.008%
36	8.680	2372	2376	2379	rBV5	830	582	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036809.D
 Acq On : 06 Aug 2024 13:51
 Operator : SY/MD
 Sample : P3398-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	8.699	2379	2382	2388	rVB7	583	442	0.02%	0.003%
38	8.780	2395	2407	2429	rBV	797827	1317921	73.09%	9.813%
39	9.050	2489	2491	2495	rBV4	770	696	0.04%	0.005%
40	9.146	2519	2521	2526	rVB5	860	555	0.03%	0.004%
41	9.188	2531	2534	2537	rBV4	900	779	0.04%	0.006%
42	9.275	2558	2561	2566	rBV4	753	782	0.04%	0.006%
43	9.346	2579	2583	2585	rBV2	645	462	0.03%	0.003%
44	9.609	2660	2665	2670	rVB6	755	877	0.05%	0.007%
45	9.638	2670	2674	2675	rBV4	719	525	0.03%	0.004%
46	9.706	2690	2695	2698	rVB4	984	831	0.05%	0.006%
47	9.802	2721	2725	2727	rBV3	828	548	0.03%	0.004%
48	9.825	2730	2732	2738	rVB5	839	693	0.04%	0.005%
49	9.857	2738	2742	2744	rBV3	680	552	0.03%	0.004%
50	9.992	2782	2784	2790	rVB5	919	772	0.04%	0.006%
51	10.024	2790	2794	2795	rBV3	722	576	0.03%	0.004%
52	10.079	2809	2811	2818	rVB4	577	540	0.03%	0.004%
53	10.146	2818	2832	2855	rBV	458814	738954	40.98%	5.502%
54	10.320	2879	2886	2887	rBV7	5311	4883	0.27%	0.036%
55	10.375	2901	2903	2905	rBV3	909	425	0.02%	0.003%
56	10.384	2905	2906	2911	rVB4	833	456	0.03%	0.003%
57	10.410	2911	2914	2915	rBV3	826	526	0.03%	0.004%
58	10.474	2928	2934	2937	rBV6	814	934	0.05%	0.007%
59	10.526	2947	2950	2954	rVB4	780	700	0.04%	0.005%
60	10.548	2954	2957	2962	rBV5	542	620	0.03%	0.005%
61	10.606	2971	2975	2980	rVB5	694	725	0.04%	0.005%
62	10.693	2999	3002	3004	rBV2	537	434	0.02%	0.003%
63	10.841	3045	3048	3051	rBV5	826	577	0.03%	0.004%
64	10.863	3052	3055	3058	rVV3	720	513	0.03%	0.004%
65	10.905	3063	3068	3070	rVV5	577	523	0.03%	0.004%
66	10.921	3071	3073	3077	rVB4	821	557	0.03%	0.004%
67	11.108	3126	3131	3134	rBV4	920	836	0.05%	0.006%
68	11.130	3134	3138	3141	rBV5	895	811	0.04%	0.006%
69	11.182	3142	3154	3181	rBV	837266	1317236	73.05%	9.808%
70	11.416	3225	3227	3232	rVB5	814	678	0.04%	0.005%
71	11.474	3243	3245	3249	rVB3	764	466	0.03%	0.003%
72	11.555	3257	3270	3307	rBV	827919	1318556	73.12%	9.818%
73	11.712	3316	3319	3322	rVB4	795	578	0.03%	0.004%
74	11.973	3396	3400	3402	rBV3	623	440	0.02%	0.003%
75	11.998	3406	3408	3412	rBV4	783	444	0.02%	0.003%
76	12.075	3429	3432	3434	rVB3	801	487	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036809.D
 Acq On : 06 Aug 2024 13:51
 Operator : SY/MD
 Sample : P3398-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	12.136	3449	3451	3454	rBV4	725	468	0.03%	0.003%
78	12.198	3465	3470	3477	rBV6	1248	1451	0.08%	0.011%
79	12.333	3508	3512	3513	rBV4	704	494	0.03%	0.004%
80	12.423	3535	3540	3543	rBV7	852	748	0.04%	0.006%
81	12.442	3543	3546	3551	rBV5	615	629	0.03%	0.005%
82	12.481	3556	3558	3563	rVB4	910	832	0.05%	0.006%
83	12.513	3563	3568	3572	rBV2	931	918	0.05%	0.007%
84	12.590	3587	3592	3595	rBV5	1026	1034	0.06%	0.008%
85	12.722	3631	3633	3640	rBV6	833	844	0.05%	0.006%
86	12.799	3654	3657	3661	rBV5	663	531	0.03%	0.004%
87	12.825	3661	3665	3666	rBV2	1605	1138	0.06%	0.008%
88	13.214	3779	3786	3792	rBV9	1674	2167	0.12%	0.016%
89	13.265	3799	3802	3804	rBV4	690	468	0.03%	0.003%
90	13.278	3804	3806	3809	rVV3	742	468	0.03%	0.003%
91	13.390	3837	3841	3844	rBV6	864	777	0.04%	0.006%
92	13.464	3854	3864	3869	rBV6	3024	5676	0.31%	0.042%
93	13.571	3894	3897	3899	rBV3	773	564	0.03%	0.004%
94	13.728	3944	3946	3950	rVB5	1024	653	0.04%	0.005%
95	13.889	3993	3996	3998	rBV2	728	424	0.02%	0.003%
96	14.255	4107	4110	4114	rBV2	934	798	0.04%	0.006%
97	14.416	4155	4160	4161	rBV3	779	658	0.04%	0.005%
98	14.445	4167	4169	4174	rVB5	697	469	0.03%	0.003%
99	14.625	4221	4225	4227	rBV5	979	846	0.05%	0.006%
100	14.779	4269	4273	4276	rBV5	1442	1419	0.08%	0.011%




Sum of corrected areas: 13430097

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036809.D
Acq On : 06 Aug 2024 13:51
Operator : SY/MD
Sample : P3398-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

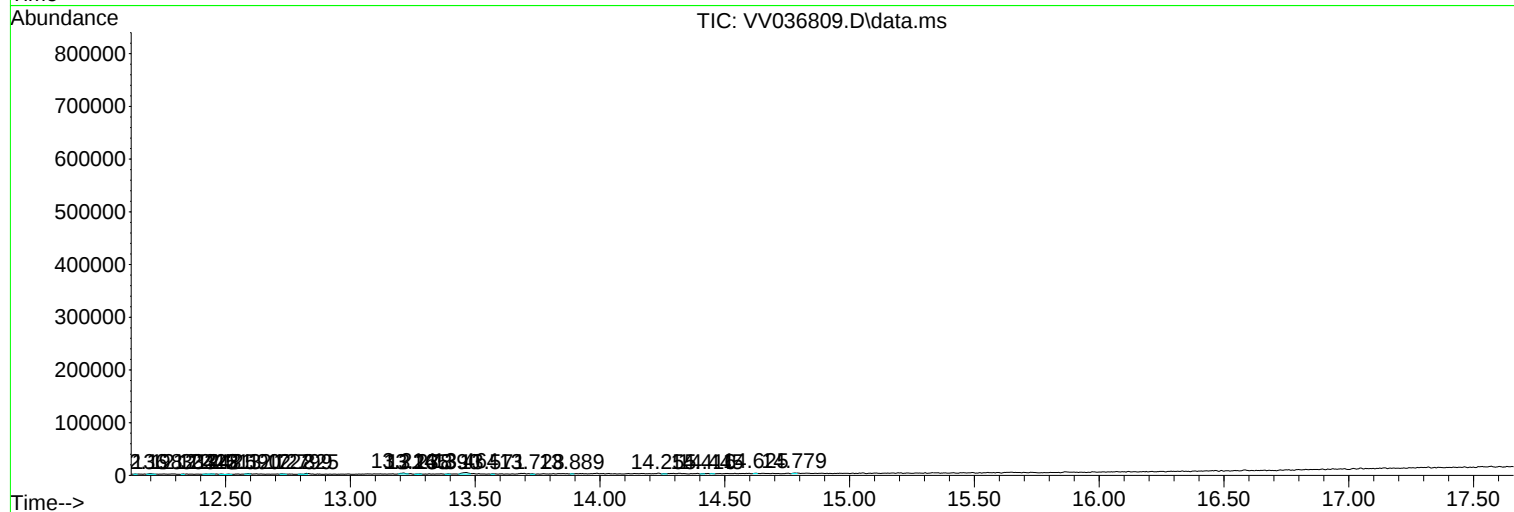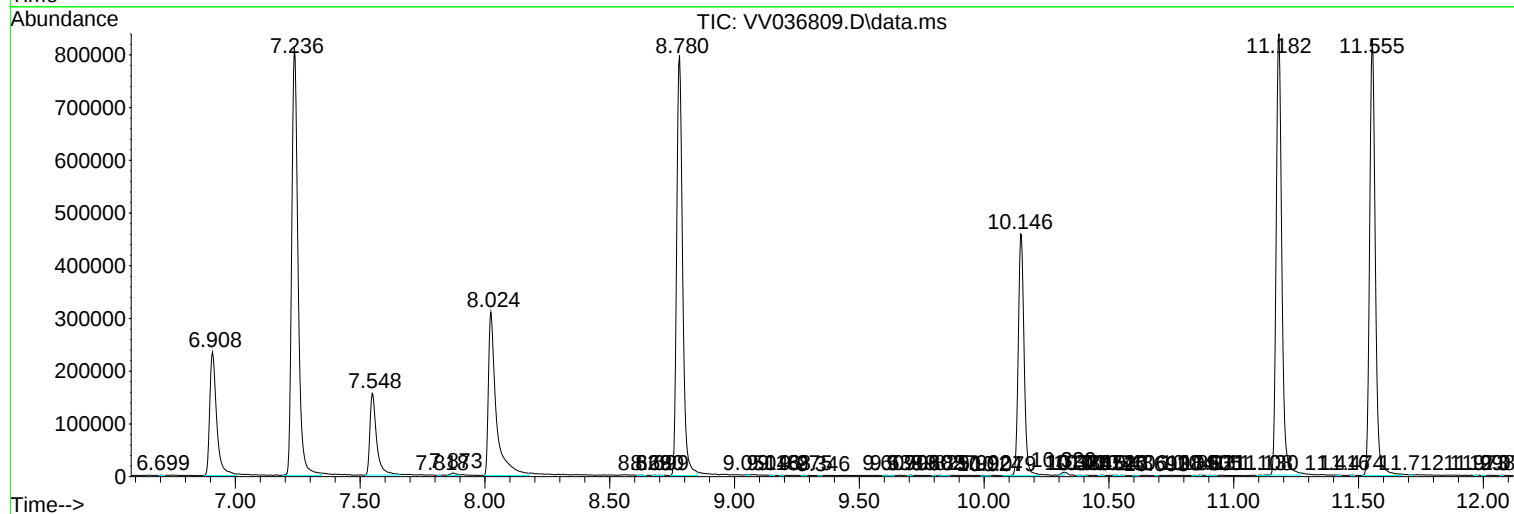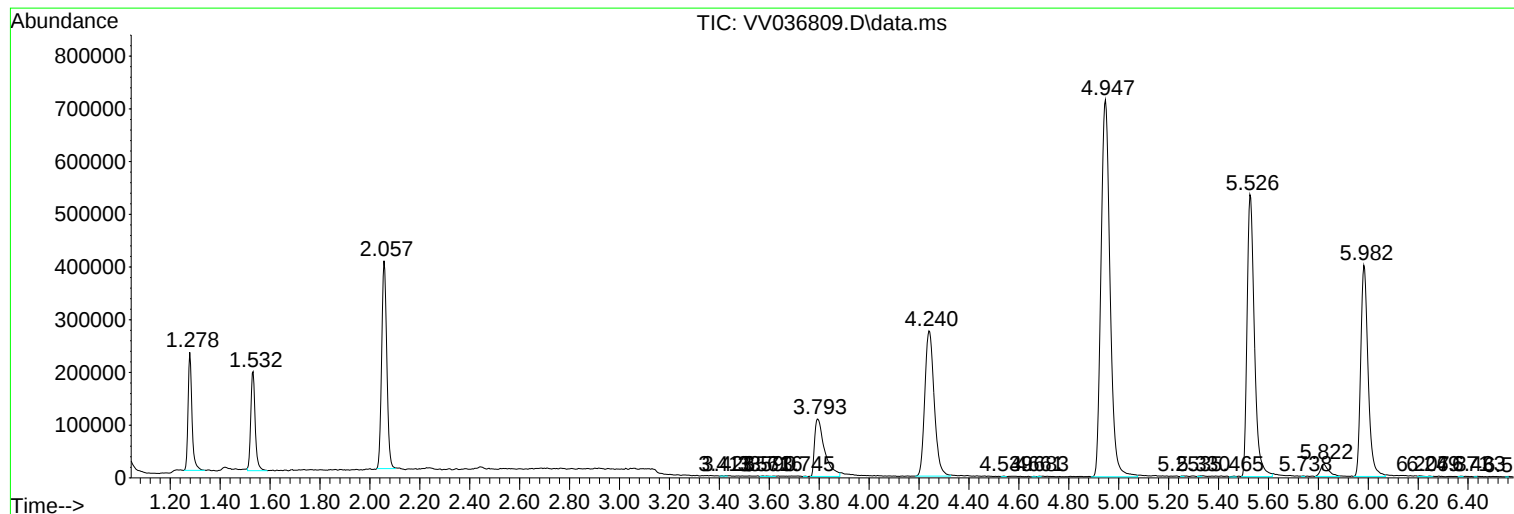

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036809.D
Acq On : 06 Aug 2024 13:51
Operator : SY/MD
Sample : P3398-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036809.D
Acq On : 06 Aug 2024 13:51
Operator : SY/MD
Sample : P3398-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
