

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036817.D
 Acq On : 06 Aug 2024 16:48
 Operator : SY/MD
 Sample : VIBLK325
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK325

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036817.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rVB	209139	219918	12.90%	1.693%
2	1.529	146	152	172	rVB	174882	211337	12.39%	1.627%
3	2.056	307	316	332	rVB	360700	514771	30.19%	3.964%
4	3.754	841	844	845	rBV3	1025	544	0.03%	0.004%
5	3.799	849	858	892	rBV	122708	377574	22.14%	2.908%
6	4.243	980	996	1025	rBV	265286	671162	39.36%	5.168%
7	4.494	1071	1074	1075	rBV2	907	542	0.03%	0.004%
8	4.690	1132	1135	1139	rVB6	735	517	0.03%	0.004%
9	4.719	1139	1144	1148	rBV5	1546	1794	0.11%	0.014%
10	4.799	1166	1169	1173	rVB3	643	554	0.03%	0.004%
11	4.950	1200	1216	1245	rBV2	679860	1705362	100.00%	13.132%
12	5.204	1293	1295	1298	rVB3	989	520	0.03%	0.004%
13	5.388	1349	1352	1356	rBV5	1129	803	0.05%	0.006%
14	5.404	1356	1357	1361	rBV4	609	455	0.03%	0.004%
15	5.529	1384	1396	1428	rBV	488661	1001367	58.72%	7.711%
16	5.761	1466	1468	1471	rVB4	898	491	0.03%	0.004%
17	5.780	1471	1474	1477	rBV3	776	681	0.04%	0.005%
18	5.825	1477	1488	1510	rVV5	26661	64626	3.79%	0.498%
19	5.986	1525	1538	1570	rBV	380562	796005	46.68%	6.130%
20	6.304	1633	1637	1642	rBB7	820	669	0.04%	0.005%
21	6.433	1673	1677	1680	rBV4	1241	1083	0.06%	0.008%
22	6.506	1698	1700	1704	rVB3	1141	587	0.03%	0.005%
23	6.529	1704	1707	1709	rBV2	755	447	0.03%	0.003%
24	6.577	1718	1722	1727	rVV4	930	753	0.04%	0.006%
25	6.622	1733	1736	1738	rVV3	610	444	0.03%	0.003%
26	6.651	1742	1745	1749	rVB3	752	614	0.04%	0.005%
27	6.680	1751	1754	1757	rBV2	908	552	0.03%	0.004%
28	6.793	1785	1789	1793	rBV5	889	755	0.04%	0.006%
29	6.912	1815	1826	1848	rBV	221671	421395	24.71%	3.245%
30	7.172	1903	1907	1910	rBV4	1234	1023	0.06%	0.008%
31	7.240	1917	1928	1952	rBV	745553	1319652	77.38%	10.162%
32	7.551	2016	2025	2053	rBV	147844	280207	16.43%	2.158%
33	7.834	2109	2113	2119	rVB4	720	739	0.04%	0.006%
34	7.870	2119	2124	2127	rBV5	852	834	0.05%	0.006%
35	7.908	2131	2136	2149	rVB9	3783	6029	0.35%	0.046%
36	8.027	2164	2173	2214	rBV2	350260	727991	42.69%	5.606%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036817.D
 Acq On : 06 Aug 2024 16:48
 Operator : SY/MD
 Sample : VIBLK325
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK325

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	8.632	2357	2361	2364	rBV5	516	446	0.03%	0.003%
38	8.709	2382	2385	2387	rBV3	942	507	0.03%	0.004%
39	8.780	2396	2407	2436	rBV	735914	1233249	72.32%	9.497%
40	8.953	2456	2461	2463	rBV6	2564	2502	0.15%	0.019%
41	9.149	2519	2522	2524	rBV3	730	499	0.03%	0.004%
42	9.172	2526	2529	2531	rVB4	758	491	0.03%	0.004%
43	9.227	2543	2546	2549	rBV4	1106	754	0.04%	0.006%
44	9.256	2553	2555	2559	rBV4	773	606	0.04%	0.005%
45	9.400	2597	2600	2602	rBV2	834	486	0.03%	0.004%
46	9.439	2609	2612	2616	rVB6	1044	944	0.06%	0.007%
47	9.487	2619	2627	2632	rBV4	4666	6593	0.39%	0.051%
48	9.622	2664	2669	2672	rBV5	680	778	0.05%	0.006%
49	9.809	2723	2727	2731	rVB5	843	566	0.03%	0.004%
50	9.866	2736	2745	2758	rBV6	3584	7705	0.45%	0.059%
51	9.915	2758	2760	2764	rVB4	1167	634	0.04%	0.005%
52	9.940	2764	2768	2770	rBV3	697	552	0.03%	0.004%
53	10.021	2789	2793	2796	rBV4	915	598	0.04%	0.005%
54	10.098	2813	2817	2819	rBV3	645	578	0.03%	0.004%
55	10.149	2822	2833	2860	rBV	482408	754875	44.26%	5.813%
56	10.320	2881	2886	2890	rVB5	1318	1209	0.07%	0.009%
57	10.436	2918	2922	2926	rBV4	785	785	0.05%	0.006%
58	10.481	2928	2936	2944	rBV5	4548	7799	0.46%	0.060%
59	10.625	2977	2981	2983	rVV2	748	501	0.03%	0.004%
60	10.706	3002	3006	3010	rBV5	973	934	0.05%	0.007%
61	10.786	3028	3031	3034	rBV4	970	628	0.04%	0.005%
62	10.860	3048	3054	3065	rVV5	4760	6261	0.37%	0.048%
63	11.021	3099	3104	3108	rBV3	755	640	0.04%	0.005%
64	11.130	3129	3138	3143	rBV8	4864	7999	0.47%	0.062%
65	11.182	3143	3154	3188	rVV	770986	1242958	72.89%	9.572%
66	11.554	3259	3270	3292	rVV	784251	1257626	73.75%	9.684%
67	11.960	3390	3396	3400	rVV7	1922	2075	0.12%	0.016%
68	11.998	3406	3408	3410	rBV2	928	481	0.03%	0.004%
69	12.066	3423	3429	3432	rBV7	1004	1036	0.06%	0.008%
70	12.130	3447	3449	3455	rVB5	854	633	0.04%	0.005%
71	12.178	3461	3464	3467	rVV3	906	584	0.03%	0.004%
72	12.201	3468	3471	3477	rVB4	1106	779	0.05%	0.006%
73	12.233	3477	3481	3483	rBV4	530	461	0.03%	0.004%
74	12.300	3499	3502	3503	rBV2	812	457	0.03%	0.004%
75	12.455	3548	3550	3553	rVB4	1138	628	0.04%	0.005%
76	12.490	3553	3561	3567	rBV8	2763	4095	0.24%	0.032%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
 Data File : VV036817.D
 Acq On : 06 Aug 2024 16:48
 Operator : SY/MD
 Sample : VIBLK325
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK325

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	12.667	3610	3616	3625	rBV7	3644	5394	0.32%	0.042%
78	12.718	3630	3632	3634	rBV	732	444	0.03%	0.003%
79	12.738	3634	3638	3639	rBV4	1533	1166	0.07%	0.009%
80	12.796	3648	3656	3658	rBV7	1676	2256	0.13%	0.017%
81	12.828	3660	3666	3673	rVV7	3558	5910	0.35%	0.046%
82	12.940	3694	3701	3707	rBV7	2743	3752	0.22%	0.029%
83	13.017	3721	3725	3726	rBV4	768	611	0.04%	0.005%
84	13.085	3743	3746	3750	rBV5	923	953	0.06%	0.007%
85	13.149	3762	3766	3770	rBV4	1050	999	0.06%	0.008%
86	13.210	3776	3785	3794	rBV8	6397	11130	0.65%	0.086%
87	13.339	3818	3825	3830	rBV6	1909	2208	0.13%	0.017%
88	13.448	3850	3859	3874	rBV2	12059	24225	1.42%	0.187%
89	13.641	3915	3919	3922	rBV5	682	610	0.04%	0.005%
90	13.683	3926	3932	3942	rVB9	5506	8972	0.53%	0.069%
91	13.837	3974	3980	3987	rBV7	4477	6362	0.37%	0.049%
92	13.963	4014	4019	4025	rBV7	1625	1715	0.10%	0.013%
93	14.008	4031	4033	4037	rBV4	922	779	0.05%	0.006%
94	14.133	4069	4072	4077	rBV6	900	773	0.05%	0.006%
95	14.214	4093	4097	4103	rBV5	1145	1196	0.07%	0.009%
96	14.246	4103	4107	4110	rBV5	998	904	0.05%	0.007%
97	14.590	4209	4214	4220	rBV8	2039	3130	0.18%	0.024%
98	14.786	4268	4275	4282	rBV5	6509	8864	0.52%	0.068%
99	15.043	4352	4355	4356	rBV3	1139	701	0.04%	0.005%
100	15.673	4545	4551	4559	rBV7	5808	8245	0.48%	0.063%




Sum of corrected areas: 12986028

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036817.D
Acq On : 06 Aug 2024 16:48
Operator : SY/MD
Sample : VIBLK325
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK325

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

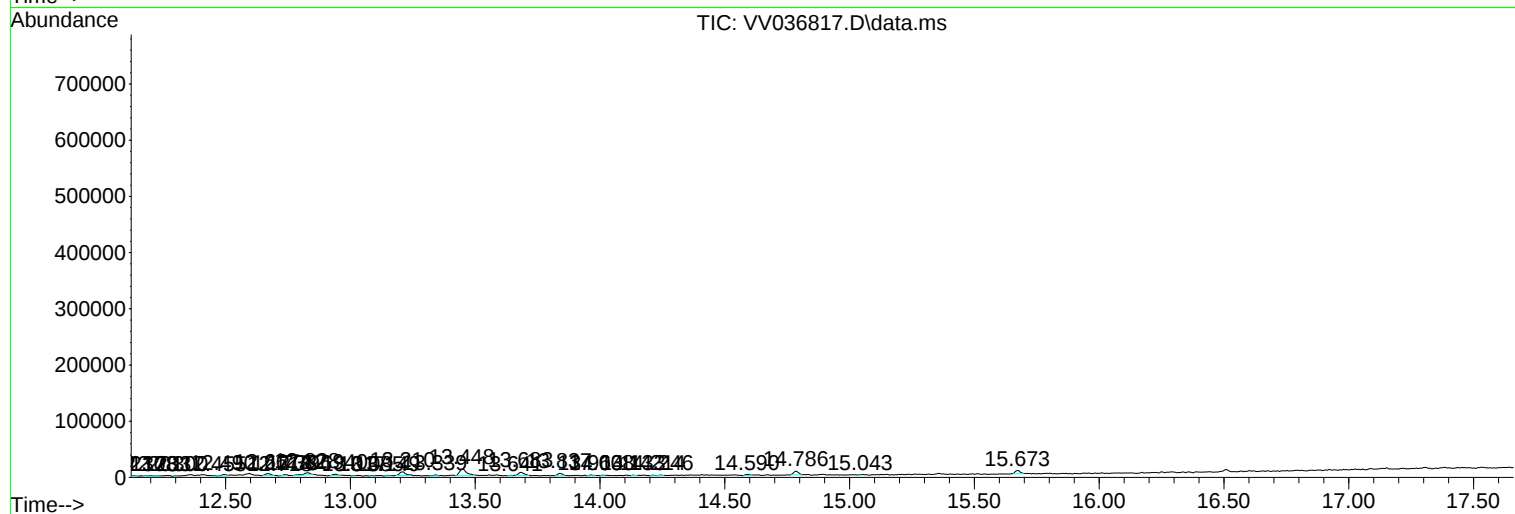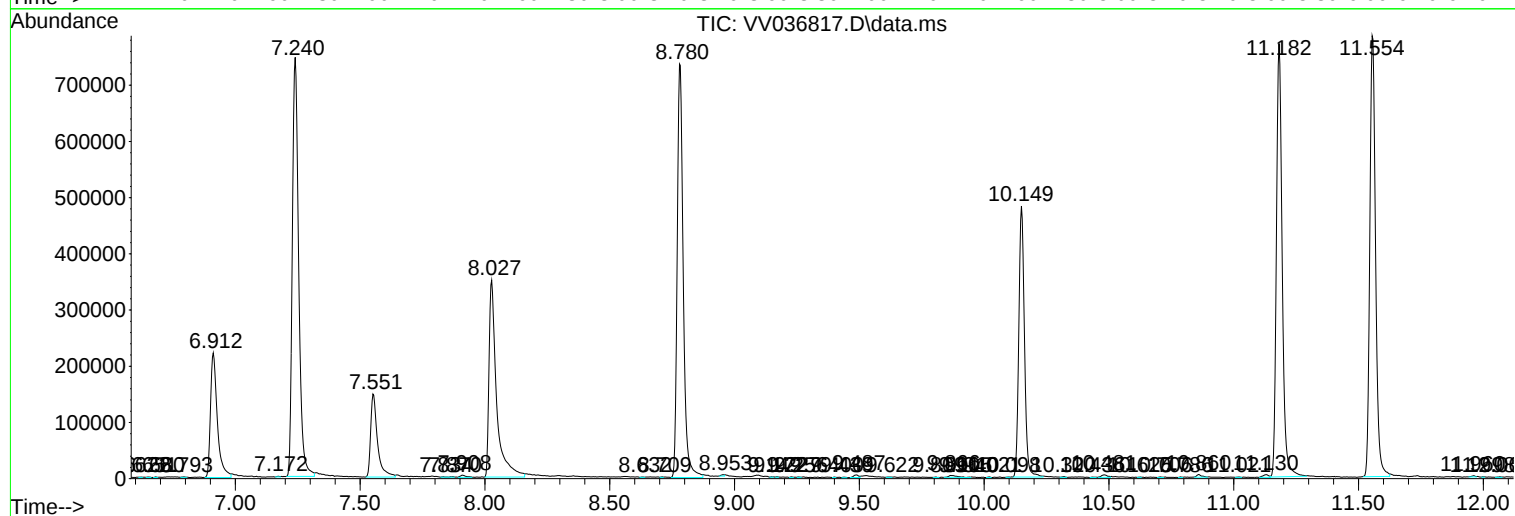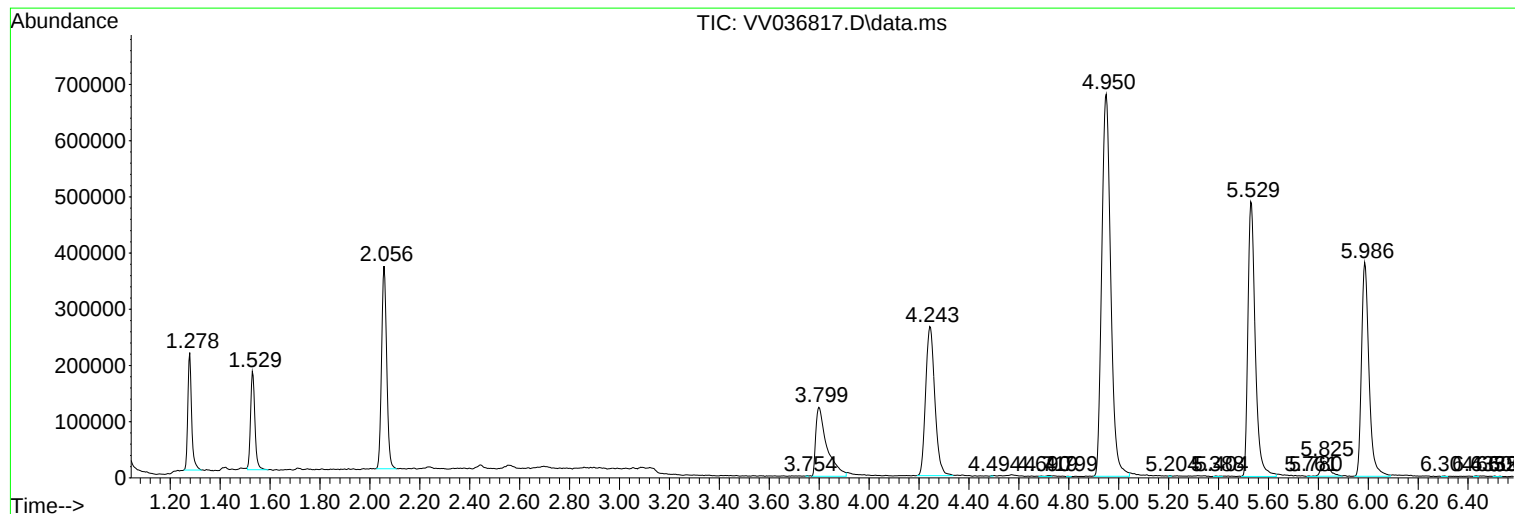

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036817.D
Acq On : 06 Aug 2024 16:48
Operator : SY/MD
Sample : VIBLK325
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK325

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036817.D
Acq On : 06 Aug 2024 16:48
Operator : SY/MD
Sample : VIBLK325
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK325

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------