
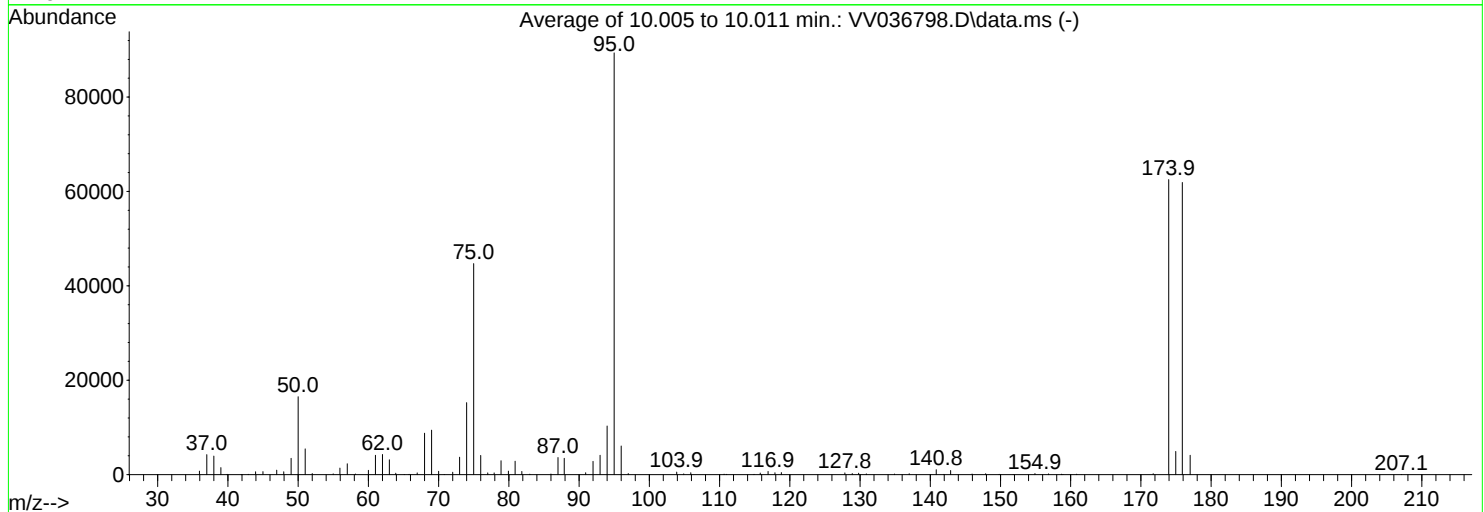


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080624\
Data File : VV036798.D
Acq On : 06 Aug 2024 08:08
Operator : SY/MD
Sample : BFB355
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB355

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Title : VOC Analysis
Last Update : Fri Aug 09 02:41:02 2024

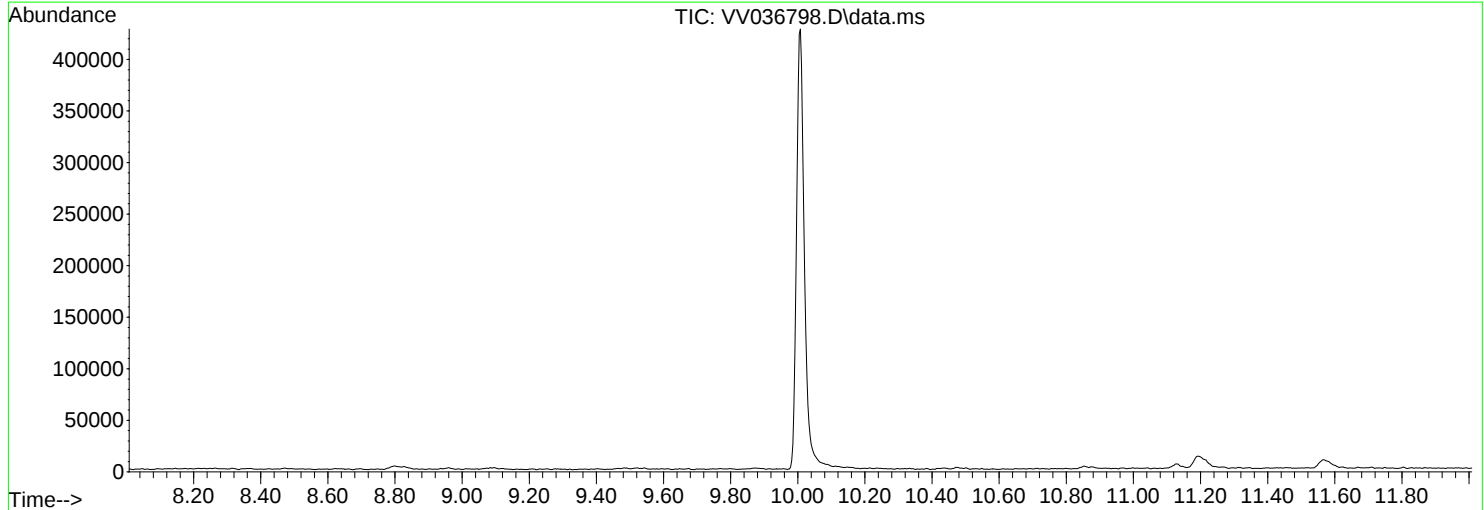

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	16509	PASS
75	95	30	80	50.1	44736	PASS
95	95	100	100	100.0	89379	PASS
96	95	5	9	6.8	6079	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.9	62520	PASS
175	174	5	9	7.9	4918	PASS
176	174	95	105	99.0	61917	PASS
177	176	5	10	6.7	4123	PASS

m/z	Abundance
39.00	144.0
39.90	252.0
41.00	223.0
42.00	205.0
42.90	174.0
43.90	933.0
45.00	120.0
55.10	152.0
77.00	183.0

Instrument :
MSVOA_V
ClientSampleId :
BFB355

m/z	Abundance
36.00	841.0
37.00	4509.0
38.00	4183.0
39.00	1699.0
39.90	372.0
40.80	138.0
41.90	214.0
42.90	293.0
44.00	1586.0
45.00	862.0
46.90	981.0
47.90	694.0
49.00	3596.0
50.00	16784.0
51.00	5772.0
52.00	289.0
55.00	401.0
56.00	1590.0
57.00	2333.0
58.10	157.0
60.00	1054.0
61.00	4033.0
62.00	4533.0
63.00	3185.0
63.90	308.0
65.10	118.0
67.00	384.0
68.00	9044.0
69.00	9743.0
70.00	765.0
70.80	110.0
72.00	522.0
73.00	3814.0
74.00	15768.0
75.00	46464.0
76.00	4387.0
77.10	606.0
77.90	435.0
78.90	2997.0
80.00	743.0
80.90	2943.0
81.90	742.0
83.00	197.0
86.00	124.0
87.00	3773.0
87.90	3600.0
90.90	384.0
92.00	2894.0
93.00	4057.0
94.00	10268.0
95.00	91416.0
96.00	6505.0
97.00	253.0
103.90	588.0
104.90	161.0
105.90	425.0
110.60	141.0
111.10	104.0
114.90	119.0
115.80	290.0
116.90	624.0
117.90	433.0
118.80	449.0
127.90	443.0
128.90	220.0
129.80	277.0
130.80	147.0
134.90	201.0
137.00	156.0
140.90	1058.0
142.00	107.0
142.90	886.0
145.90	165.0
147.90	184.0
149.80	112.0
155.00	198.0
156.80	150.0
158.70	130.0
160.90	103.0
171.70	218.0
174.00	62680.0
174.90	5064.0
175.90	61128.0
177.00	4167.0
207.10	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB355

m/z	Abundance
36.00	760.0
37.00	4358.0
38.00	4043.0
39.00	1696.0
39.90	340.0
40.80	169.0
41.90	244.0
42.90	254.0
44.00	1564.0
45.00	743.0
46.90	971.0
47.90	610.0
49.00	3587.0
50.00	17176.0
51.00	5612.0
52.00	252.0
55.00	325.0
56.00	1404.0
57.00	2378.0
58.20	133.0
60.00	963.0
61.00	4235.0
62.00	4428.0
63.00	3198.0
63.90	336.0
65.80	116.0
66.90	379.0
68.00	9002.0
69.00	9714.0
70.00	731.0
72.00	512.0
73.00	3713.0
74.00	15734.0
75.00	46016.0
76.00	4180.0
77.10	543.0
77.90	379.0
78.90	3038.0
79.90	786.0
80.90	2910.0
81.90	712.0
83.00	122.0
86.00	151.0
87.00	3756.0
87.90	3507.0
91.00	418.0
92.00	2960.0
93.00	4250.0
94.00	10644.0
95.00	92520.0
96.00	6306.0
97.00	226.0
103.90	589.0
104.90	195.0
105.90	418.0
110.70	127.0
114.90	104.0
115.80	345.0
116.90	685.0
117.90	427.0
118.80	459.0
127.80	387.0
128.90	253.0
129.80	335.0
130.90	184.0
134.90	157.0
137.00	198.0
140.80	1084.0
141.90	109.0
142.90	893.0
145.90	147.0
147.90	198.0
149.80	113.0
154.80	174.0
155.10	181.0
156.90	166.0
158.70	136.0
160.80	118.0
171.80	205.0
173.90	64600.0
175.00	5093.0
175.90	63976.0
177.00	4346.0

Instrument :
MSVOA_V
ClientSampleId :
BFB355

m/z	Abundance
35.90	687.0
37.00	3806.0
38.00	3571.0
39.00	1479.0
39.90	273.0
40.80	185.0
41.90	203.0
43.00	198.0
44.00	1490.0
45.00	673.0
47.00	913.0
48.00	525.0
49.00	3242.0
50.00	15567.0
51.00	4973.0
52.00	215.0
55.00	248.0
55.90	1164.0
57.00	2244.0
58.20	109.0
60.00	780.0
61.00	4014.0
62.00	3908.0
63.00	3078.0
63.90	297.0
65.80	119.0
66.90	336.0
68.00	8261.0
69.00	8785.0
70.00	651.0
72.00	482.0
73.00	3540.0
74.00	14276.0
75.00	41728.0
76.00	3684.0
77.00	490.0
77.90	344.0
78.90	2797.0
79.90	761.0
80.90	2680.0
81.80	601.0
86.00	164.0
87.00	3361.0
87.90	3257.0
91.00	386.0
92.00	2636.0
93.00	3972.0
94.00	10027.0
95.00	84200.0
96.00	5426.0
97.00	212.0
103.90	490.0
104.90	203.0
105.90	394.0
110.90	130.0
115.80	369.0
116.90	695.0
117.90	373.0
118.80	459.0
127.90	316.0
128.90	217.0
129.80	352.0
131.00	199.0
134.90	107.0
137.00	227.0
140.80	980.0
142.90	866.0
146.00	124.0
147.90	187.0
151.80	119.0
154.80	184.0
156.90	160.0
158.90	122.0
160.80	116.0
171.80	202.0
173.90	60280.0
175.00	4598.0
175.90	60648.0
177.00	3855.0

Instrument :
MSVOA_V
ClientSampleId :
BFB355