

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036827.D
 Acq On : 07 Aug 2024 09:56
 Operator : SY/MD
 Sample : VV0807WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 08 02:36:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 08 02:35:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	484706	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	447094	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	217886	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	135907	35.105	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	70.220%
7) Chloroethane-d5	1.532	69	121751	39.879	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	79.760%
11) 1,1-Dichloroethene-d2	2.060	65	61112	36.903	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.800%
21) 2-Butanone-d5	3.796	46	186105	90.730	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	90.730%
24) Chloroform-d	4.243	84	294983	42.460	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.920%
26) 1,2-Dichloroethane-d4	4.937	65	198937	44.536	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.080%
32) Benzene-d6	4.953	84	595267	44.081	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.160%
36) 1,2-Dichloropropane-d6	5.986	67	198515	45.567	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.140%
41) Toluene-d8	7.240	98	519885	41.969	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.940%
43) trans-1,3-Dichloroprop...	7.551	79	91506	40.360	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.720%
47) 2-Hexanone-d5	8.024	63	106941	85.373	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.370%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	234606	46.900	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.800%
66) 1,2-Dichlorobenzene-d4	11.554	152	203076	45.738	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.480%
Target Compounds						
37) 1,2-Dichloropropane	5.986	63	21220	5.990	ug/L	Qvalue # 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036827.D
Acq On : 07 Aug 2024 09:56
Operator : SY/MD
Sample : VV0807WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Aug 08 02:36:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 08 02:35:03 2024
Response via : Initial Calibration

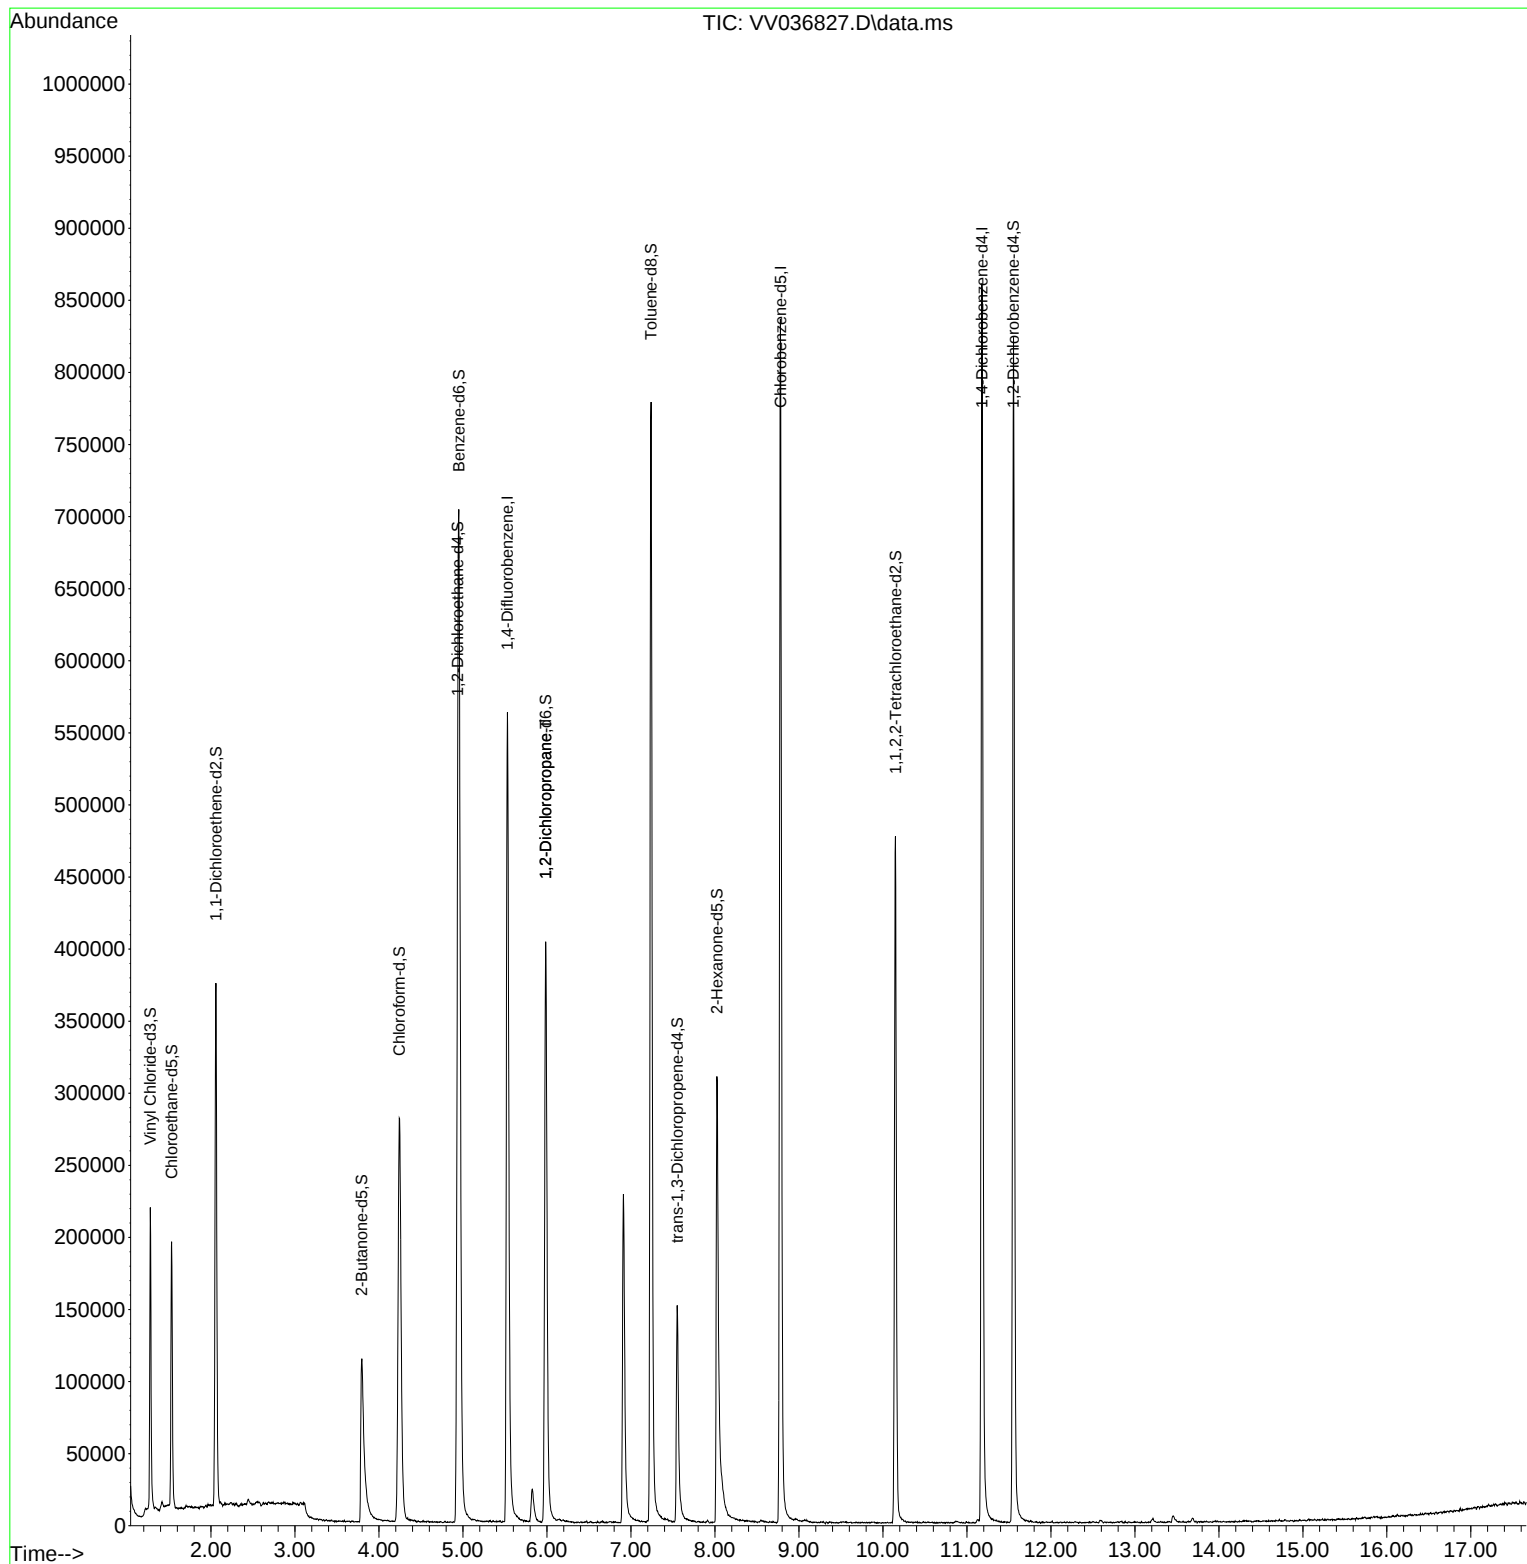

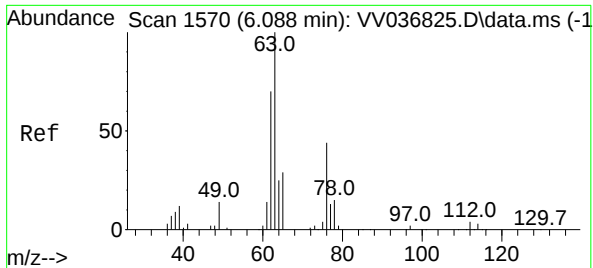

#37
 1,2-Dichloropropane
 Concen: 5.990 ug/L
 RT: 5.986 min Scan# 11
 Delta R.T. -0.103 min
 Lab File: VV036827.D
 Acq: 07 Aug 2024 09:56

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 63 Resp: 21220
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.6 5.4#

