

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036835.D
 Acq On : 07 Aug 2024 13:15
 Operator : SY/MD
 Sample : P3498-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 08 02:37:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 08 02:35:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	495336	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	454578	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	211633	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	147310	37.234	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	74.460%		
7) Chloroethane-d5	1.532	69	125131	40.107	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	80.220%		
11) 1,1-Dichloroethene-d2	2.059	65	63369	37.445	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.900%		
21) 2-Butanone-d5	3.796	46	160285	76.465	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	76.470%		
24) Chloroform-d	4.246	84	290823	40.962	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.920%		
26) 1,2-Dichloroethane-d4	4.937	65	195354	42.796	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.600%		
32) Benzene-d6	4.953	84	585877	42.672	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.340%		
36) 1,2-Dichloropropane-d6	5.985	67	195219	44.073	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	88.140%		
41) Toluene-d8	7.239	98	506619	40.225	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	80.460%		
43) trans-1,3-Dichloroprop...	7.551	79	87036	37.756	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	75.520%		
47) 2-Hexanone-d5	8.024	63	95873	75.277	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	75.280%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	215699	42.411	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	84.820%		
66) 1,2-Dichlorobenzene-d4	11.554	152	188731	43.764	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.520%		
Target Compounds						Qvalue
13) Acetone	2.114	43	6246	3.561	ug/L	94
39) cis-1,3-Dichloropropene	6.911	75	5506	0.893	ug/L #	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036835.D
Acq On : 07 Aug 2024 13:15
Operator : SY/MD
Sample : P3498-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Aug 08 02:37:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 08 02:35:03 2024
Response via : Initial Calibration

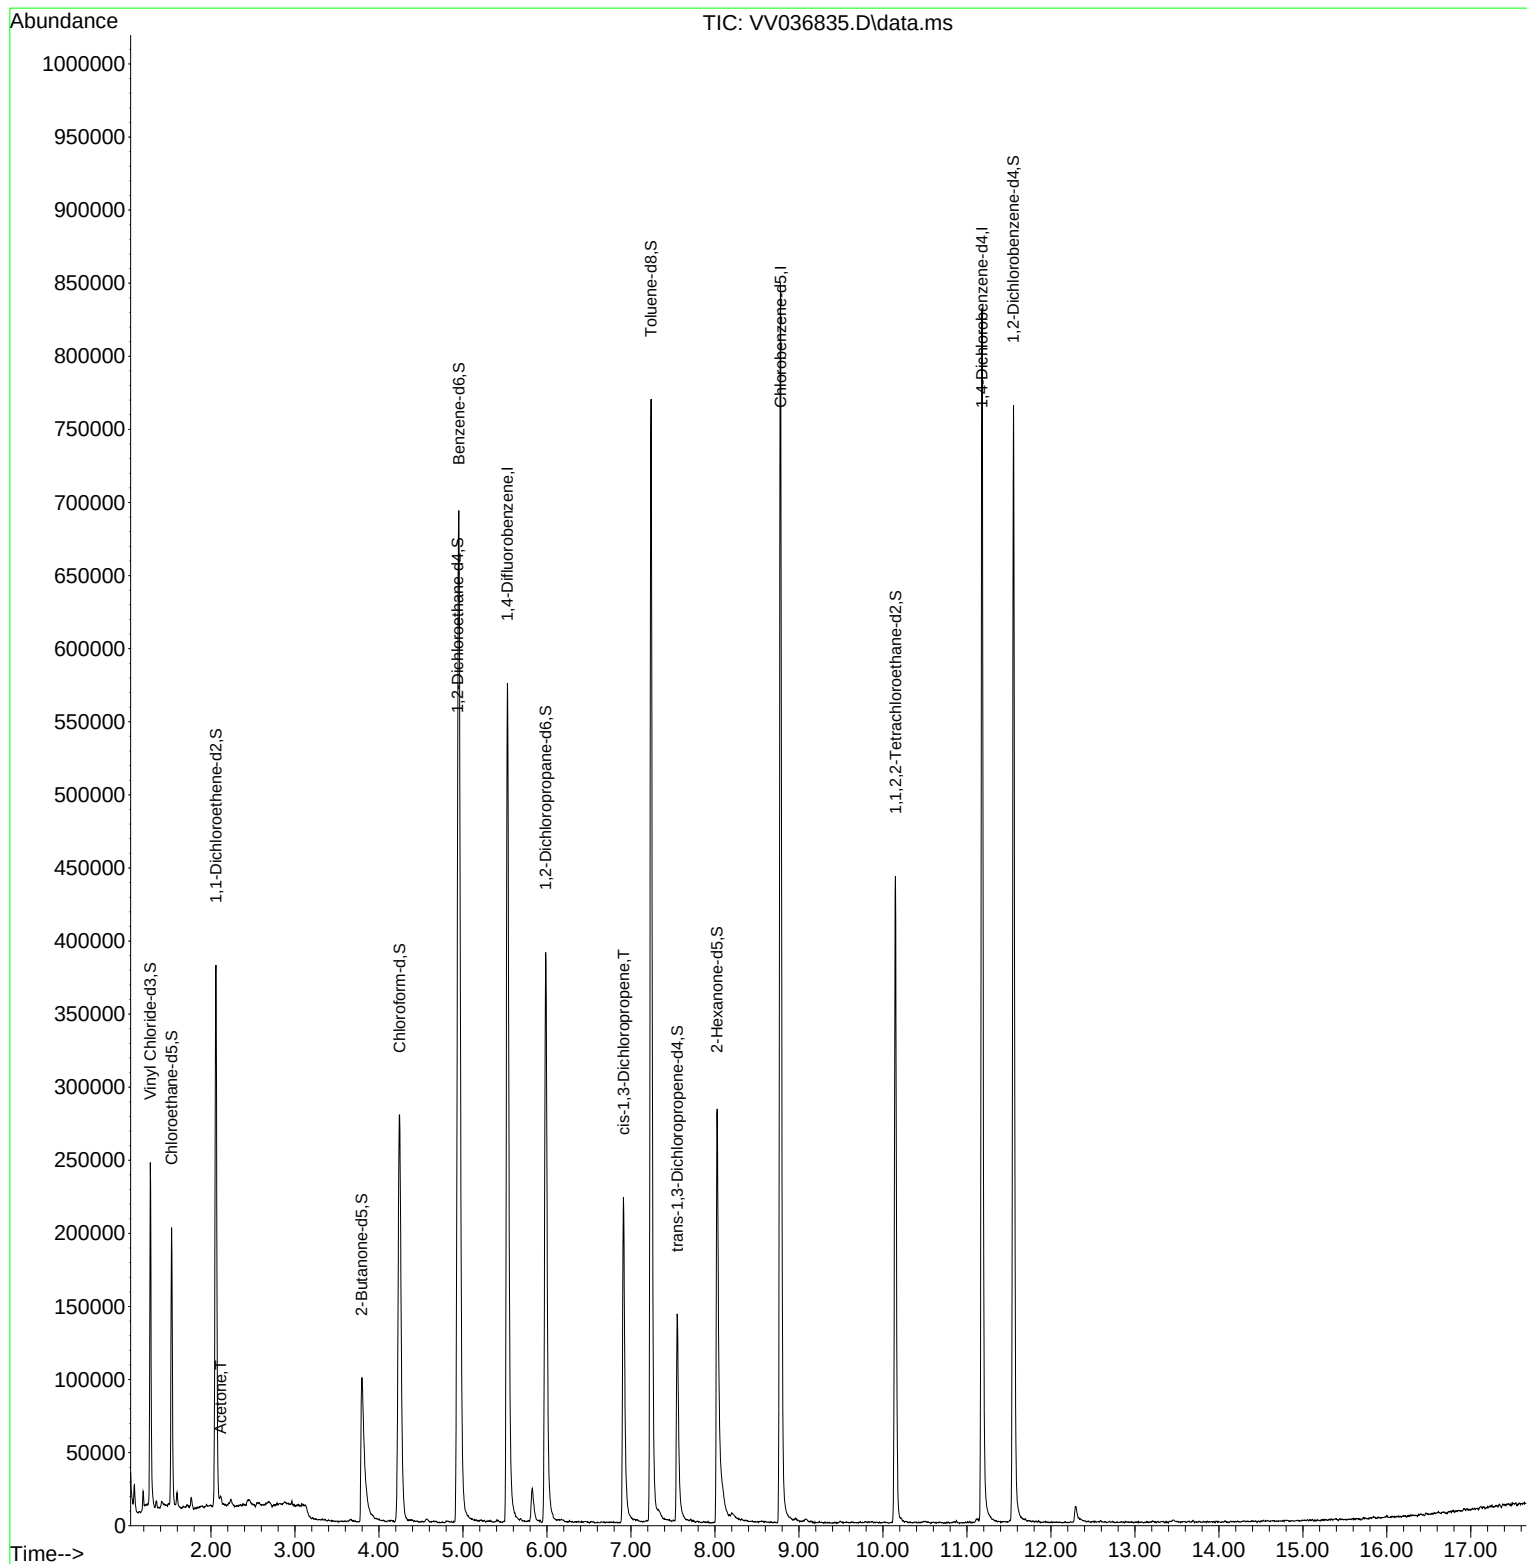

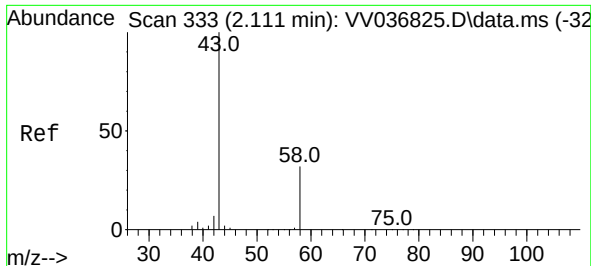

#13

Acetone

Concen: 3.561 ug/L

RT: 2.114 min Scan# 333

Delta R.T. 0.003 min

Lab File: VV036835.D

Acq: 07 Aug 2024 13:15

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 43 Resp: 6246

Ion Ratio Lower Upper

43 100

58 28.2 0.0 63.4

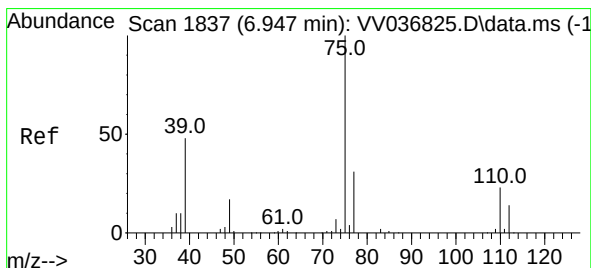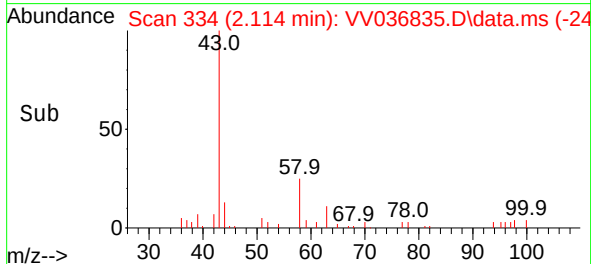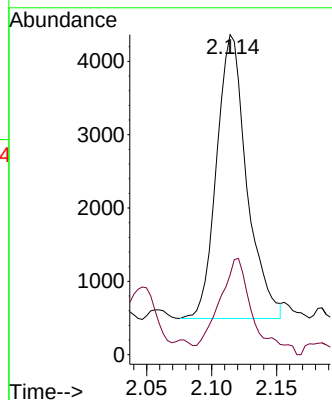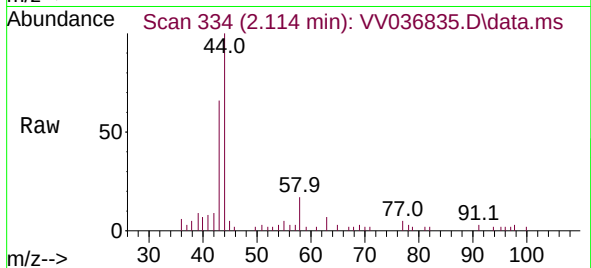

#39

cis-1,3-Dichloropropene

Concen: 0.893 ug/L

RT: 6.911 min Scan# 1826

Delta R.T. -0.036 min

Lab File: VV036835.D

Acq: 07 Aug 2024 13:15

Tgt Ion: 75 Resp: 5506

Ion Ratio Lower Upper

75 100

77 55.8 22.2 41.2#

