

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036830.D
 Acq On : 07 Aug 2024 11:26
 Operator : SY/MD
 Sample : P3480-05
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AD3

Quant Time: Aug 08 02:36:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 08 02:35:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	496369	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	465457	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	226962	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	157717	39.782	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	79.560%	
7) Chloroethane-d5	1.532	69	129865	41.537	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	83.080%	
11) 1,1-Dichloroethene-d2	2.060	65	68928	40.645	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	81.300%	
21) 2-Butanone-d5	3.796	46	173274	82.490	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	82.490%	
24) Chloroform-d	4.246	84	305794	42.981	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	85.960%	
26) 1,2-Dichloroethane-d4	4.937	65	205942	45.021	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	90.040%	
32) Benzene-d6	4.953	84	625548	44.496	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	89.000%	
36) 1,2-Dichloropropane-d6	5.985	67	207306	45.707	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	91.420%	
41) Toluene-d8	7.239	98	548092	42.501	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	85.000%	
43) trans-1,3-Dichloroprop...	7.551	79	96234	40.770	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	81.540%	
47) 2-Hexanone-d5	8.024	63	96677	74.134	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	74.130%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	206740	39.699	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	79.400%	
66) 1,2-Dichlorobenzene-d4	11.554	152	214952	46.477	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	92.960%	
Target Compounds					Qvalue	
13) Acetone	2.114	43	32420	18.447	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036830.D
Acq On : 07 Aug 2024 11:26
Operator : SY/MD
Sample : P3480-05
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AD3

Quant Time: Aug 08 02:36:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 08 02:35:03 2024
Response via : Initial Calibration

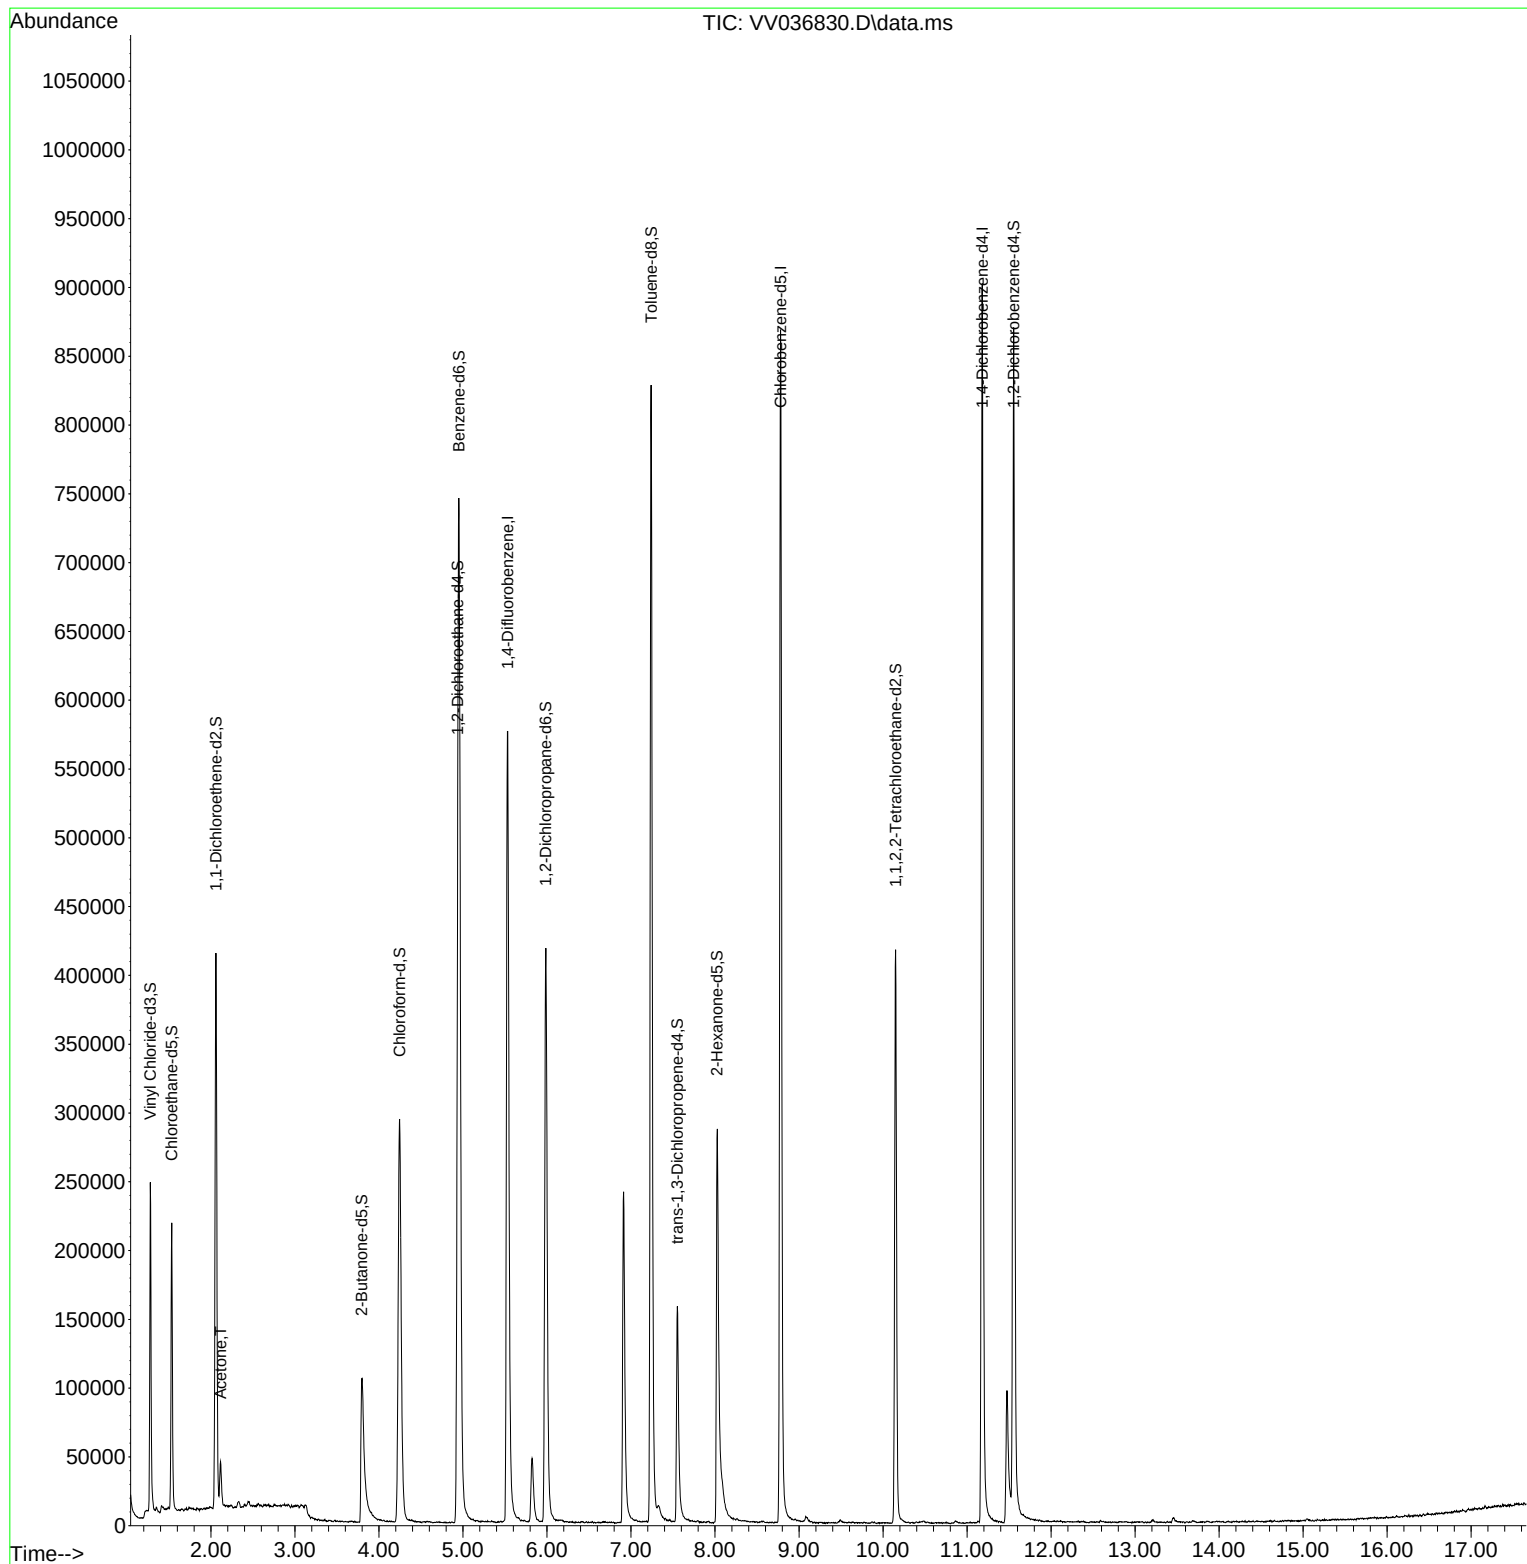

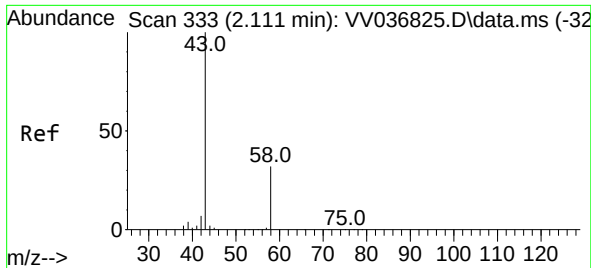

#13

Acetone

Concen: 18.447 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV036830.D

Acq: 07 Aug 2024 11:26

Instrument :

MSVOA_V

ClientSampleId :

E0AD3

Tgt Ion: 43 Resp: 32420

Ion Ratio Lower Upper

43 100

58 30.8 0.0 63.4

